

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040622AL\
 Data File : FC059090.D
 Signal(s) : FID1A.CH
 Acq On : 06 Apr 2022 20:44
 Operator : UA/NP
 Sample : N2276-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 07 01:59:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.103	5939249	41.221 ug/ml
Spiked Amount 50.000		Recovery =	82.44%
12) S 1-chlorooctadecane (S...	12.550	4414068	39.378 ug/ml
Spiked Amount 50.000		Recovery =	78.76%
Target Compounds			
10) T n-Eicosane (C20)	12.155	199369	1.522 ug/ml
18) T n-Dotriacontane (C32)	18.080	214791	2.005 ug/ml
19) T n-Tetratriacontane (C34)	18.871	164534	1.628 ug/ml
21) T n-Octatriacontane (C38)	20.301	1751963	19.039 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040622AL\
Data File : FC059090.D
Signal(s) : FID1A.CH
Acq On : 06 Apr 2022 20:44
Operator : UA/NP
Sample : N2276-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 01:59:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

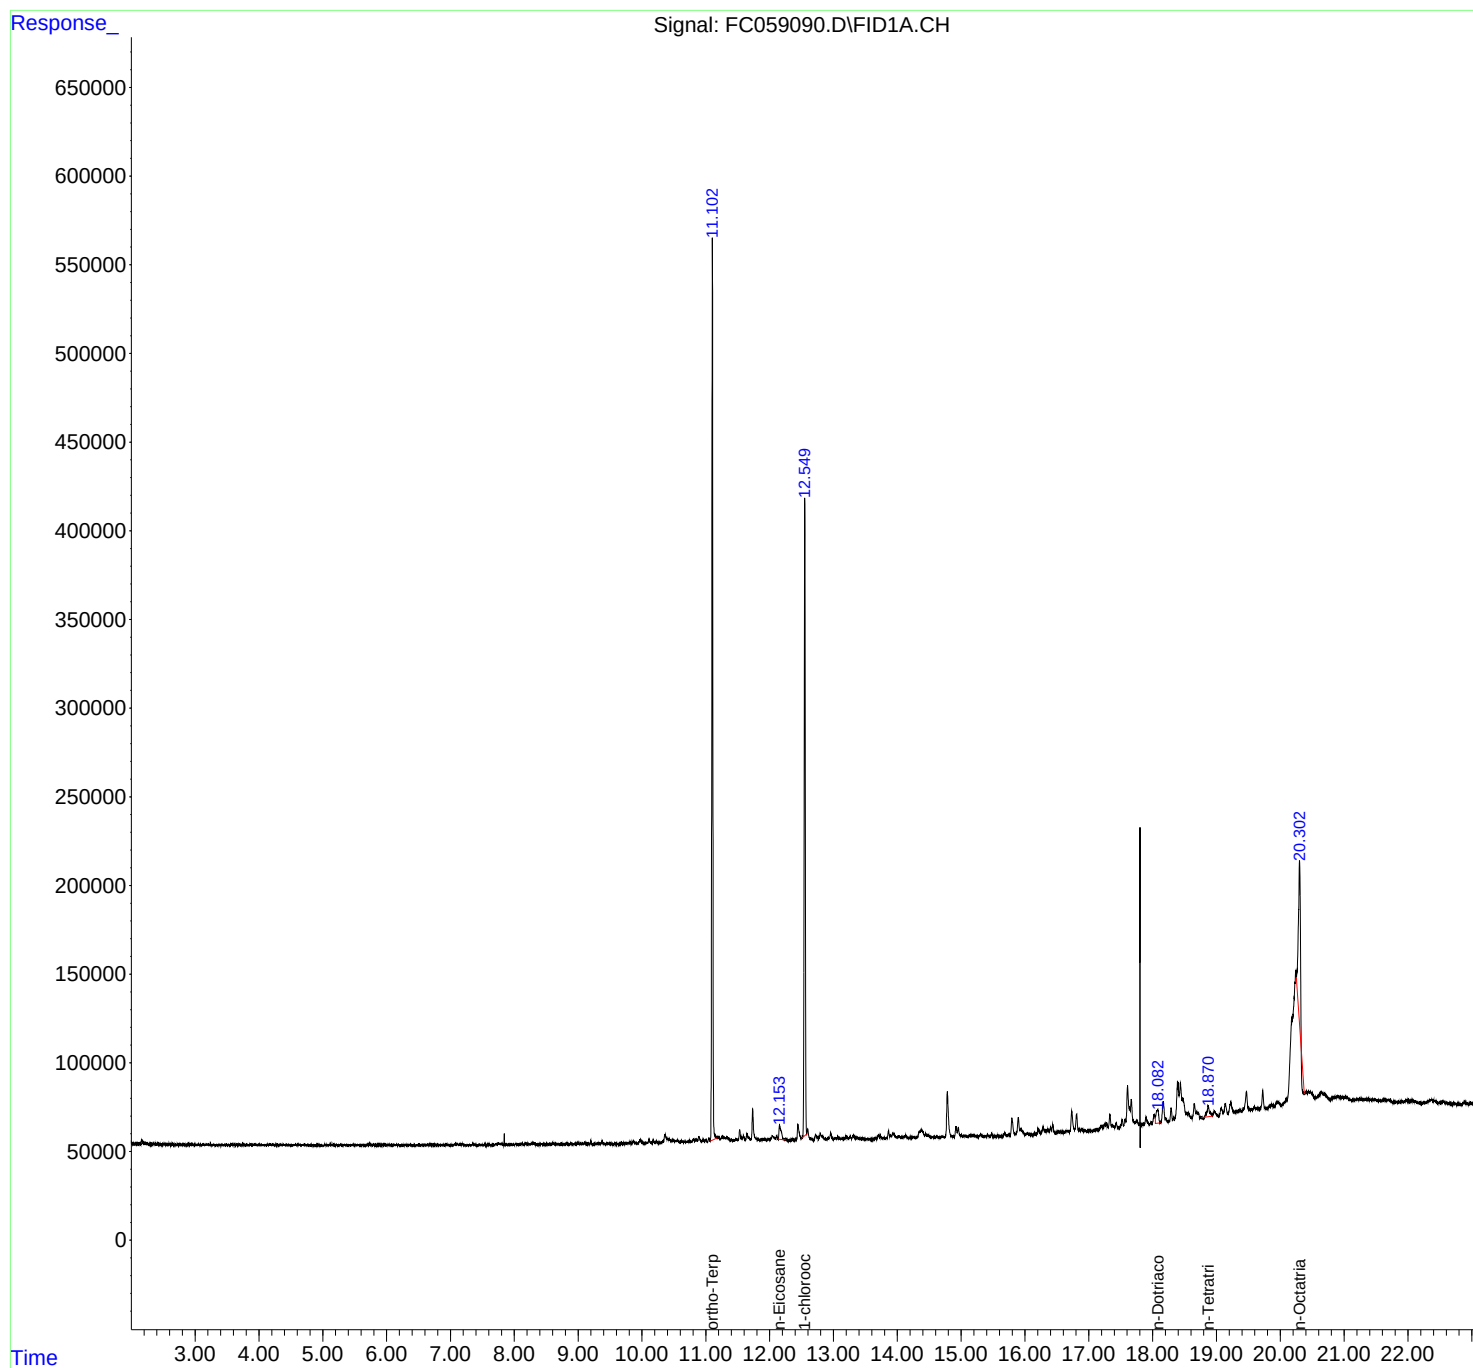


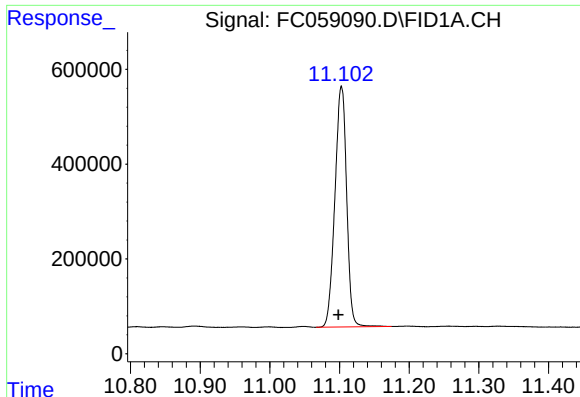

#9 ortho-Terphenyl (SURR)


R.T.: 11.103 min
Delta R.T.: 0.004 min
Response: 5939249
Conc: 41.22 ug/ml

Instrument :
FID_C
ClientSampleId :

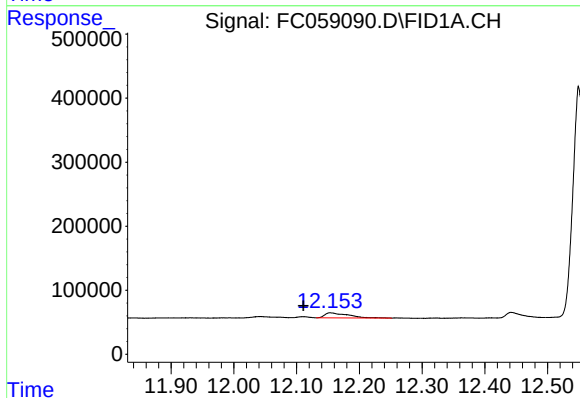


#10 n-Eicosane (C20)

R.T.: 12.155 min
Delta R.T.: 0.044 min
Response: 199369
Conc: 1.52 ug/ml

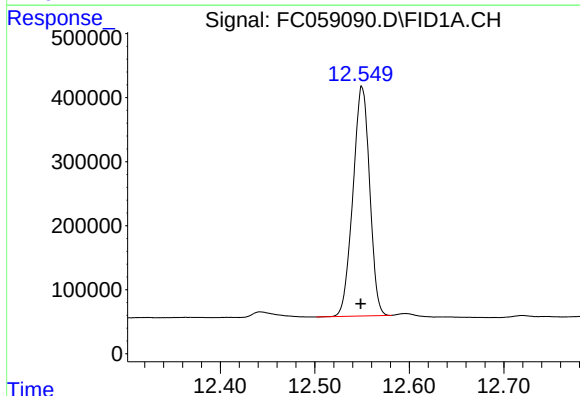


#12 1-chlorooctadecane (SURR)

R.T.: 12.550 min
Delta R.T.: 0.002 min
Response: 4414068
Conc: 39.38 ug/ml

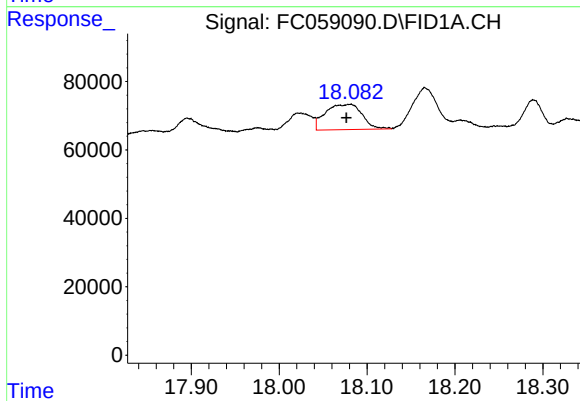

#18 n-Dotriacontane (C32)


R.T.: 18.080 min
Delta R.T.: 0.004 min
Response: 214791
Conc: 2.00 ug/ml

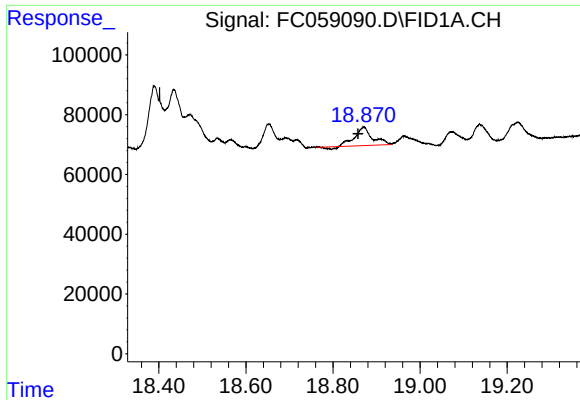

#19 n-Tetratriacontane (C34)

R.T.: 18.871 min
Delta R.T.: 0.013 min
Response: 164534
Conc: 1.63 ug/ml

Instrument :
FID_C
ClientSampleId :

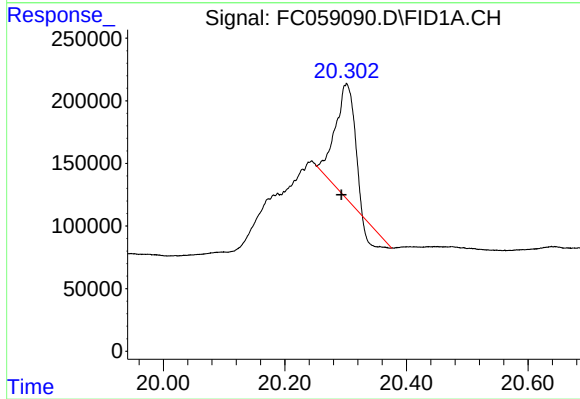

#21 n-Octatriacontane (C38)

R.T.: 20.301 min
Delta R.T.: 0.008 min
Response: 1751963
Conc: 19.04 ug/ml