

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040622AL\
 Data File : FC059099.D
 Signal(s) : FID1A.CH
 Acq On : 07 Apr 2022 2:42
 Operator : UA/NP
 Sample : N2263-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 07 06:56:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.102	5932463	41.174 ug/ml
Spiked Amount 50.000		Recovery =	82.35%
12) S 1-chlorooctadecane (S...	12.550	4605750	41.088 ug/ml
Spiked Amount 50.000		Recovery =	82.18%
Target Compounds			
10) T n-Eicosane (C20)	12.154	177490	1.355 ug/ml
14) T n-Tetracosane (C24)	14.442	268763	2.128 ug/ml
15) T n-Hexacosane (C26)	15.474f	176144	1.458 ug/ml
18) T n-Dotriacontane (C32)	18.071	180047	1.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040622AL\
Data File : FC059099.D
Signal(s) : FID1A.CH
Acq On : 07 Apr 2022 2:42
Operator : UA/NP
Sample : N2263-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 07 06:56:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

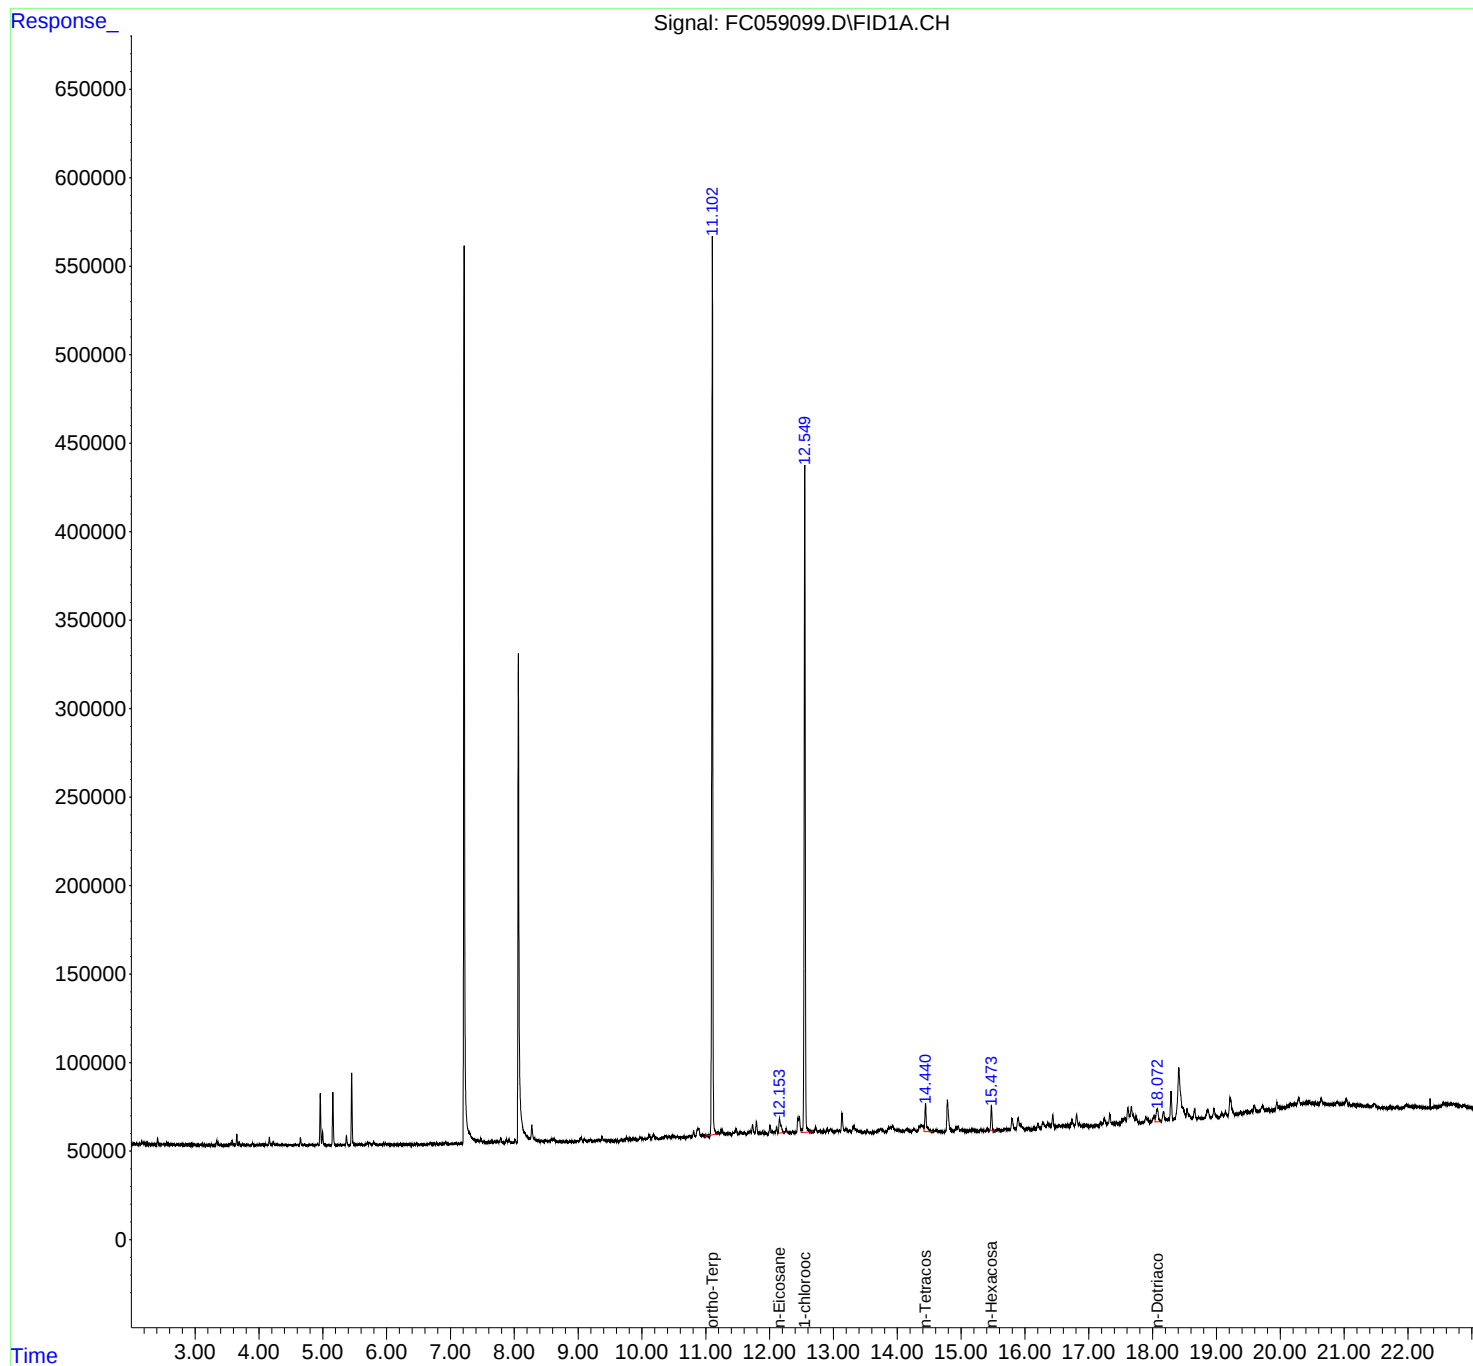


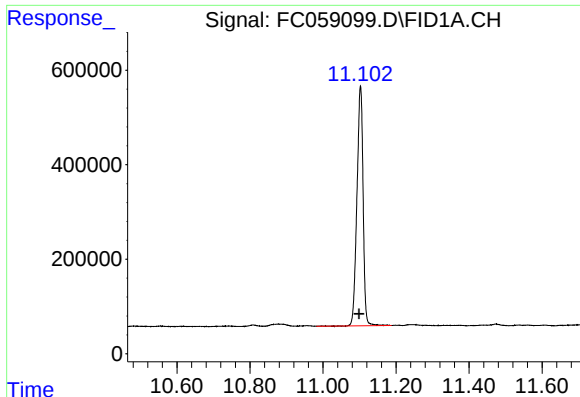

#9 ortho-Terphenyl (SURR)


R.T.: 11.102 min
Delta R.T.: 0.004 min
Response: 5932463
Conc: 41.17 ug/ml

Instrument :
FID_C
ClientSampleId :

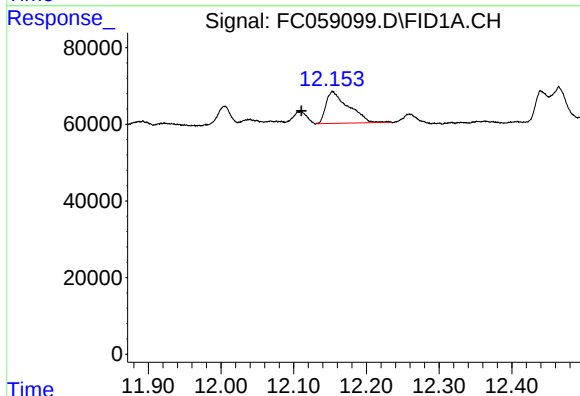


#10 n-Eicosane (C20)

R.T.: 12.154 min
Delta R.T.: 0.043 min
Response: 177490
Conc: 1.35 ug/ml

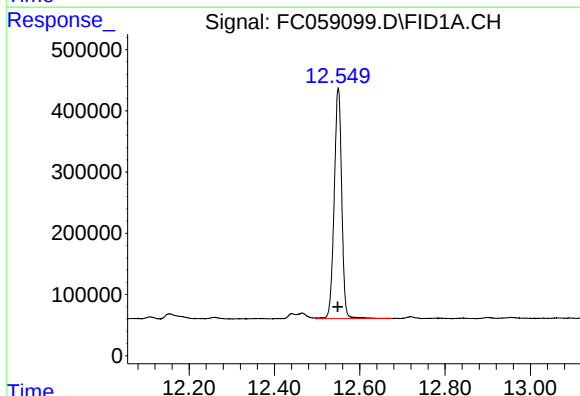


#12 1-chlorooctadecane (SURR)

R.T.: 12.550 min
Delta R.T.: 0.001 min
Response: 4605750
Conc: 41.09 ug/ml

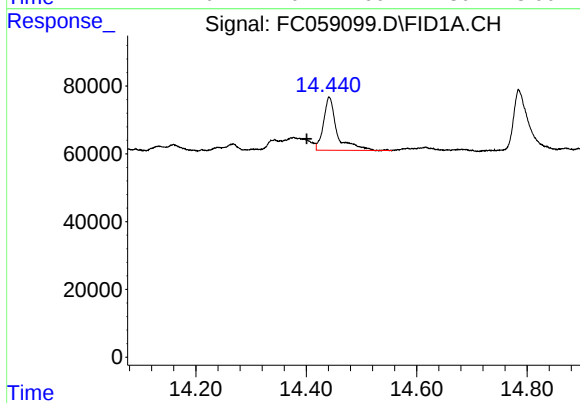

#14 n-Tetracosane (C24)


R.T.: 14.442 min
Delta R.T.: 0.041 min
Response: 268763
Conc: 2.13 ug/ml

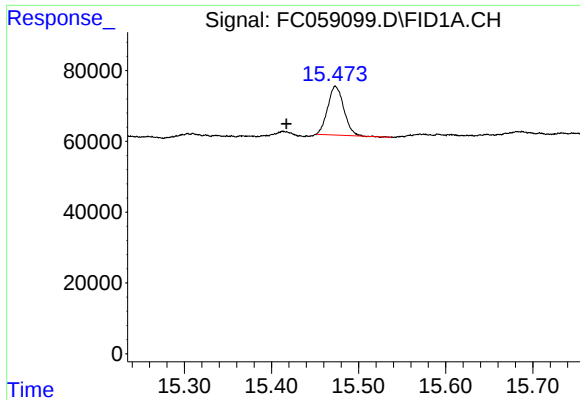

#15 n-Hexacosane (C26)

R.T.: 15.474 min
Delta R.T.: 0.057 min
Response: 176144
Conc: 1.46 ug/ml

Instrument :
FID_C
ClientSampleId :

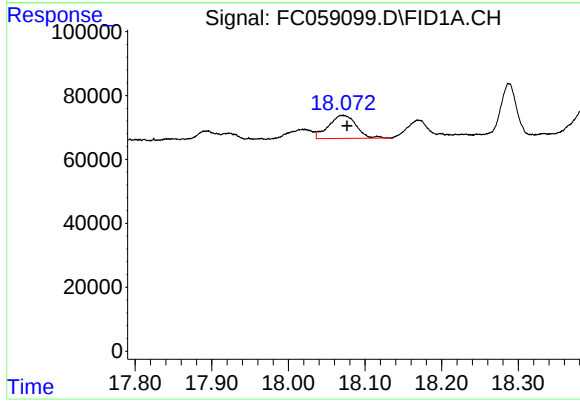

#18 n-Dotriacontane (C32)

R.T.: 18.071 min
Delta R.T.: -0.006 min
Response: 180047
Conc: 1.68 ug/ml