

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040723AL\
 Data File : FC063344.D
 Signal(s) : FID1A.ch
 Acq On : 07 Apr 2023 23:09
 Operator : YP/AJ
 Sample : 02213-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2023
 Supervised By :Ankita Jodhani 04/10/2023

Integration File: autoint1.e
 Quant Time: Apr 10 05:51:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 05 07:22:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.971	4867322	43.990 ug/ml
Spiked Amount 50.000		Recovery =	87.98%
Target Compounds			
1) T n-Nonane (C9)	3.301	156854	1.117 ug/ml
2) T n-Decane (C10)	4.366	194391	1.426 ug/ml
4) T n-Dodecane (C12)	6.383	257579	1.915 ug/ml
6) T n-Tetradecane (C14)	8.177	231120	1.707 ug/ml
7) T n-Hexadecane (C16)	9.776	241435	1.778 ug/ml
8) T n-Octadecane (C18)	11.217	263852	1.905 ug/ml
10) T n-Eicosane (C20)	12.525	270195	2.011 ug/ml
11) T n-Heneicosane (C21)	13.135	243703	1.811 ug/ml
13) T n-Docosane (C22)	13.721	266999	2.002 ug/ml
14) T n-Tetracosane (C24)	14.823	274975	2.045 ug/mlm
15) T n-Hexacosane (C26)	15.841	258791	1.933 ug/ml
16) T n-Octacosane (C28)	16.790	261321	1.930 ug/ml
17) T n-Tricontane (C30)	17.674	278041	2.010 ug/ml
18) T n-Dotriacontane (C32)	18.504	291284	2.063 ug/ml
19) T n-Tetratriacontane (C34)	19.286	287936	2.086 ug/ml
20) T n-Hexatriacontane (C36)	20.023	286519	2.242 ug/ml
21) T n-Octatriacontane (C38)	20.748	346939	2.818 ug/mlm
22) T n-Tetracontane (C40)	21.646	238078	2.023 ug/mlm

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC040723AL\
Data File : FC063344.D
Signal(s) : FID1A.ch
Acq On : 07 Apr 2023 23:09
Operator : YP/AJ
Sample : 02213-09
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

Integration File: autoint1.e
Quant Time: Apr 10 05:51:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 07:22:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

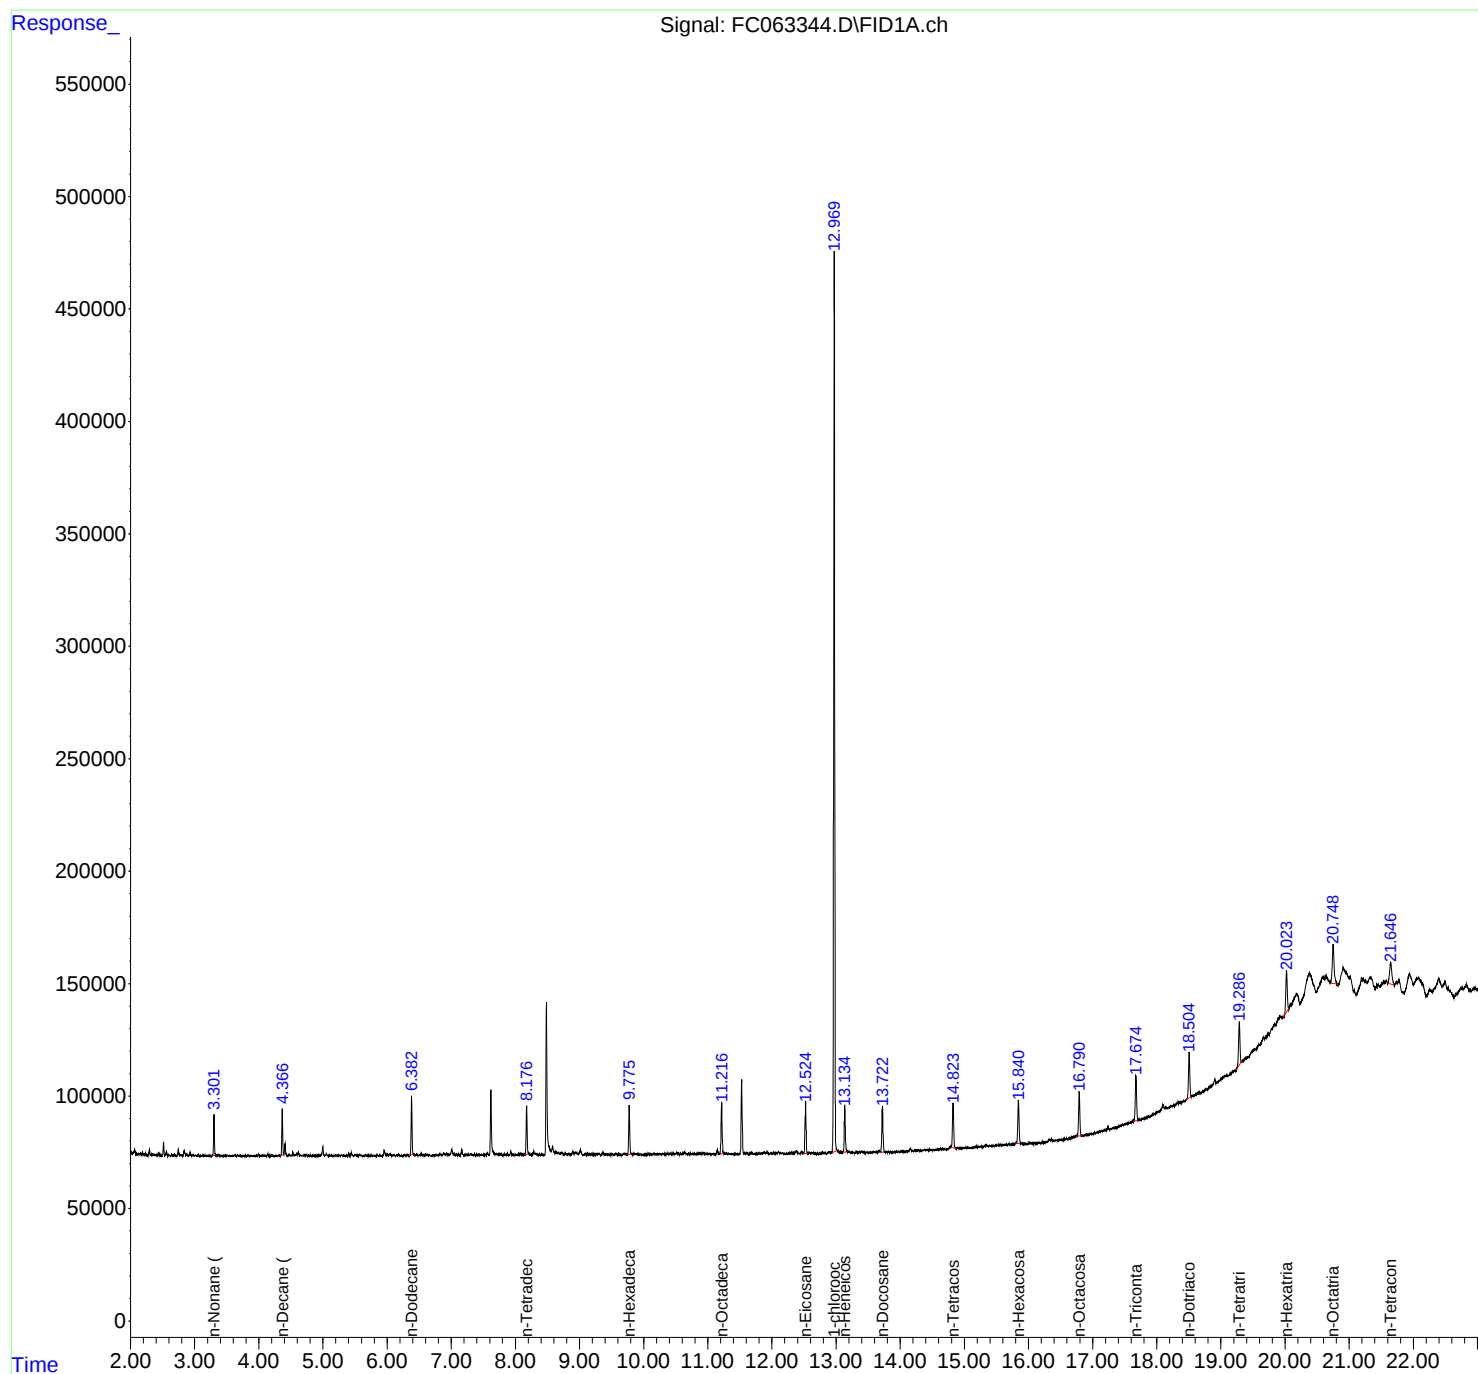

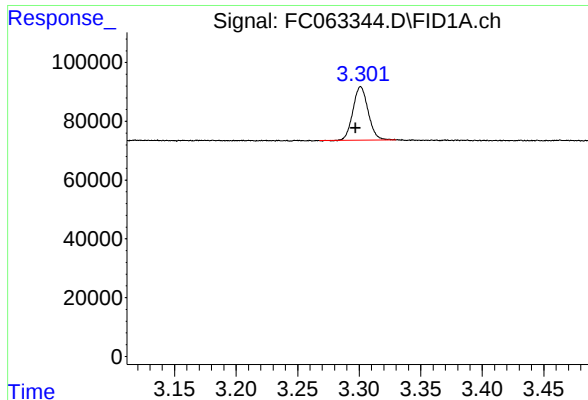


#1 n-Nonane (C9)

R.T.: 3.301 min
Delta R.T.: 0.004 min
Response: 156854
Conc: 1.12 ug/ml

Instrument :
FID_C
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

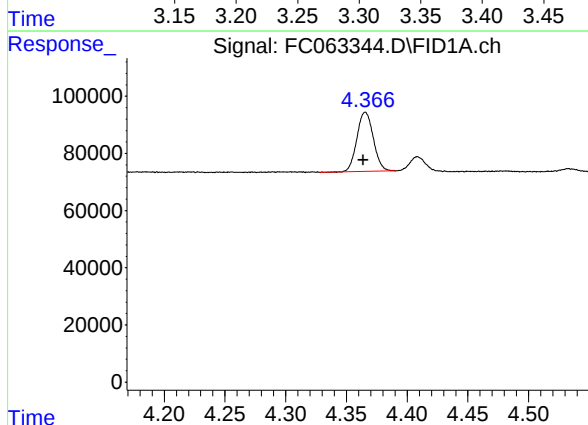


#2 n-Decane (C10)

R.T.: 4.366 min
Delta R.T.: 0.002 min
Response: 194391
Conc: 1.43 ug/ml

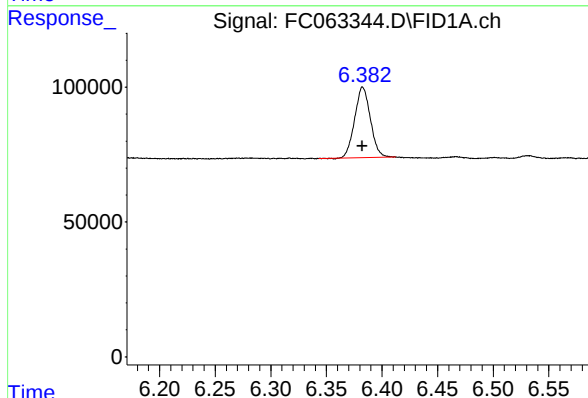


#4 n-Dodecane (C12)

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 257579
Conc: 1.91 ug/ml

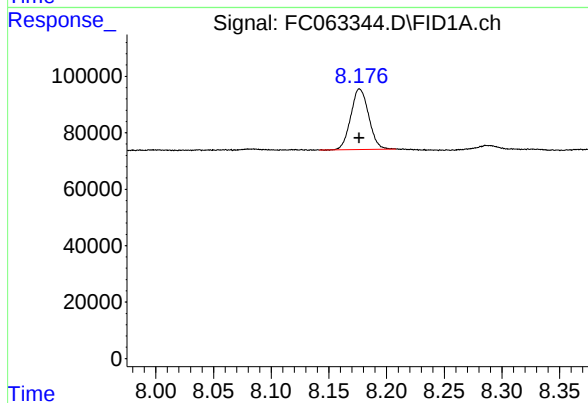

#6 n-Tetradecane (C14)

R.T.: 8.177 min
Delta R.T.: 0.000 min
Response: 231120
Conc: 1.71 ug/ml

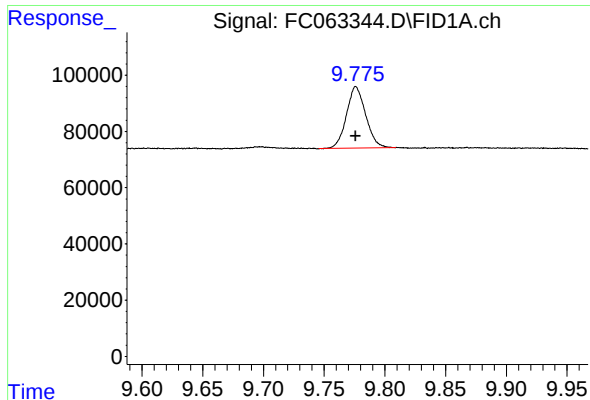


#7 n-Hexadecane (C16)

R.T.: 9.776 min
Delta R.T.: 0.000 min
Response: 241435
Conc: 1.78 ug/ml

Instrument : FID_C
ClientSampleId : MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

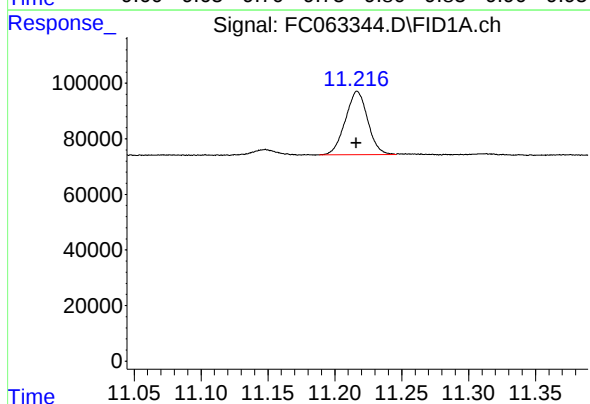


#8 n-Octadecane (C18)

R.T.: 11.217 min
Delta R.T.: 0.000 min
Response: 263852
Conc: 1.90 ug/ml

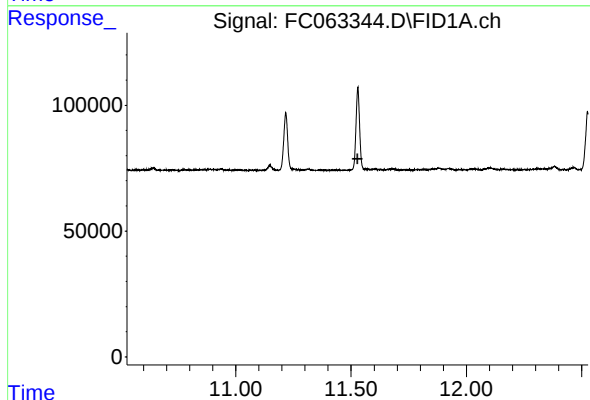


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.528 min
Response: 0
Conc: N.D.

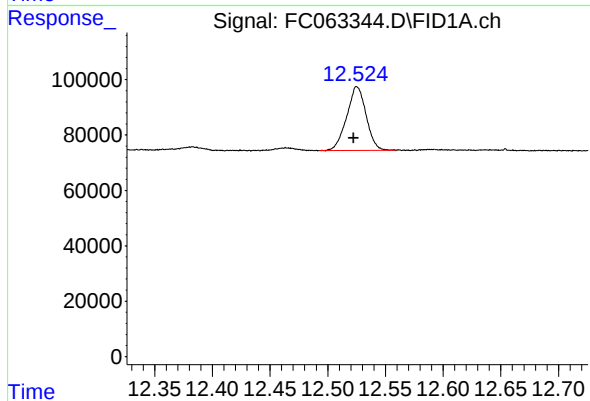

#10 n-Eicosane (C20)

R.T.: 12.525 min
Delta R.T.: 0.003 min
Response: 270195
Conc: 2.01 ug/ml

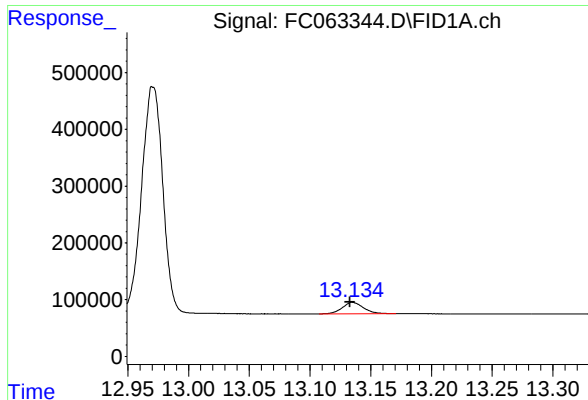


#11 n-Heneicosane (C21)

R.T.: 13.135 min
Delta R.T.: 0.002 min
Response: 243703
Conc: 1.81 ug/ml

Instrument :
FID_C
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

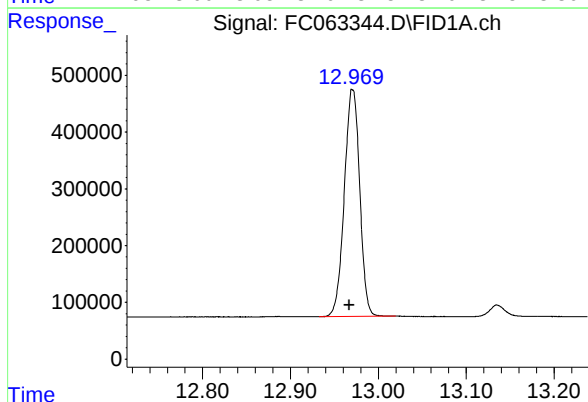


#12 1-chlorooctadecane (SURR)

R.T.: 12.971 min
Delta R.T.: 0.004 min
Response: 4867322
Conc: 43.99 ug/ml

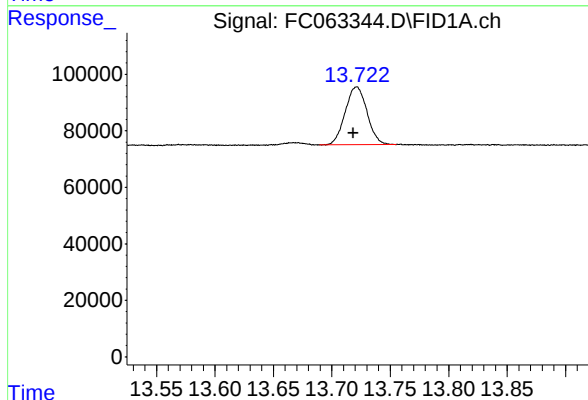


#13 n-Docosane (C22)

R.T.: 13.721 min
Delta R.T.: 0.003 min
Response: 266999
Conc: 2.00 ug/ml

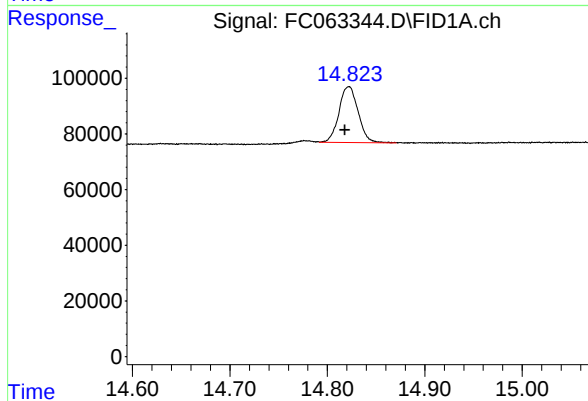

#14 n-Tetracosane (C24)

R.T.: 14.823 min
Delta R.T.: 0.005 min
Response: 274975
Conc: 2.05 ug/ml m

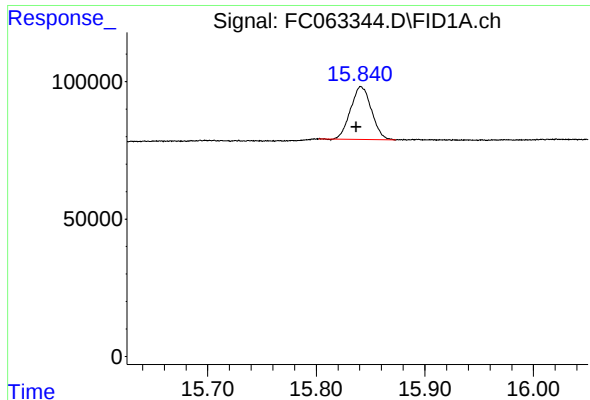

#15 n-Hexacosane (C26)

R.T.: 15.841 min
Delta R.T.: 0.004 min
Response: 258791
Conc: 1.93 ug/ml

Instrument :


FID_C

ClientSampleId :

MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

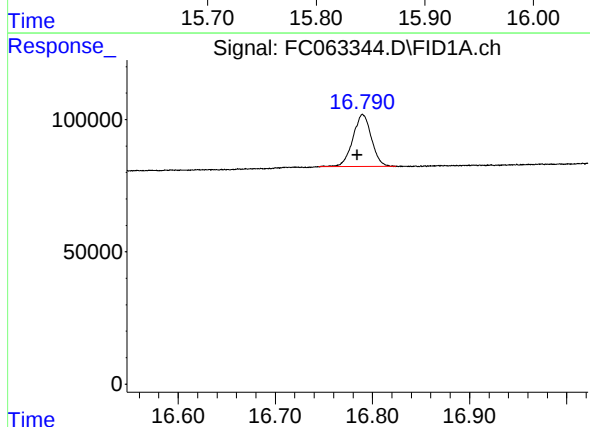


#16 n-Octacosane (C28)

R.T.: 16.790 min
Delta R.T.: 0.006 min
Response: 261321
Conc: 1.93 ug/ml

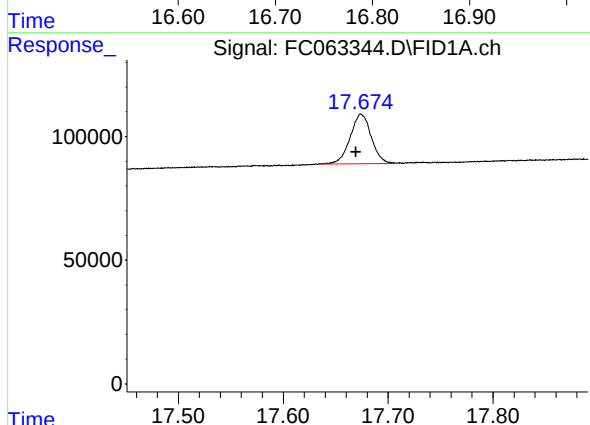


#17 n-Tricontane (C30)

R.T.: 17.674 min
Delta R.T.: 0.005 min
Response: 278041
Conc: 2.01 ug/ml

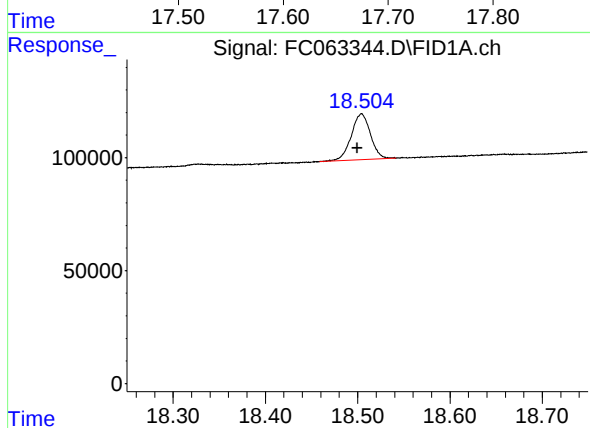

#18 n-Dotriacontane (C32)

R.T.: 18.504 min
Delta R.T.: 0.005 min
Response: 291284
Conc: 2.06 ug/ml

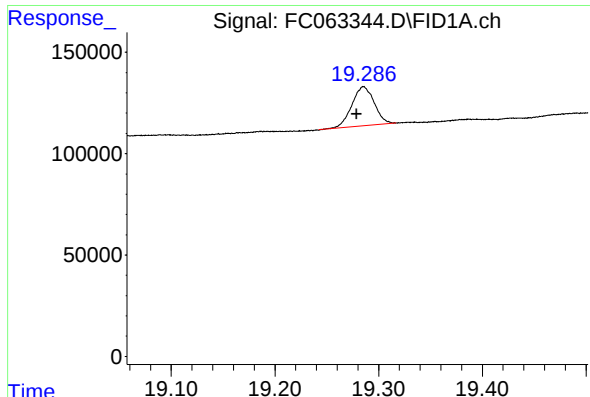


#19 n-Tetratriacontane (C34)

R.T.: 19.286 min
Delta R.T.: 0.007 min
Response: 287936
Conc: 2.09 ug/ml

Instrument :
FID_C
ClientSampleId :
MDL-WATER-03-QT2-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

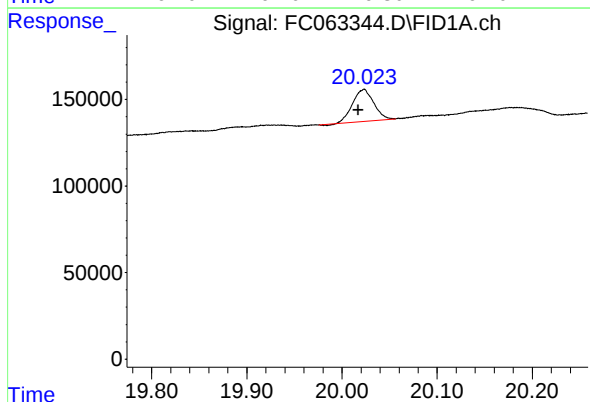


#20 n-Hexatriacontane (C36)

R.T.: 20.023 min
Delta R.T.: 0.006 min
Response: 286519
Conc: 2.24 ug/ml

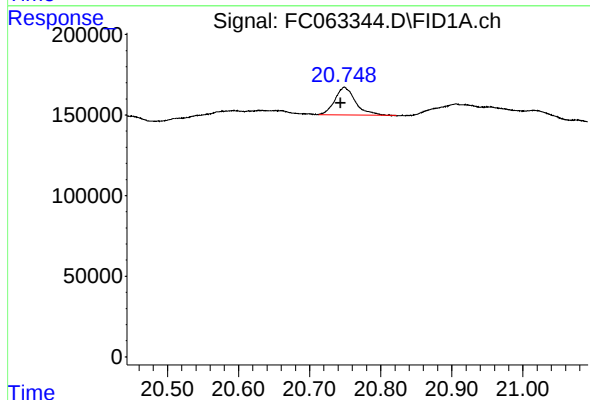

#21 n-Octatriacontane (C38)

R.T.: 20.748 min
Delta R.T.: 0.005 min
Response: 346939
Conc: 2.82 ug/ml m

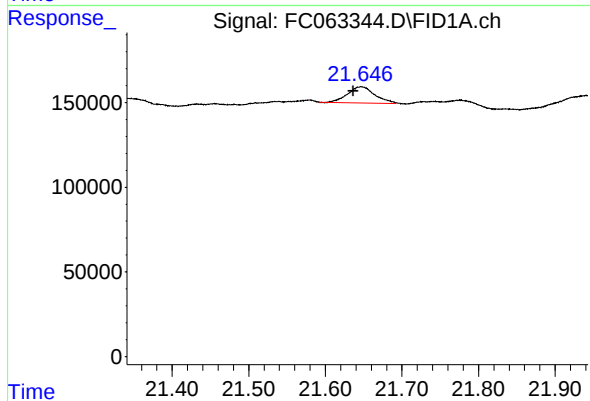

#22 n-Tetracontane (C40)

R.T.: 21.646 min
Delta R.T.: 0.009 min
Response: 238078
Conc: 2.02 ug/ml m