

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041322AL\
 Data File : FC059250.D
 Signal(s) : FID1A.CH
 Acq On : 15 Apr 2022 5:06
 Operator : UA/NP
 Sample : N2376-01DL 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 NB-07-041222DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/15/2022
 Supervised By :mohammad ahmed 04/18/2022

Integration File: autoint1.e
 Quant Time: Apr 15 05:57:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.097	2049586	14.225 ug/mlm
Spiked Amount 50.000		Recovery =	28.45%
12) S 1-chlorooctadecane (S...	12.546	1568237	13.990 ug/ml
Spiked Amount 50.000		Recovery =	27.98%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041322AL\
Data File : FC059250.D
Signal(s) : FID1A.CH
Acq On : 15 Apr 2022 5:06
Operator : UA/NP
Sample : N2376-01DL 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
NB-07-041222DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/15/2022
Supervised By :mohammad ahmed 04/18/2022

Integration File: autoint1.e
Quant Time: Apr 15 05:57:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

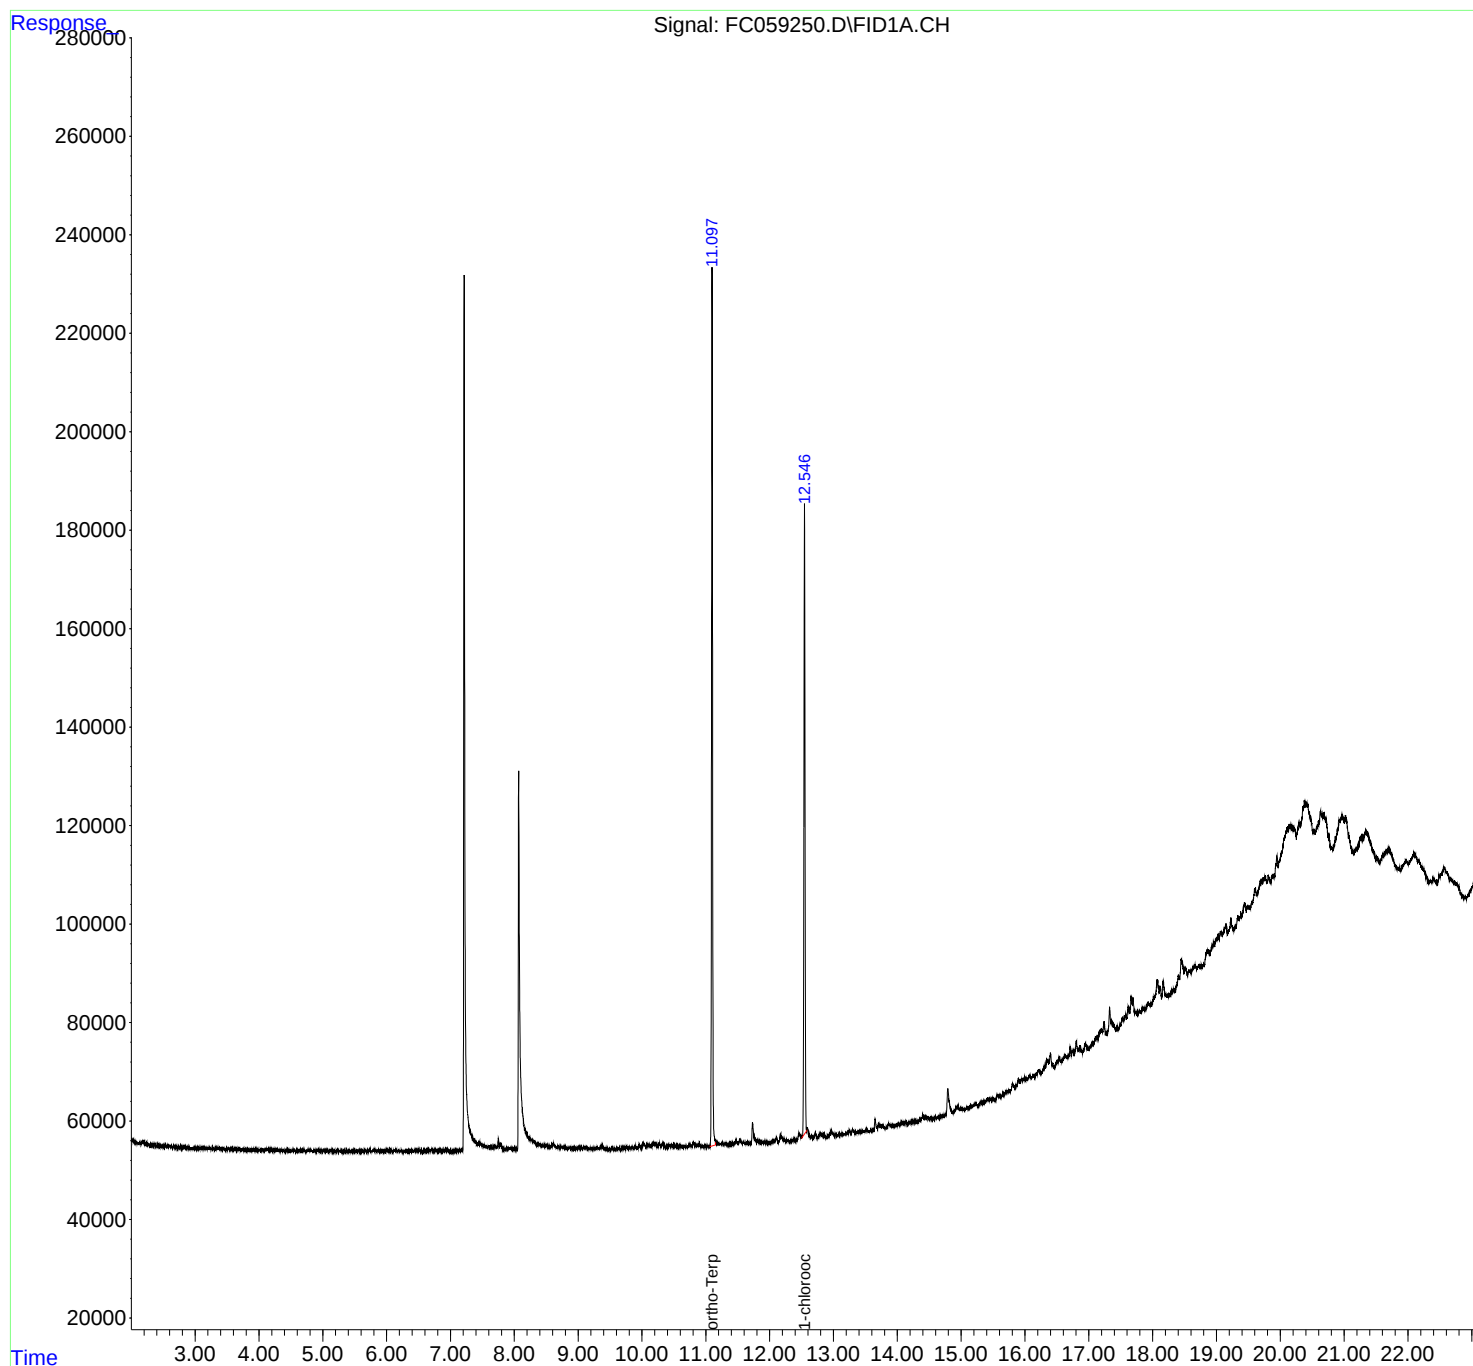

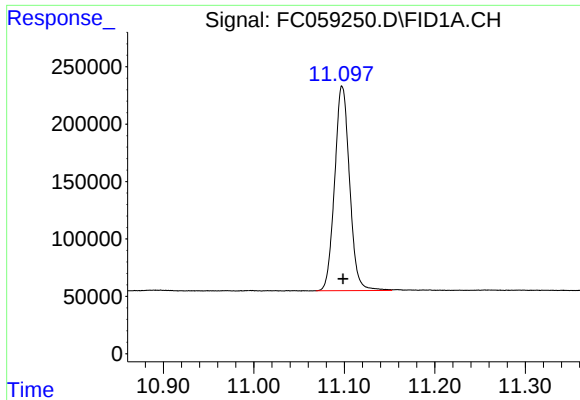

#9 ortho-Terphenyl (SURR)

R.T.: 11.097 min
Delta R.T.: -0.002 min
Response: 2049586
Conc: 14.23 ug/ml

Instrument :

FID_C

ClientSampleId :


NB-07-041222DL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/15/2022

Supervised By :mohammad ahmed 04/18/2022

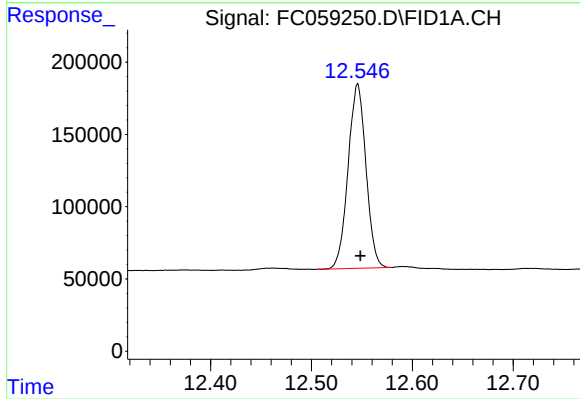

#12 1-chlorooctadecane (SURR)

R.T.: 12.546 min
Delta R.T.: -0.003 min
Response: 1568237
Conc: 13.99 ug/ml