

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041723AL\
Data File : FC063390.D
Signal(s) : FID1A.ch
Acq On : 17 Apr 2023 08:04
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 17 15:42:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 07:22:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.129	523720	3.891 ug/ml
13) T	n-Docosane (C22)	13.715	315607	2.367 ug/ml
14) T	n-Tetracosane (C24)	14.821	287282	2.137 ug/ml
15) T	n-Hexacosane (C26)	15.841	199286	1.489 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041723AL\
Data File : FC063390.D
Signal(s) : FID1A.ch
Acq On : 17 Apr 2023 08:04
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 17 15:42:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 07:22:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

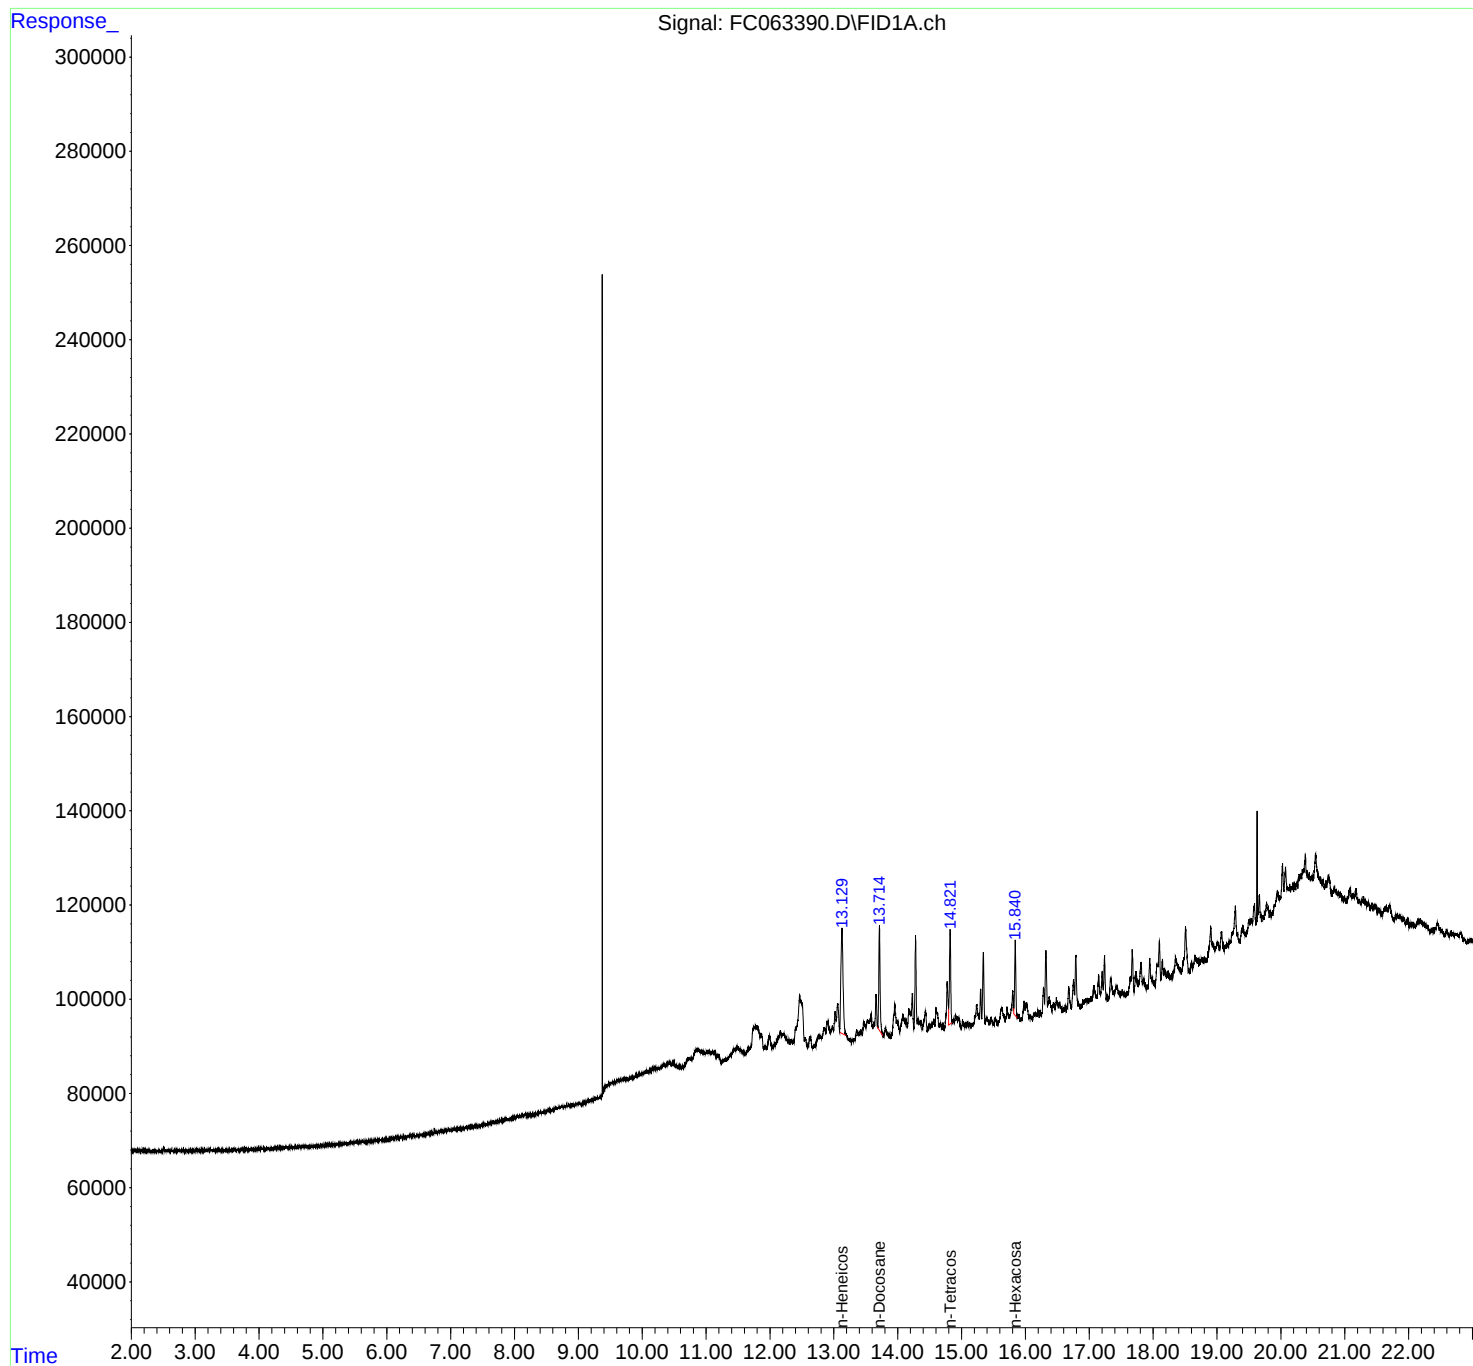


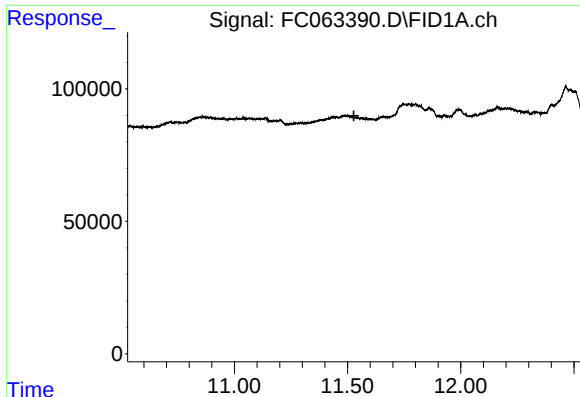

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.528 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

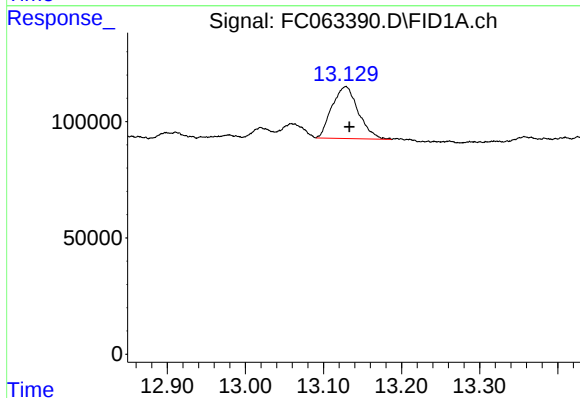


#11 n-Heneicosane (C21)

R.T.: 13.129 min
Delta R.T.: -0.005 min
Response: 523720
Conc: 3.89 ug/ml

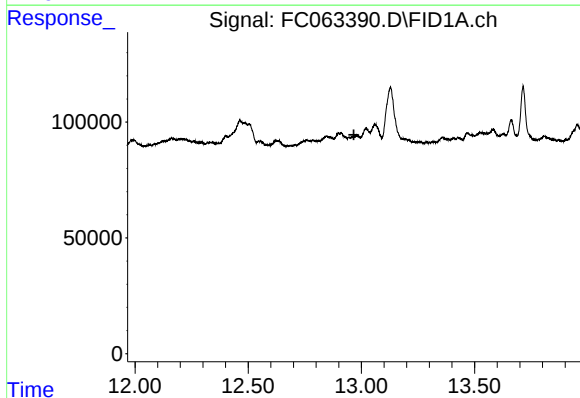


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.967 min
Response: 0
Conc: N.D.

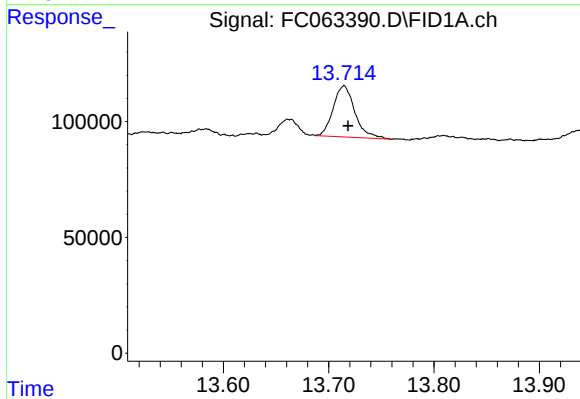

#13 n-Docosane (C22)


R.T.: 13.715 min
Delta R.T.: -0.004 min
Response: 315607
Conc: 2.37 ug/ml

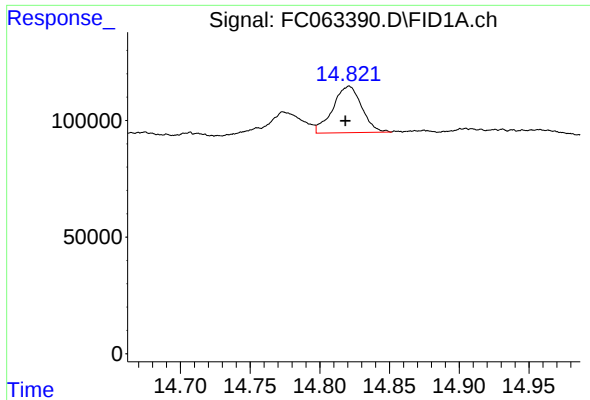

#14 n-Tetracosane (C24)

R.T.: 14.821 min
Delta R.T.: 0.003 min
Response: 287282
Conc: 2.14 ug/ml

Instrument :
FID_C
ClientSampleId :

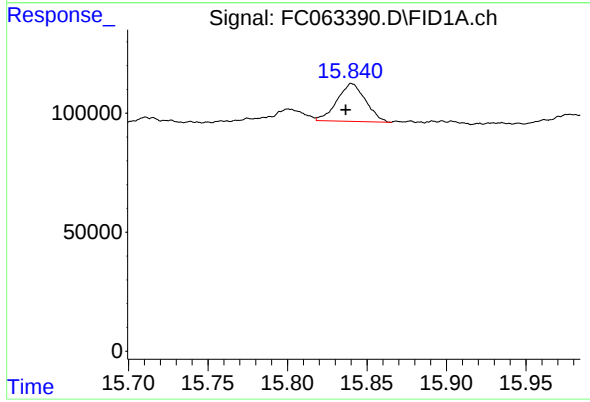

#15 n-Hexacosane (C26)

R.T.: 15.841 min
Delta R.T.: 0.004 min
Response: 199286
Conc: 1.49 ug/ml