

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041822AL\
 Data File : FC059282.D
 Signal(s) : FID1A.CH
 Acq On : 18 Apr 2022 15:14
 Operator : UA/NP
 Sample : N2423-05DL 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 D2460-D2462DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/19/2022
 Supervised By :mohammad ahmed 04/20/2022

Integration File: autoint1.e
 Quant Time: Apr 19 03:14:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 25 23:18:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.104	344364	2.390 ug/mlm
Spiked Amount	50.000	Recovery =	4.78%
12) S 1-chlorooctadecane (S...	12.553	225791	2.014 ug/mlm
Spiked Amount	50.000	Recovery =	4.03%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC041822AL\
Data File : FC059282.D
Signal(s) : FID1A.CH
Acq On : 18 Apr 2022 15:14
Operator : UA/NP
Sample : N2423-05DL 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
D2460-D2462DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2022
Supervised By :mohammad ahmed 04/20/2022

Integration File: autoint1.e
Quant Time: Apr 19 03:14:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 032522.M
Quant Title : GC Extractables
QLast Update : Fri Mar 25 23:18:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

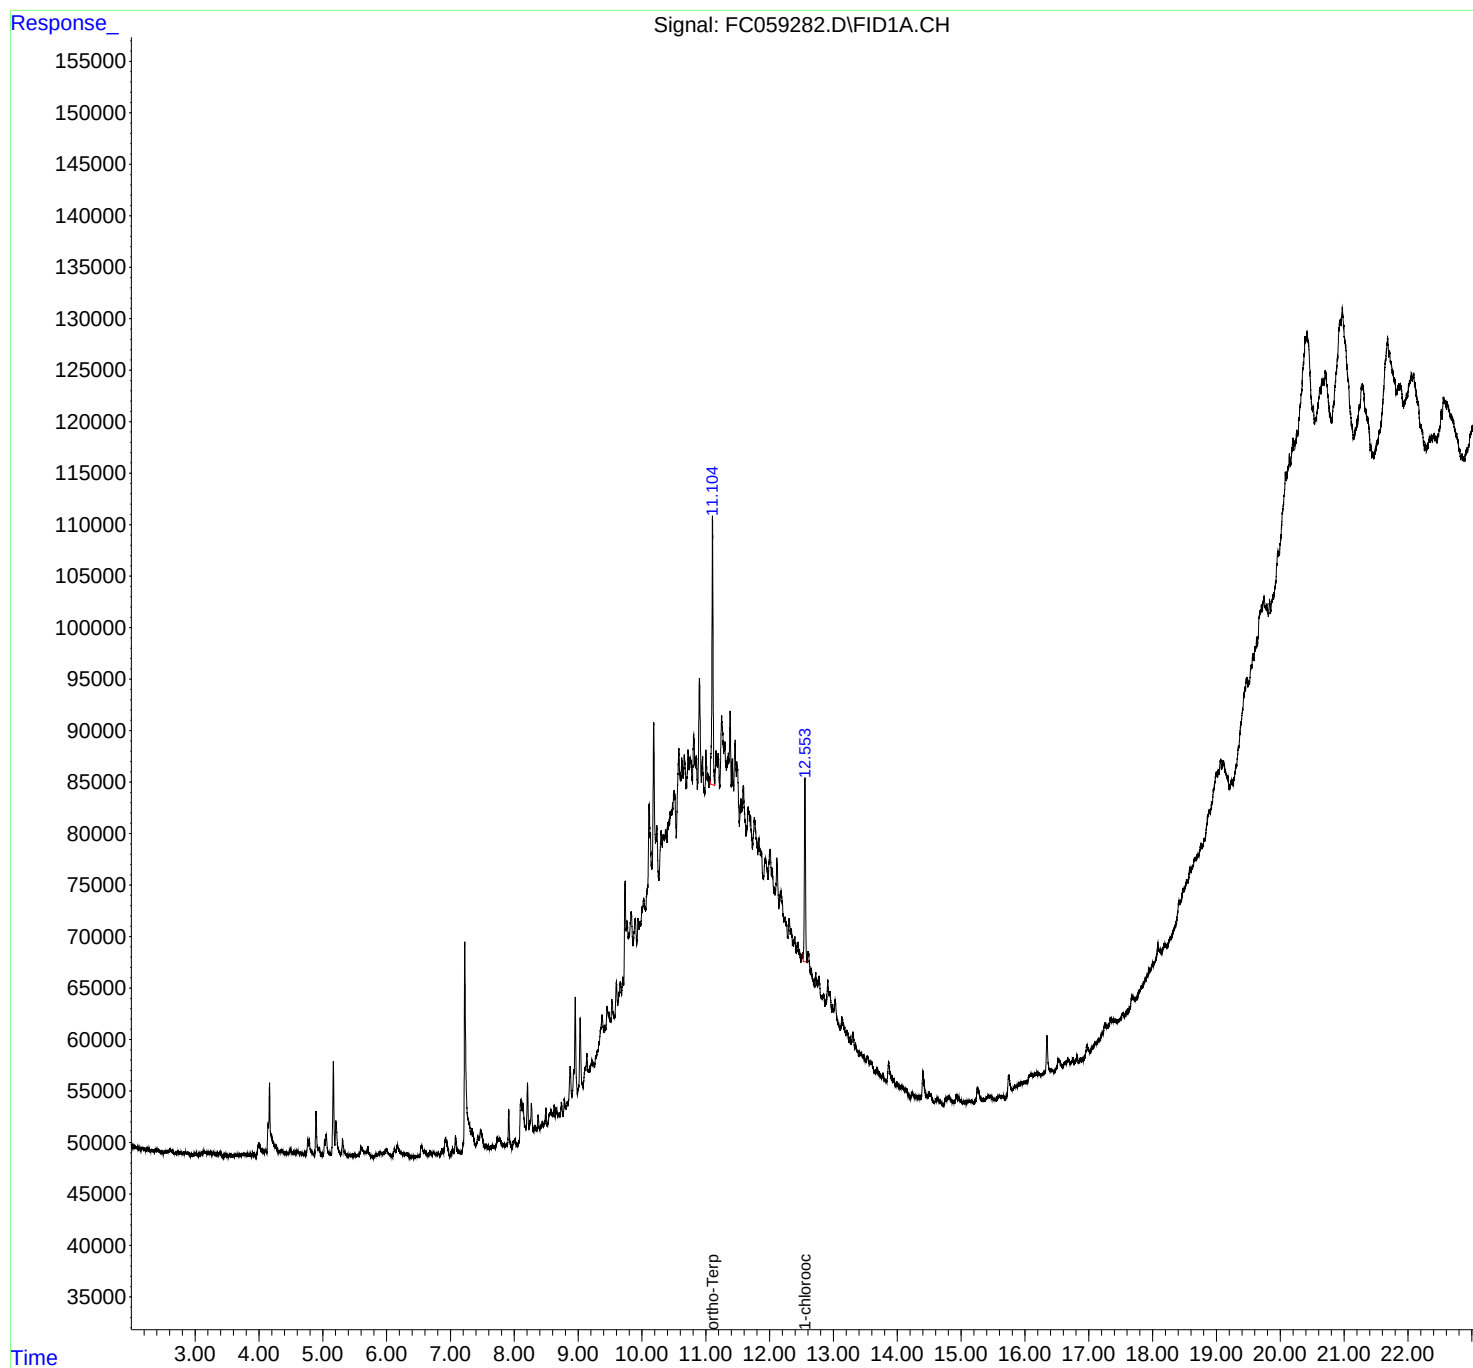

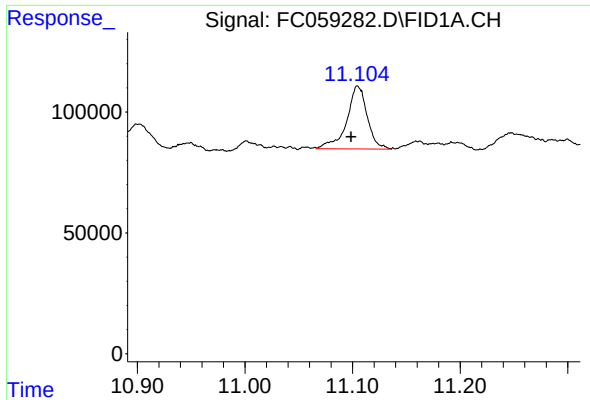


#9 ortho-Terphenyl (SURR)

R.T.: 11.104 min
Delta R.T.: 0.006 min
Response: 344364
Conc: 2.39 ug/ml

Instrument :
FID_C
ClientSampleId :
D2460-D2462DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2022
Supervised By :mohammad ahmed 04/20/2022

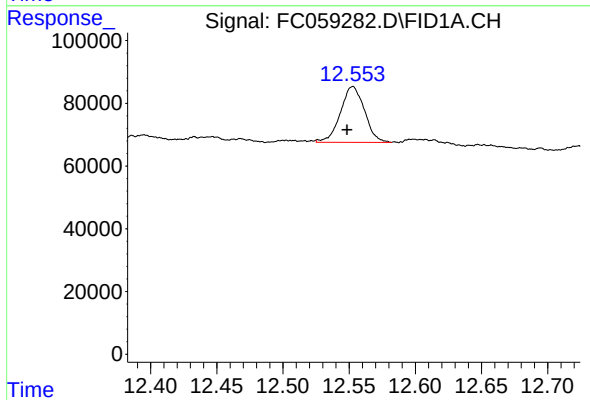

#12 1-chlorooctadecane (SURR)

R.T.: 12.553 min
Delta R.T.: 0.004 min
Response: 225791
Conc: 2.01 ug/ml m