

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC041825AL\  
 Data File : FC068645.D  
 Signal(s) : FID1A.ch  
 Acq On : 18 Apr 2025 22:17  
 Operator : YP/AJ  
 Sample : Q1825-04DL 10X  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 TP-10DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 04/21/2025  
 Supervised By :mohammad ahmed 04/22/2025

Integration File: autoint1.e  
 Quant Time: Apr 19 00:28:11 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 040925.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Apr 08 17:31:27 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.717 | 448680     | 3.524 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 7.05%        |
| 12) S 1-chlorooctadecane (S... | 13.152 | 381422     | 4.106 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 8.21%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC041825AL\  
Data File : FC068645.D  
Signal(s) : FID1A.ch  
Acq On : 18 Apr 2025 22:17  
Operator : YP/AJ  
Sample : Q1825-04DL 10X  
Misc :  
ALS Vial : 23 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
TP-10DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/21/2025  
Supervised By :mohammad ahmed 04/22/2025

Integration File: autoint1.e  
Quant Time: Apr 19 00:28:11 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 040925.M  
Quant Title : GC Extractables  
QLast Update : Tue Apr 08 17:31:27 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

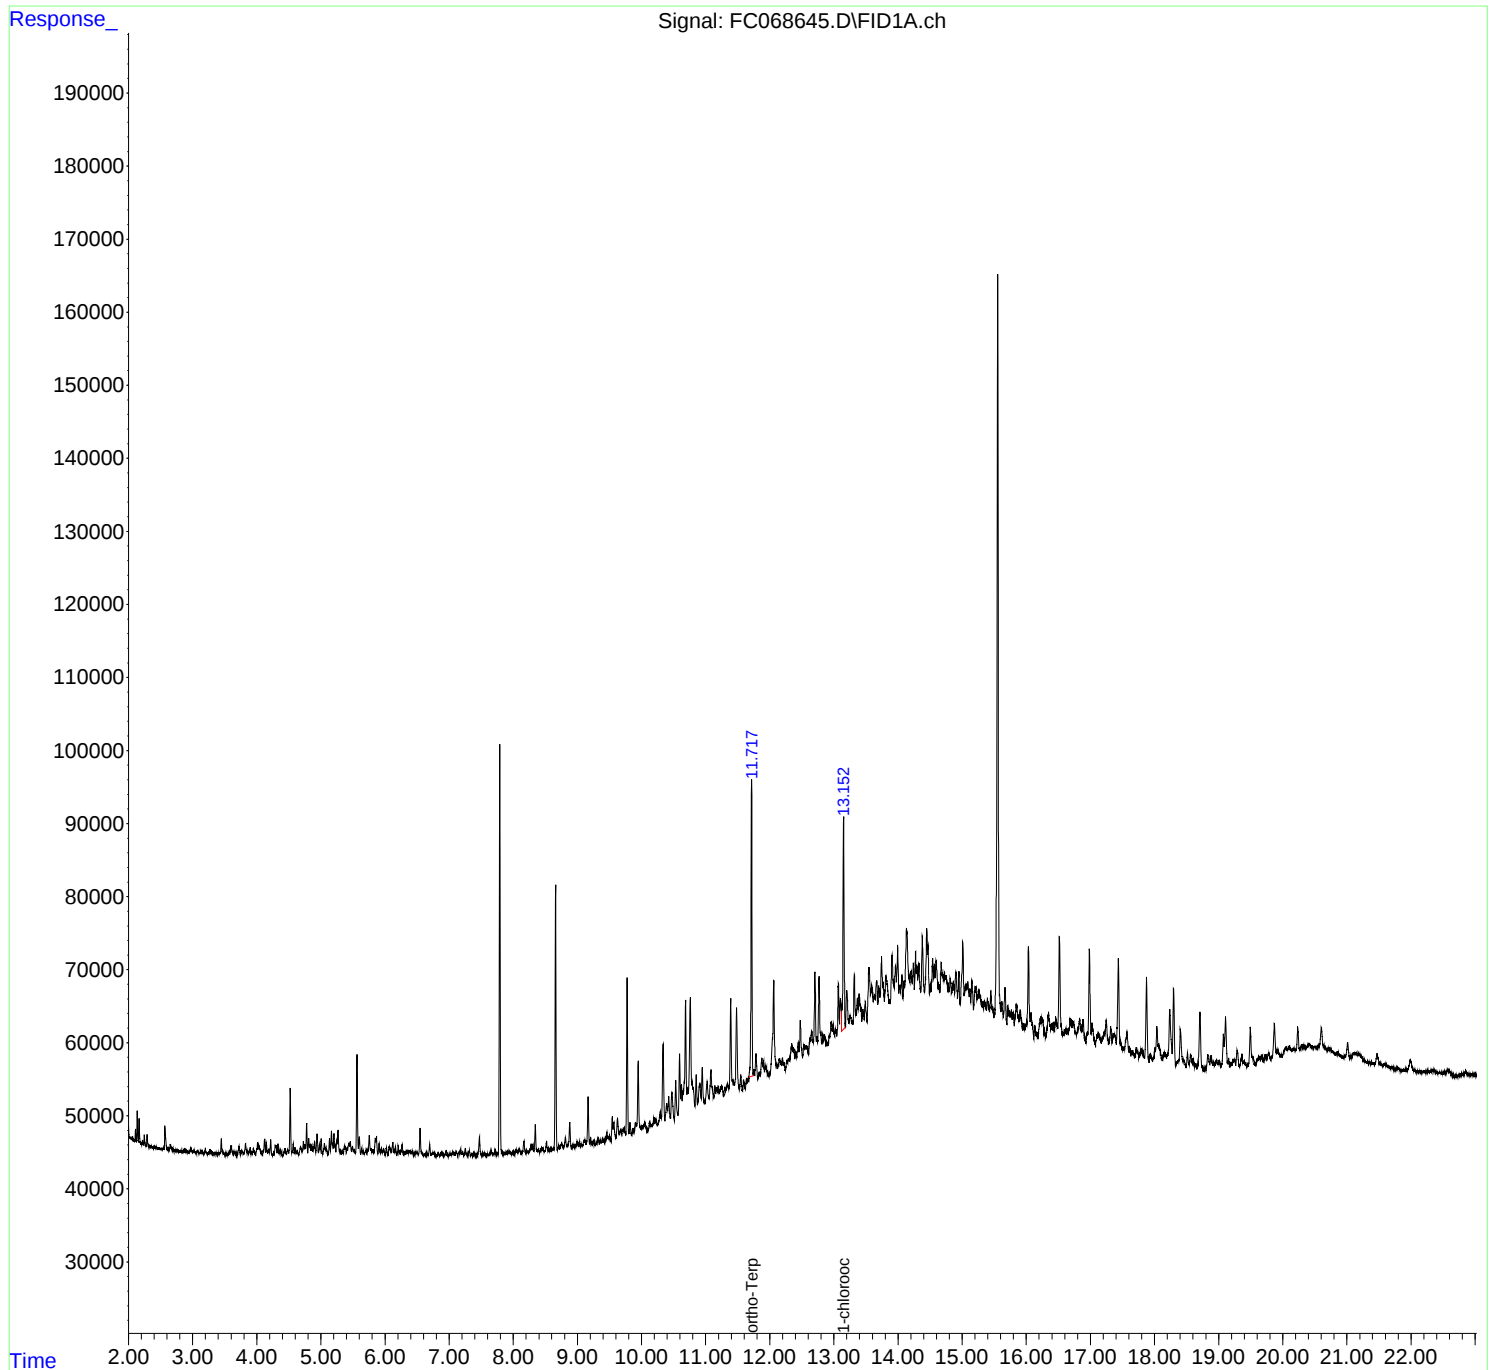

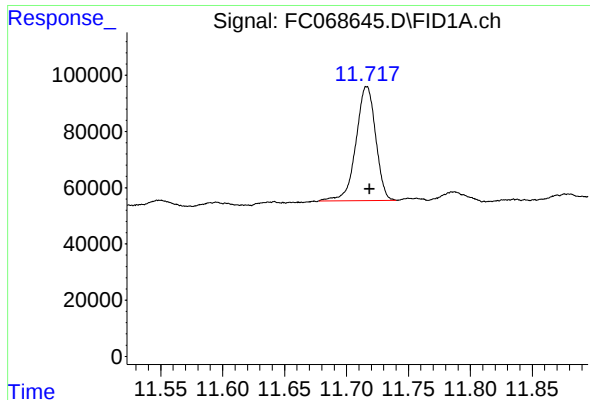


#9 ortho-Terphenyl (SURR)

R.T.: 11.717 min  
Delta R.T.: -0.002 min  
Response: 448680  
Conc: 3.52 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
TP-10DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 04/21/2025  
Supervised By :mohammad ahmed 04/22/2025

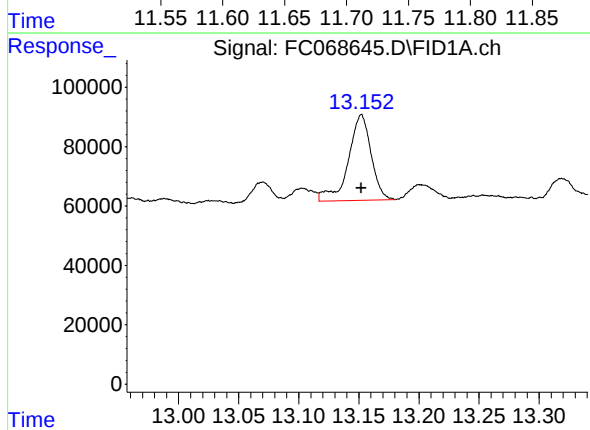

#12 1-chlorooctadecane (SURR)

R.T.: 13.152 min  
Delta R.T.: 0.000 min  
Response: 381422  
Conc: 4.11 ug/ml