

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
 Data File : PS019104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 01:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:19:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
 Quant Title : 8080.M
 QLast Update : Mon Apr 18 17:28:16 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.798	1635.3E6	376.6E6	437.227	518.874
Target Compounds							
8) T	DICHLORPROP	0.000	7.615	0	2180657	N.D.	2.610
11) T	2,4,5-TP ...	9.203	8.628f	-253521	6883887	N.D.	1.462
12) T	2,4,5-T	9.486	9.111f	8946865	2922592	<MDL	<MDL #
13) T	2,4-DB	10.039	0.000	2678201	0	<MDL	N.D. #
14) T	DINOSEB	11.140f	0.000	31314598	0	2.047	N.D. #
15) T	Picloram	11.039	10.878	47417164	8125418	1.770	1.372
16) T	DCPA	0.000	10.878f	0	8125418	N.D.	1.420


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS042022\
Data File : PS019104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 01:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:19:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041822.M
Quant Title : 8080.M
QLast Update : Mon Apr 18 17:28:16 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

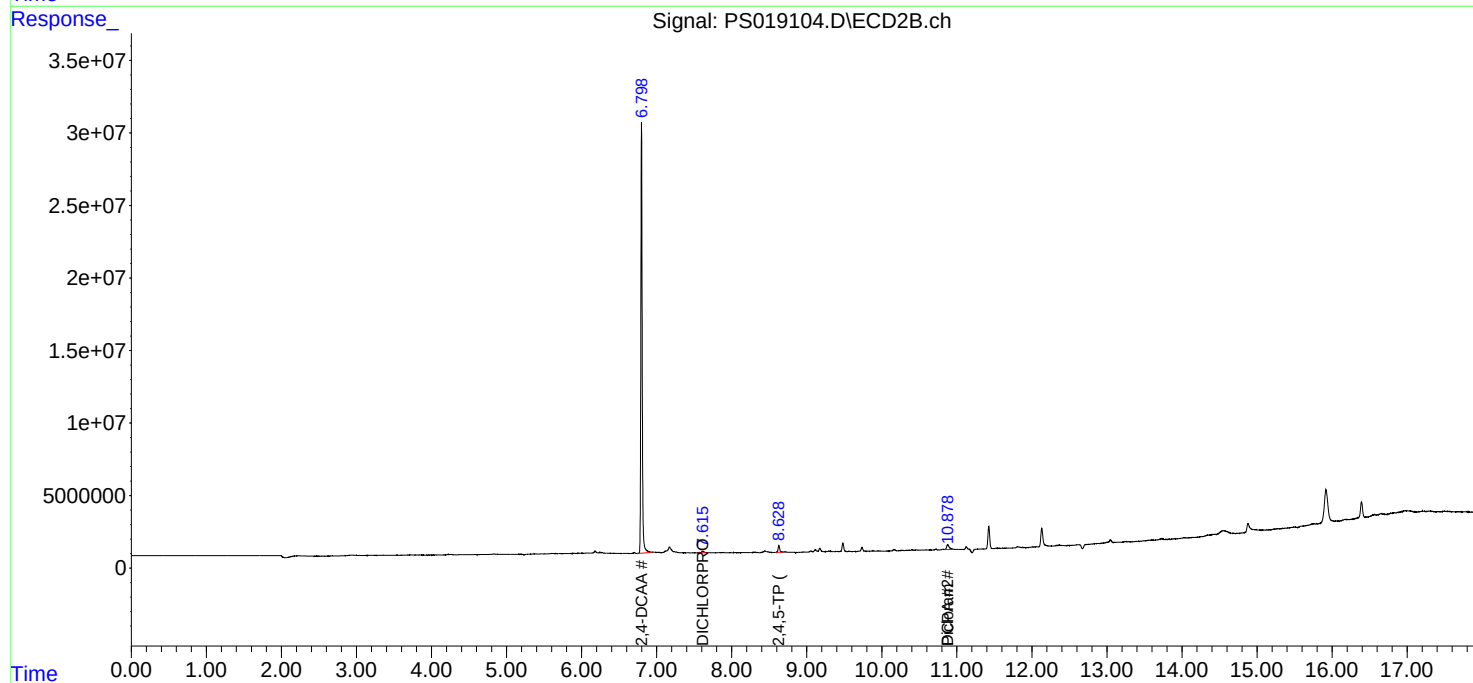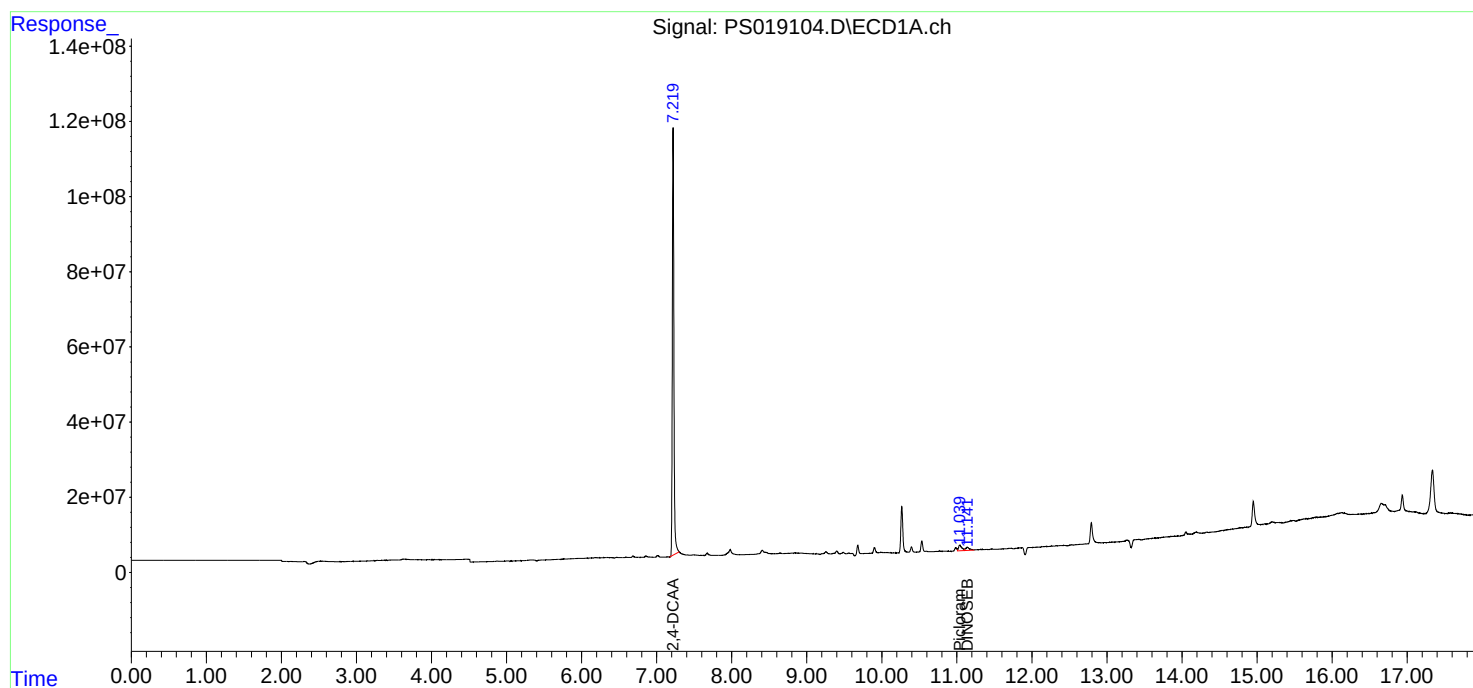

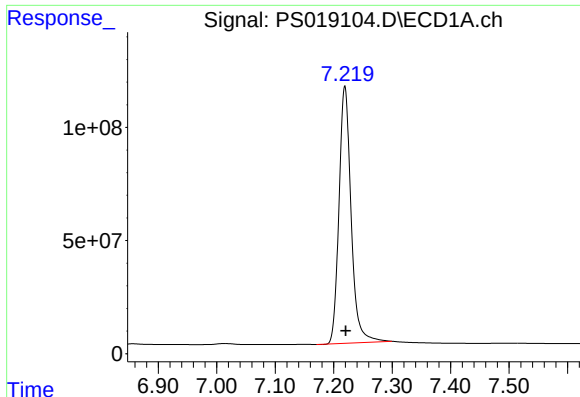


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.002 min
Response: 1635253870
Conc: 437.23 ng/ml

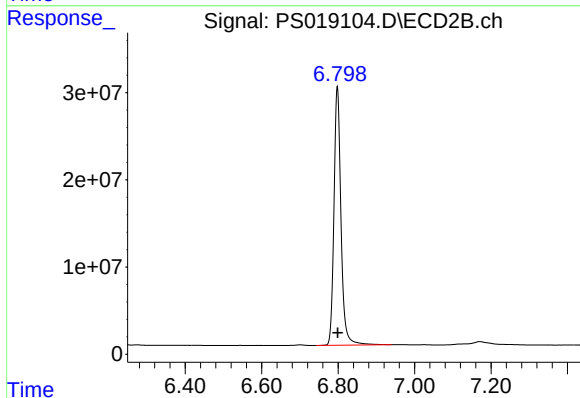


#4 2,4-DCAA

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 376638857
Conc: 518.87 ng/ml

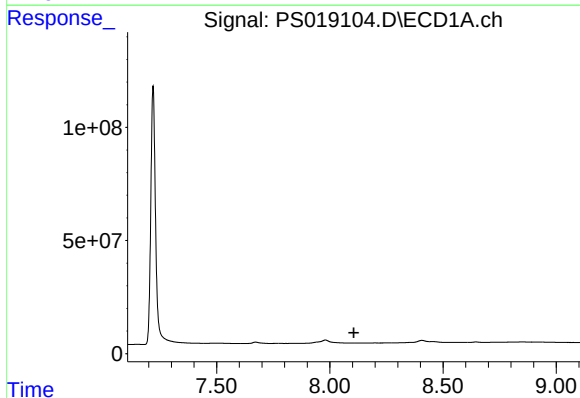


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.106 min
Response: 0
Conc: N.D.

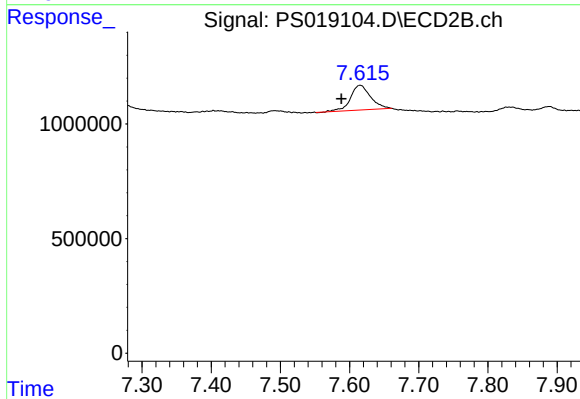


#8 DICHLORPROP

R.T.: 7.615 min
Delta R.T.: 0.027 min
Response: 2180657
Conc: 2.61 ng/ml

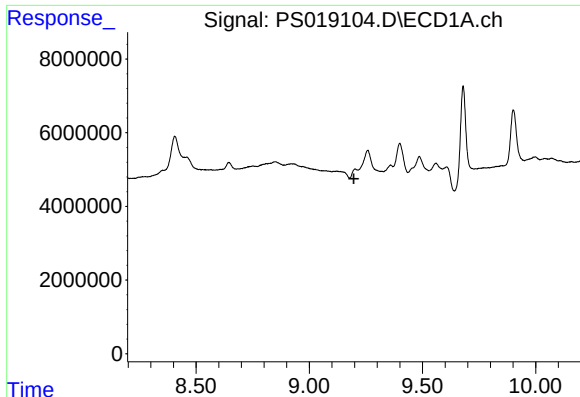


#11 2,4,5-TP (SILVEX)

R.T.: 9.203 min
Delta R.T.: 0.006 min
Response: -253521
Conc: N.D.

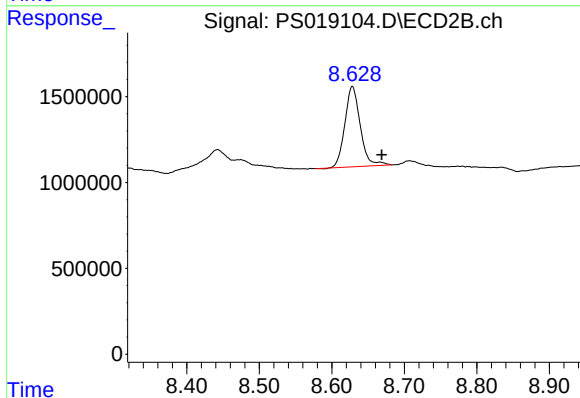


#11 2,4,5-TP (SILVEX)

R.T.: 8.628 min
Delta R.T.: -0.041 min
Response: 6883887
Conc: 1.46 ng/ml

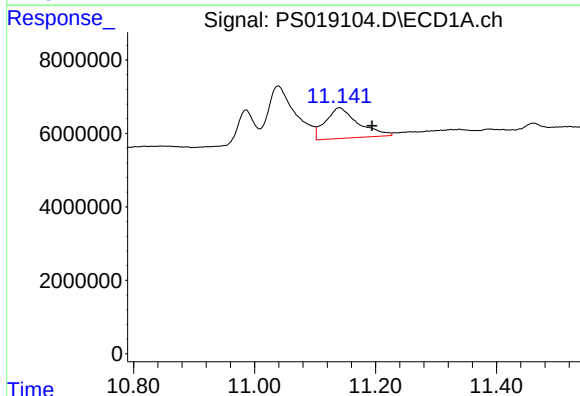


#14 DINOSEB

R.T.: 11.140 min
Delta R.T.: -0.054 min
Response: 31314598
Conc: 2.05 ng/ml

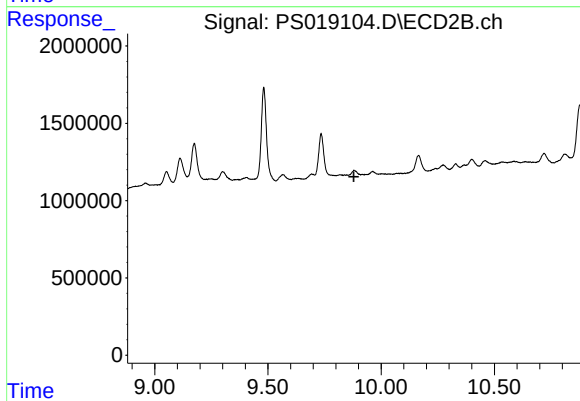


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.880 min
Response: 0
Conc: N.D.

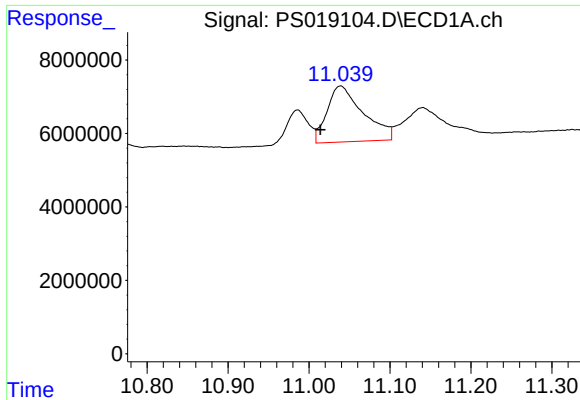


#15 Picloram

R.T.: 11.039 min
Delta R.T.: 0.025 min
Response: 47417164
Conc: 1.77 ng/ml

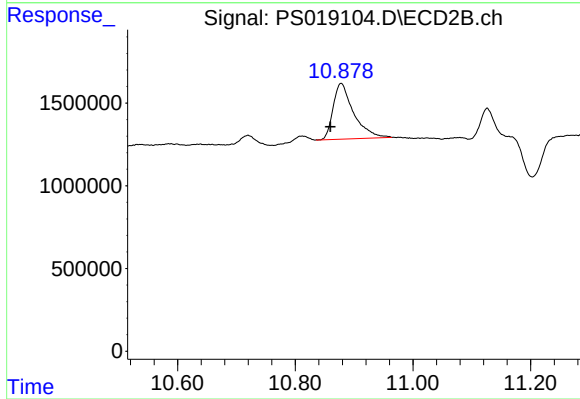


#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.018 min
Response: 8125418
Conc: 1.37 ng/ml

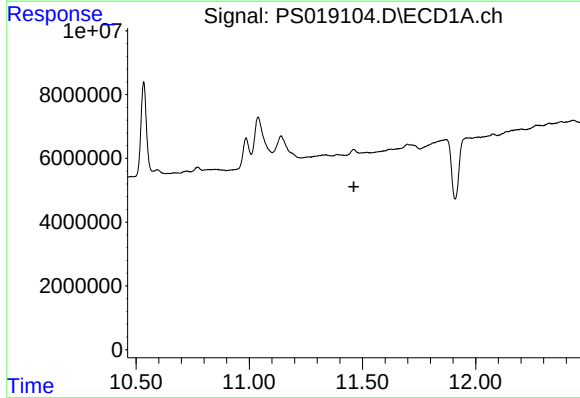

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.462 min
Response: 0
Conc: N.D.

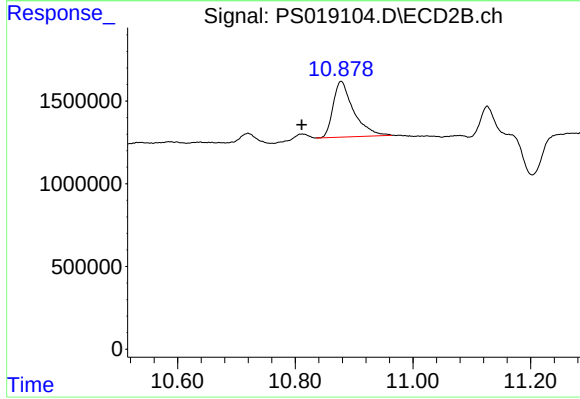

#16 DCPA

R.T.: 10.878 min
Delta R.T.: 0.067 min
Response: 8125418
Conc: 1.42 ng/ml