

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042320AL\
 Data File : FC047063.D
 Signal(s) : FID1A.CH
 Acq On : 24 Apr 2020 3:24
 Operator : DD\AJ
 Sample : L2351-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-20B

Integration File: autoint1.e
 Quant Time: Apr 24 05:46:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 23 16:30:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.171	4321446	48.390 ug/ml
Spiked Amount 50.000		Recovery =	96.78%
Target Compounds			
4) T n-Dodecane (C12)	6.622	290820	2.958 ug/ml
6) T n-Tetradecane (C14)	8.401	458613	4.644 ug/ml
16) T n-Octacosane (C28)	16.971	164352	1.538 ug/ml
17) T n-Tricontane (C30)	17.854	502393	5.021 ug/ml
18) T n-Dotriacontane (C32)	18.679	425372	5.582 ug/ml
19) T n-Tetratriacontane (C34)	19.474	282985	5.036 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042320AL\
Data File : FC047063.D
Signal(s) : FID1A.CH
Acq On : 24 Apr 2020 3:24
Operator : DD\AJ
Sample : L2351-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
TP-20B

Integration File: autoint1.e
Quant Time: Apr 24 05:46:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
Quant Title : GC Extractables
QLast Update : Thu Apr 23 16:30:34 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

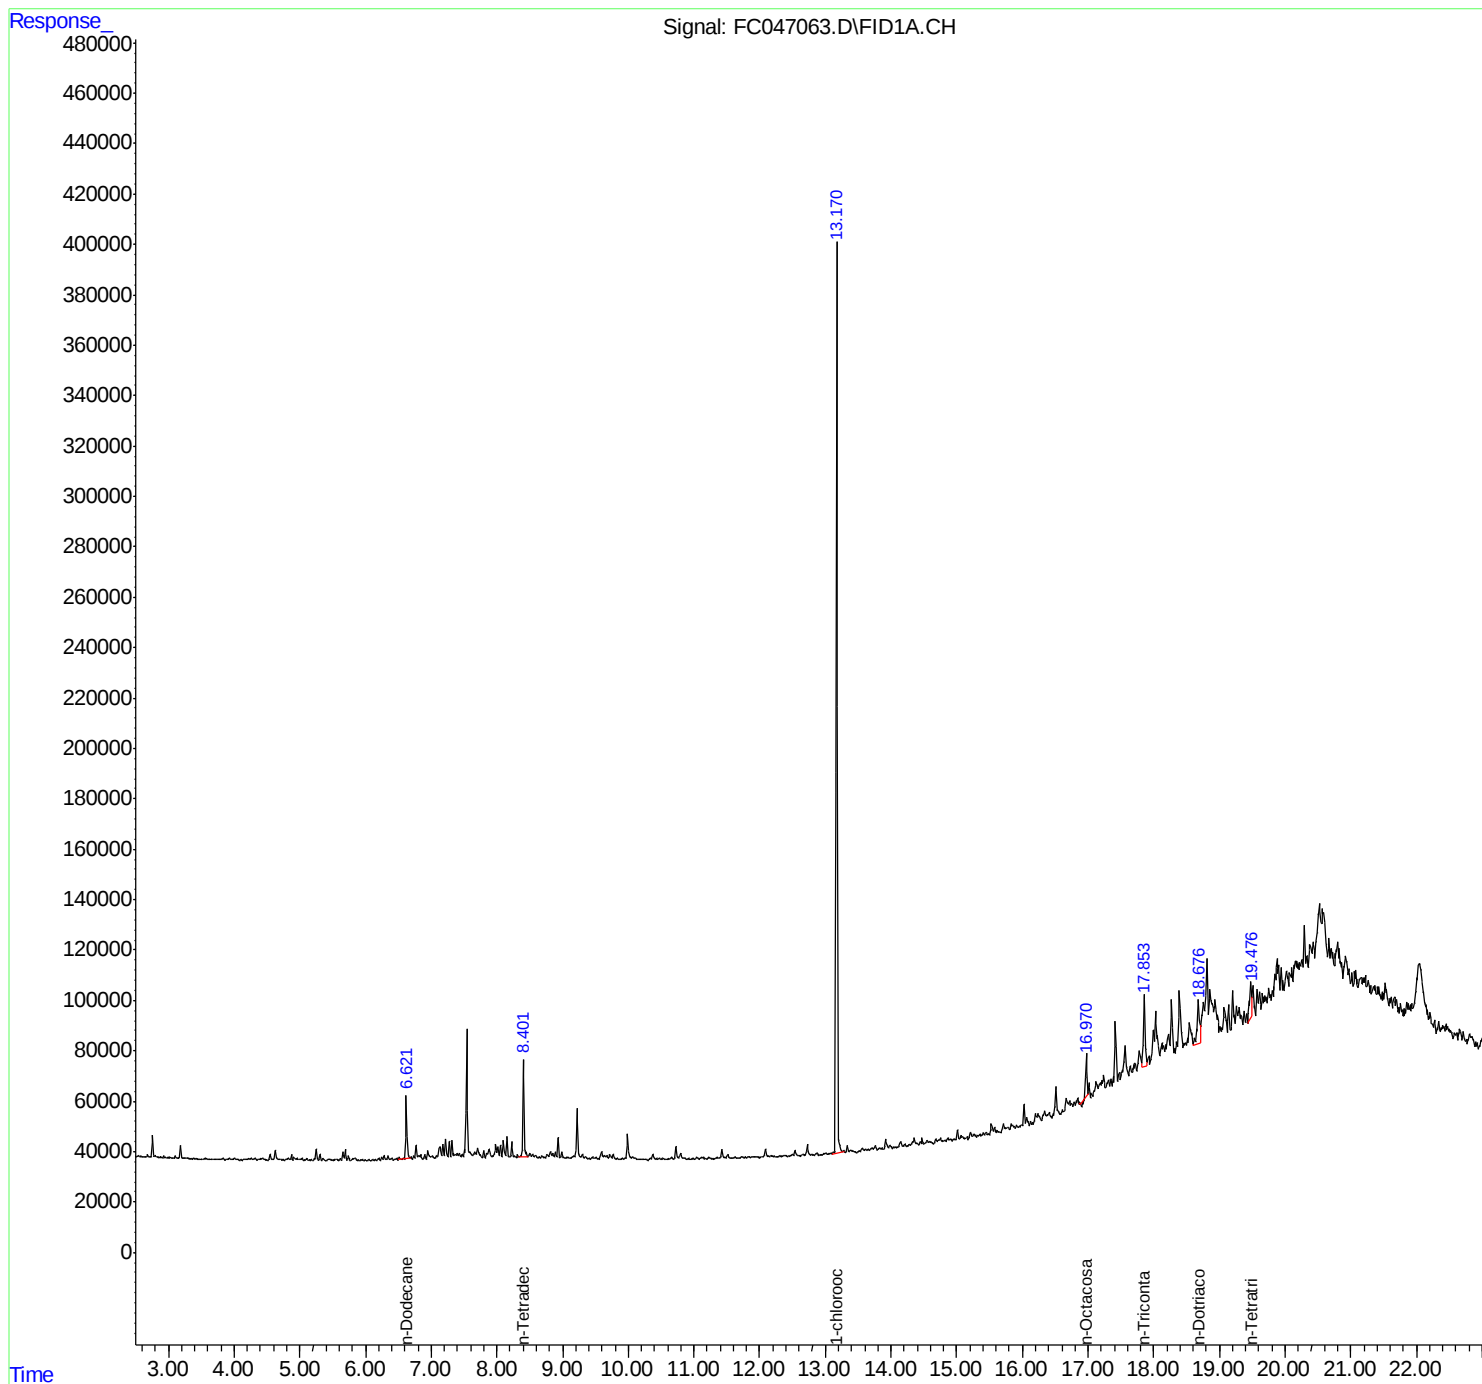


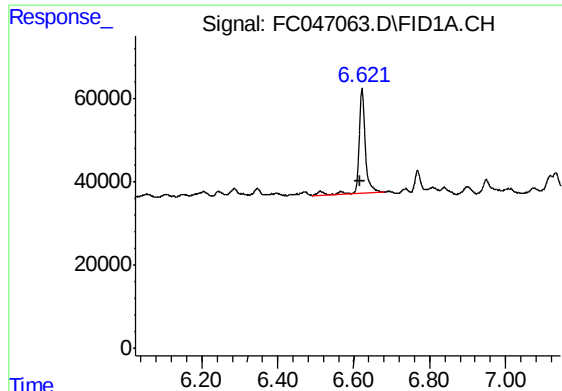

#4 n-Dodecane (C12)


R.T.: 6.622 min
Delta R.T.: 0.004 min
Response: 290820
Conc: 2.96 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-20B

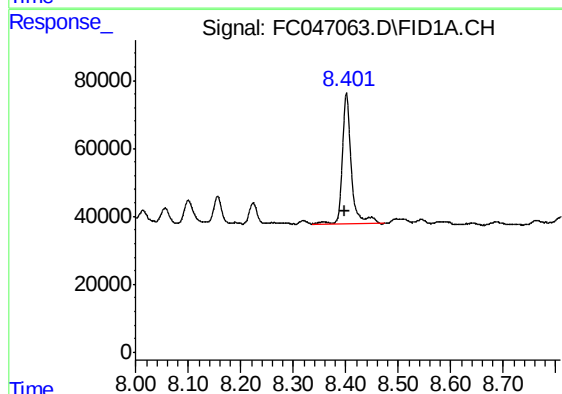


#6 n-Tetradecane (C14)

R.T.: 8.401 min
Delta R.T.: 0.004 min
Response: 458613
Conc: 4.64 ug/ml

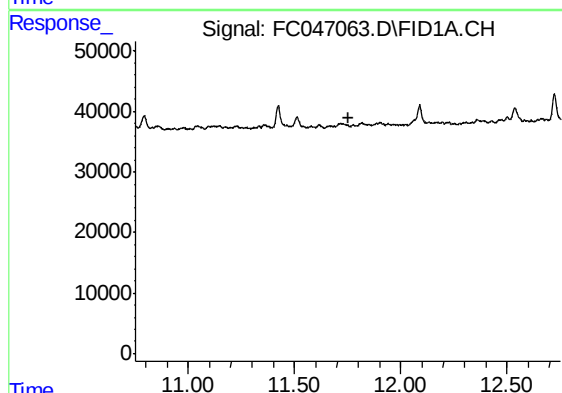


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.751 min
Response: 0
Conc: N.D.

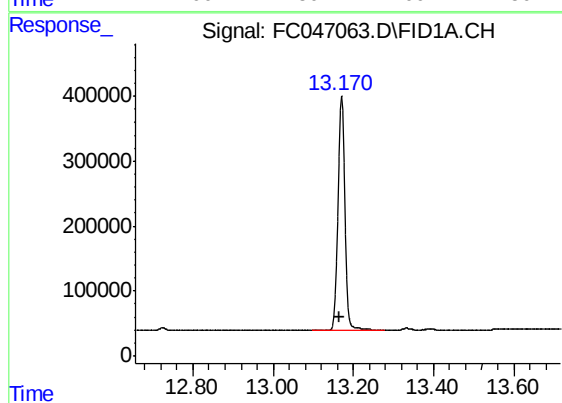

#12 1-chlorooctadecane (SURR)


R.T.: 13.171 min
Delta R.T.: 0.004 min
Response: 4321446
Conc: 48.39 ug/ml

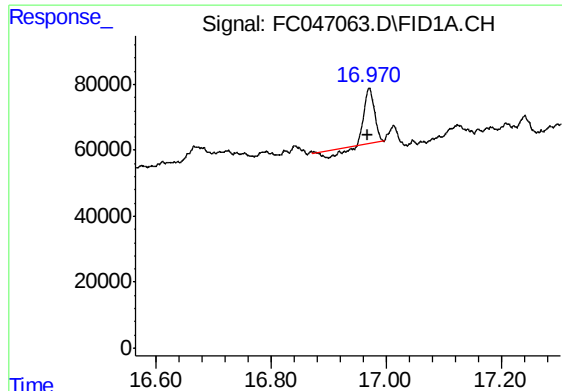

#16 n-Octacosane (C28)


R.T.: 16.971 min
Delta R.T.: 0.004 min
Response: 164352
Conc: 1.54 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-20B

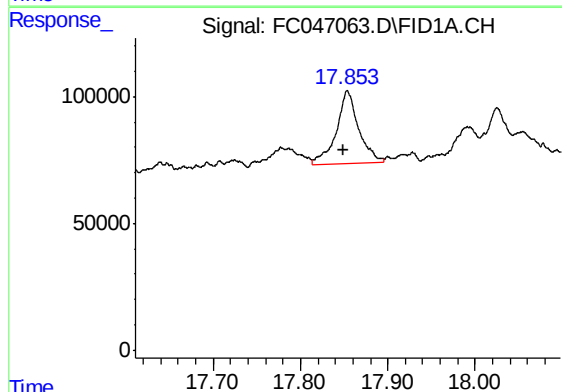


#17 n-Tricontane (C30)

R.T.: 17.854 min
Delta R.T.: 0.004 min
Response: 502393
Conc: 5.02 ug/ml

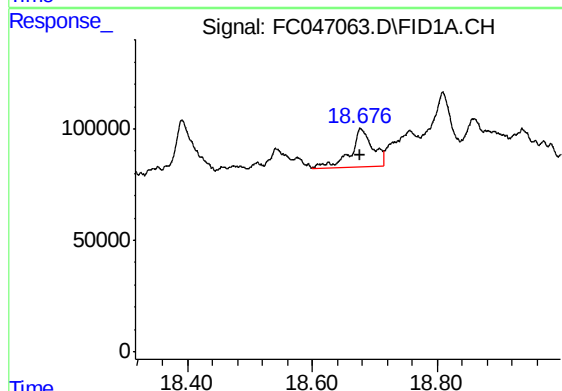

#18 n-Dotriacontane (C32)

R.T.: 18.679 min
Delta R.T.: 0.002 min
Response: 425372
Conc: 5.58 ug/ml

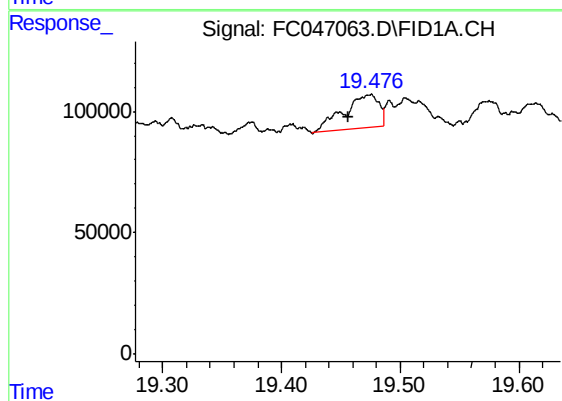

#19 n-Tetratriacontane (C34)

R.T.: 19.474 min
Delta R.T.: 0.018 min
Response: 282985
Conc: 5.04 ug/ml