

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042320AL\
 Data File : FC047085.D
 Signal(s) : FID1A.CH
 Acq On : 24 Apr 2020 17:16
 Operator : DD\AJ
 Sample : L2314-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 WB-8-2

Integration File: autoint1.e
 Quant Time: Apr 25 00:46:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 23 16:30:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.170	3000770	33.601 ug/ml
Spiked Amount 50.000		Recovery =	67.20%
Target Compounds			
13) T n-Docosane (C22)	13.914	167251	1.572 ug/ml
14) T n-Tetracosane (C24)	15.010	202883	1.887 ug/ml
15) T n-Hexacosane (C26)	16.025	321909	2.984 ug/ml
16) T n-Octacosane (C28)	16.971	433982	4.060 ug/ml
17) T n-Tricontane (C30)	17.853	418800	4.185 ug/ml
18) T n-Dotriacontane (C32)	18.679	238381	3.128 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042320AL\
Data File : FC047085.D
Signal(s) : FID1A.CH
Acq On : 24 Apr 2020 17:16
Operator : DD\AJ
Sample : L2314-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
WB-8-2

Integration File: autoint1.e
Quant Time: Apr 25 00:46:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
Quant Title : GC Extractables
QLast Update : Thu Apr 23 16:30:34 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

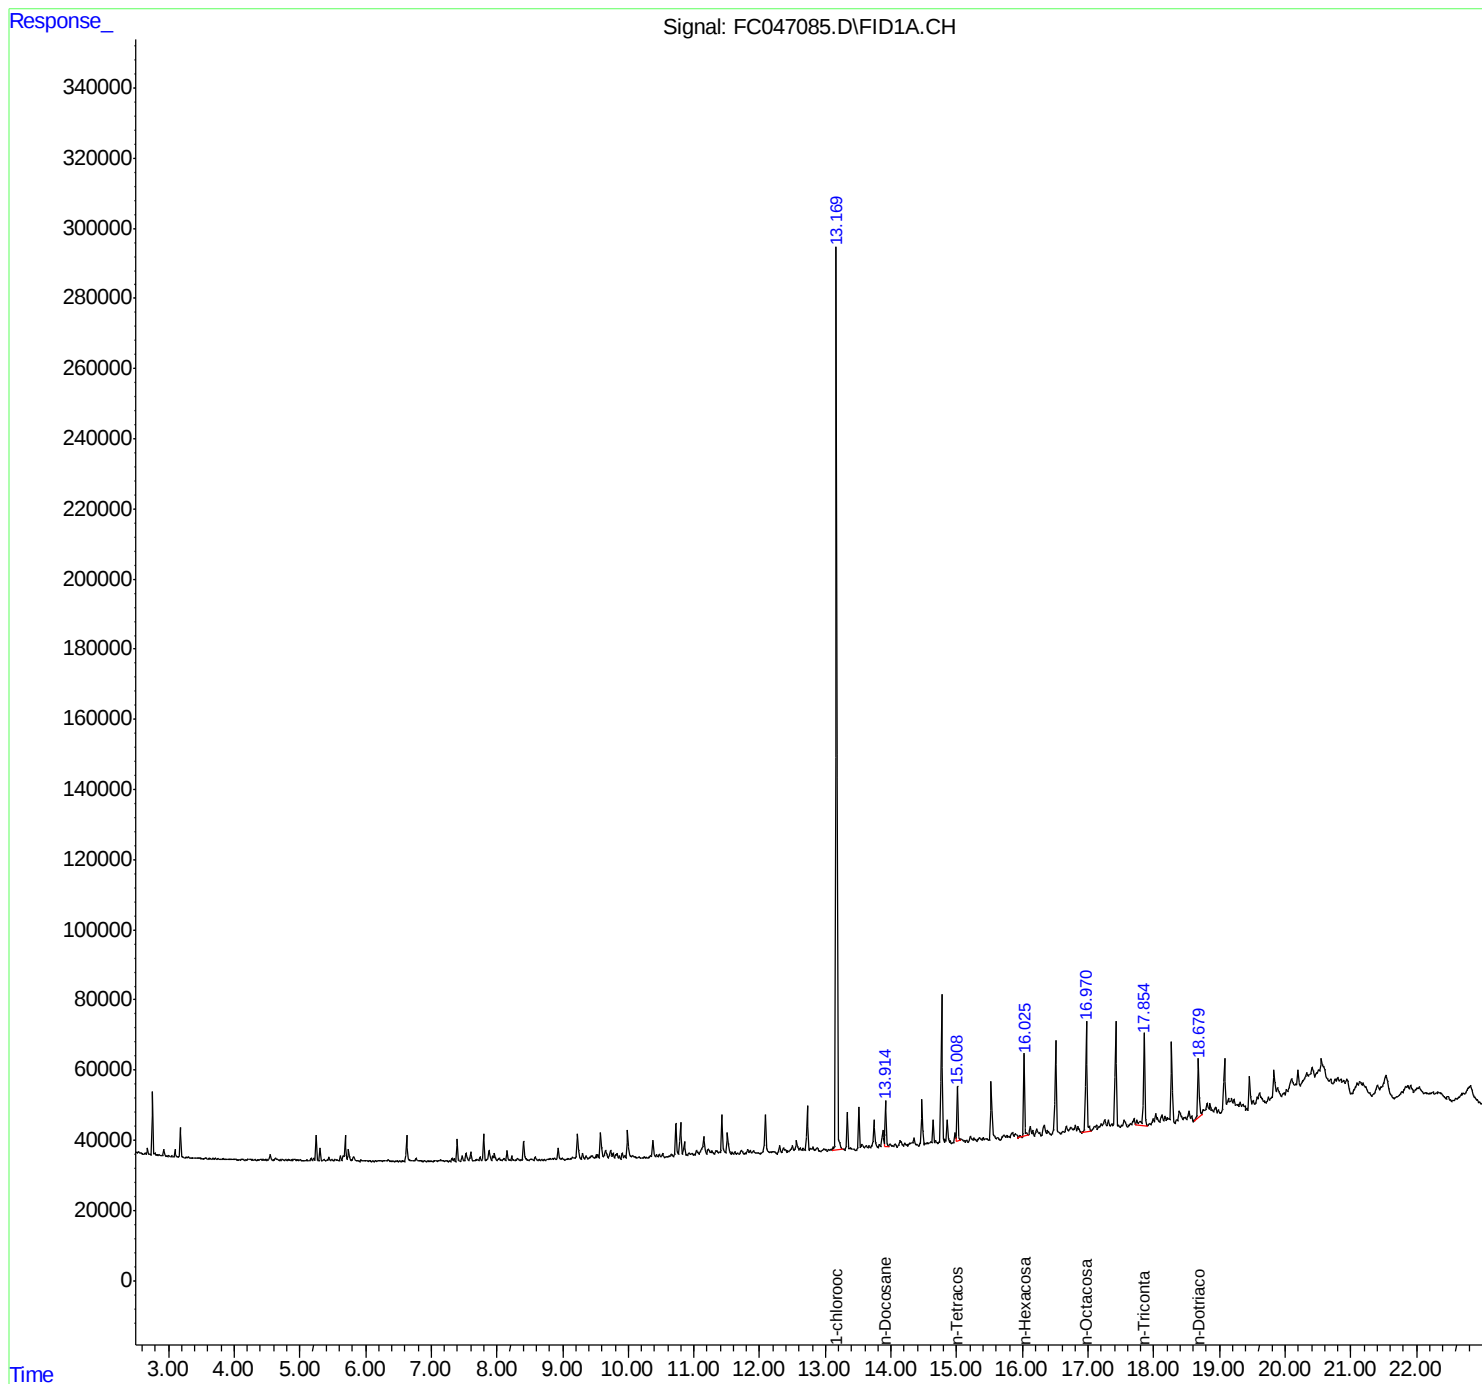


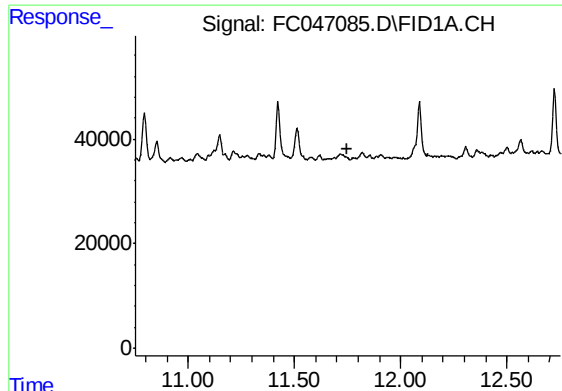

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.751 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
WB-8-2

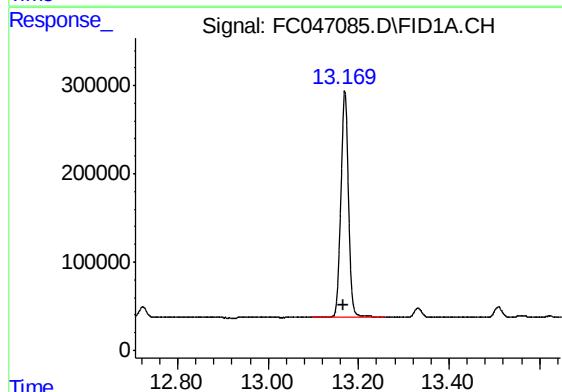


#12 1-chlorooctadecane (SURR)

R.T.: 13.170 min
Delta R.T.: 0.003 min
Response: 3000770
Conc: 33.60 ug/ml

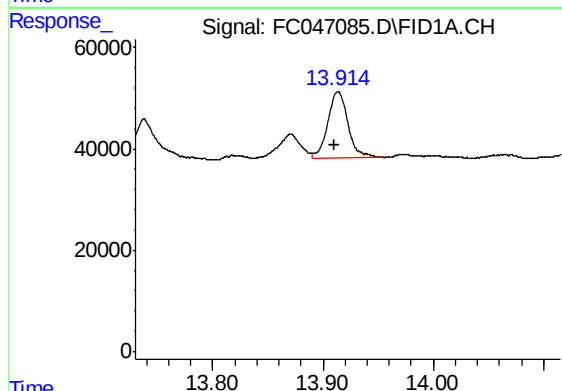


#13 n-Docosane (C22)

R.T.: 13.914 min
Delta R.T.: 0.003 min
Response: 167251
Conc: 1.57 ug/ml

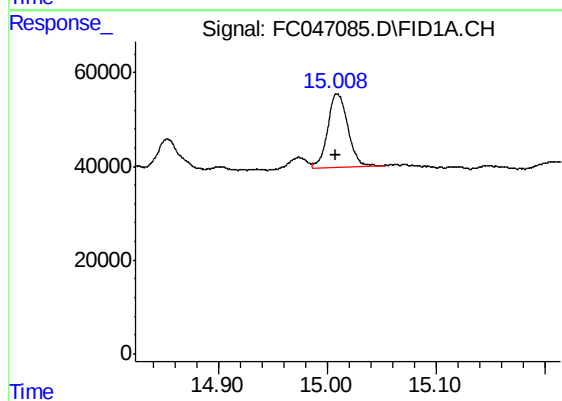

#14 n-Tetracosane (C24)


R.T.: 15.010 min
Delta R.T.: 0.002 min
Response: 202883
Conc: 1.89 ug/ml

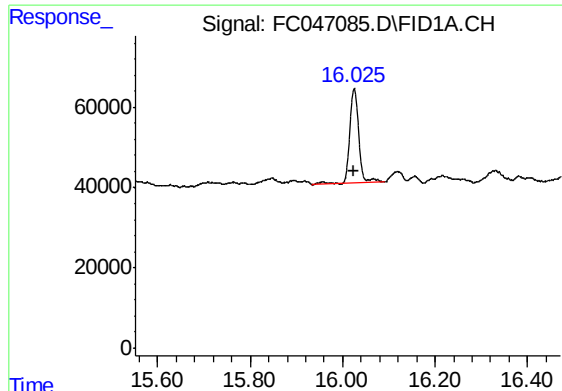

#15 n-Hexacosane (C26)


R.T.: 16.025 min
Delta R.T.: 0.002 min
Response: 321909
Conc: 2.98 ug/ml

Instrument :
FID_C
ClientSampleId :
WB-8-2

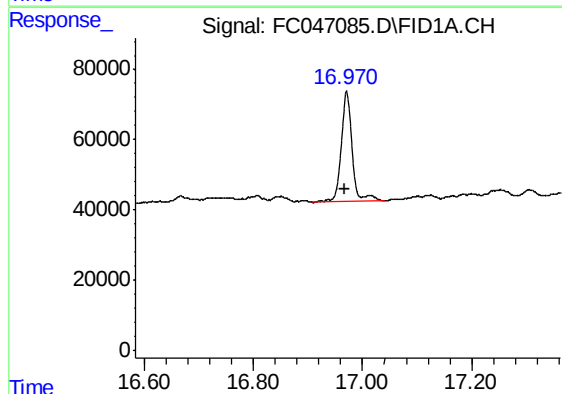


#16 n-Octacosane (C28)

R.T.: 16.971 min
Delta R.T.: 0.004 min
Response: 433982
Conc: 4.06 ug/ml

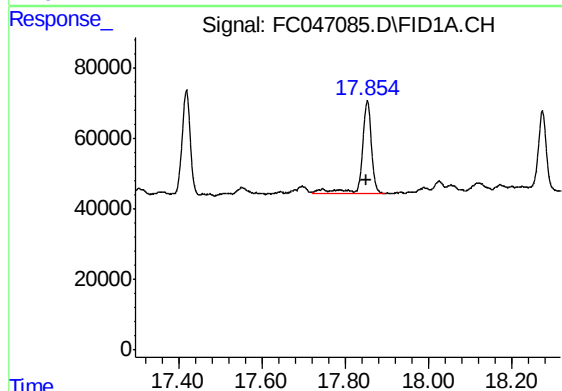

#17 n-Tricontane (C30)

R.T.: 17.853 min
Delta R.T.: 0.003 min
Response: 418800
Conc: 4.19 ug/ml

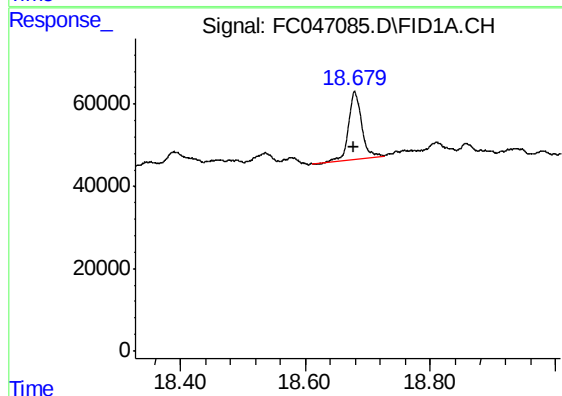

#18 n-Dotriacontane (C32)

R.T.: 18.679 min
Delta R.T.: 0.002 min
Response: 238381
Conc: 3.13 ug/ml