

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042420AL\
 Data File : FC047114.D
 Signal(s) : FID1A.CH
 Acq On : 25 Apr 2020 23:13
 Operator : DD\AJ
 Sample : L2376-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-8

Integration File: autoint1.e
 Quant Time: Apr 27 00:47:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 23 16:30:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.753	2574814	23.139 ug/ml
Spiked Amount 50.000		Recovery =	46.28%
12) S 1-chlorooctadecane (S...	13.168	1878211	21.031 ug/ml
Spiked Amount 50.000		Recovery =	42.06%
Target Compounds			
14) T n-Tetracosane (C24)	15.008	256789	2.388 ug/ml
16) T n-Octacosane (C28)	16.966	545786	5.106 ug/ml
17) T n-Tricontane (C30)	17.851	467665	4.674 ug/ml
18) T n-Dotriacontane (C32)	18.679	337841	4.434 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042420AL\
Data File : FC047114.D
Signal(s) : FID1A.CH
Acq On : 25 Apr 2020 23:13
Operator : DD\AJ
Sample : L2376-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
TP-8

Integration File: autoint1.e
Quant Time: Apr 27 00:47:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
Quant Title : GC Extractables
QLast Update : Thu Apr 23 16:30:34 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

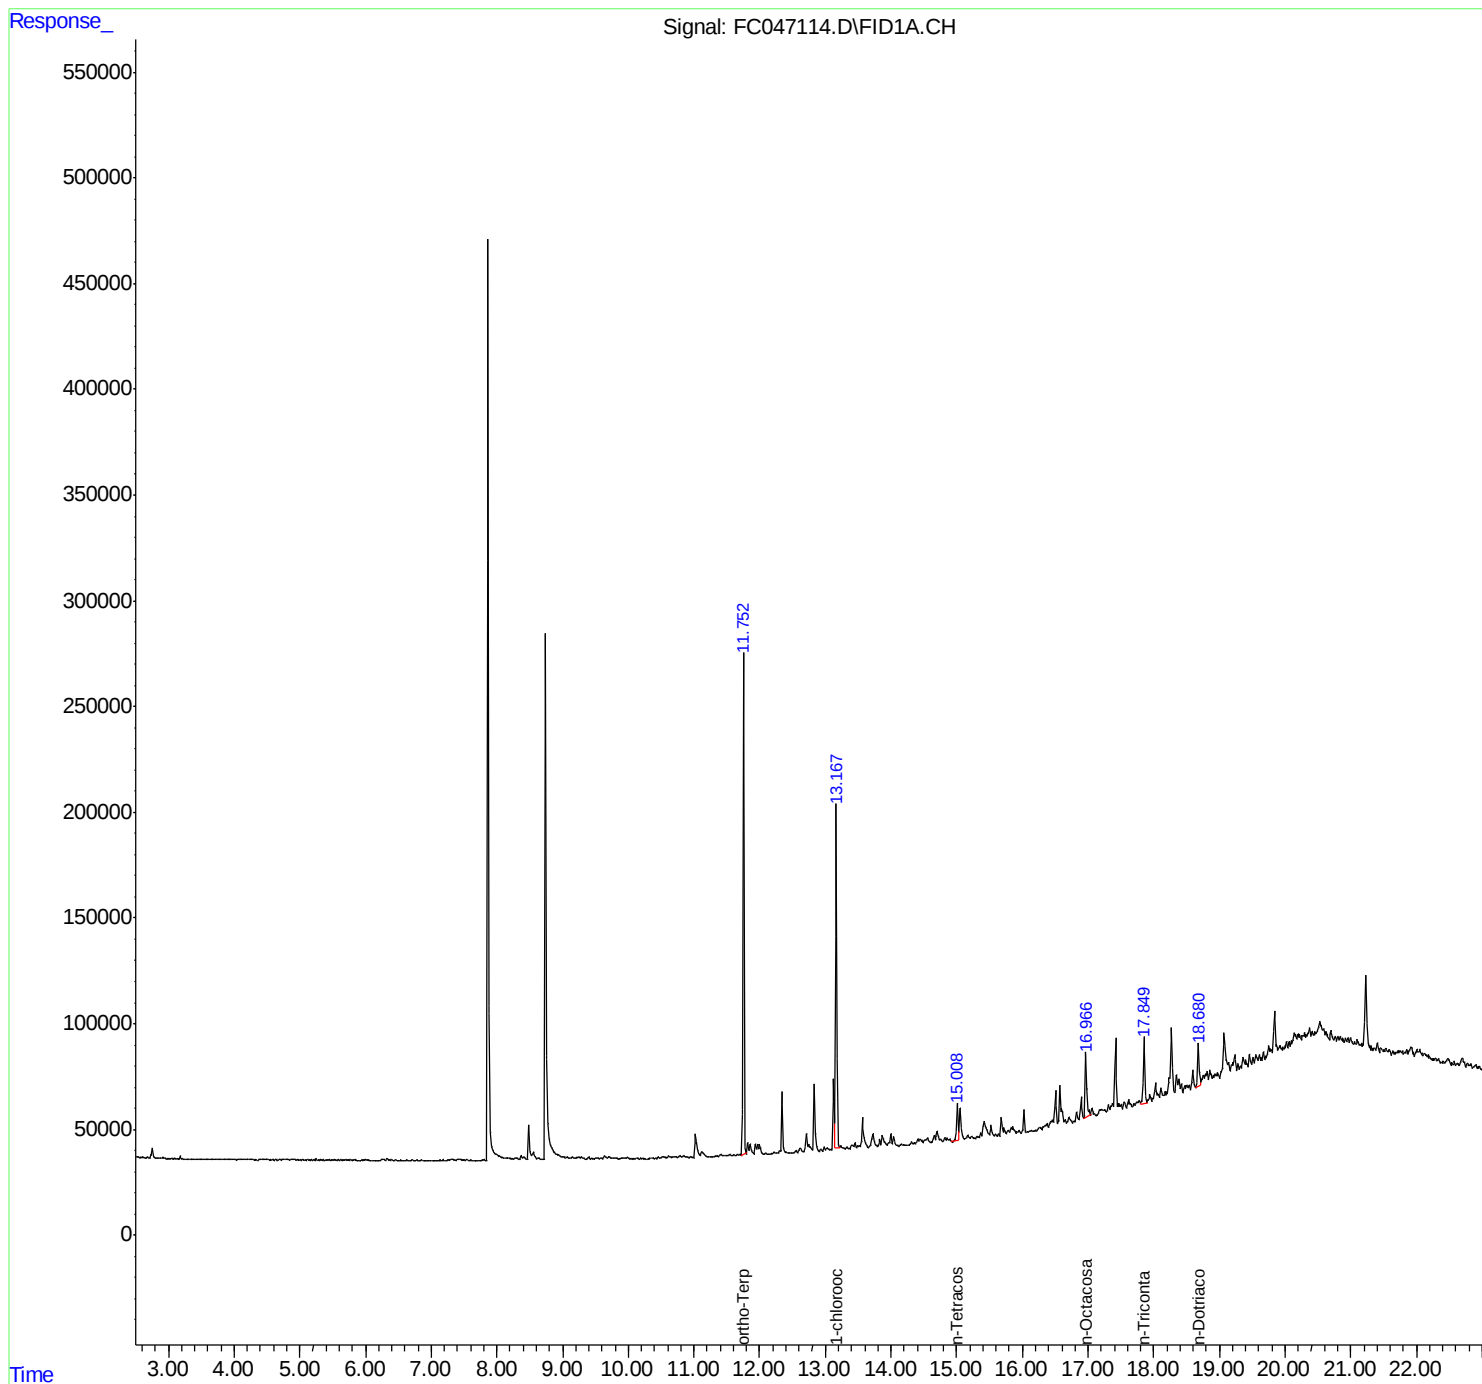


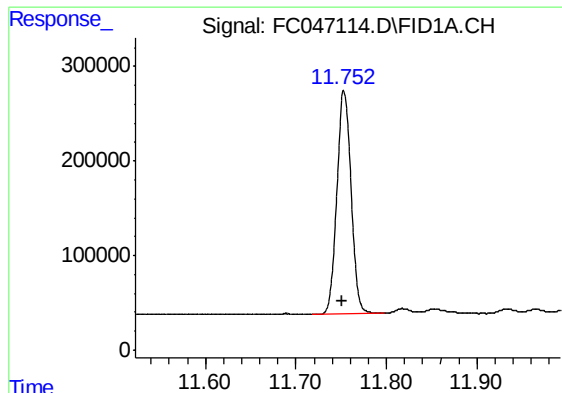

#9 ortho-Terphenyl (SURR)


R.T.: 11.753 min
Delta R.T.: 0.002 min
Response: 2574814
Conc: 23.14 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-8

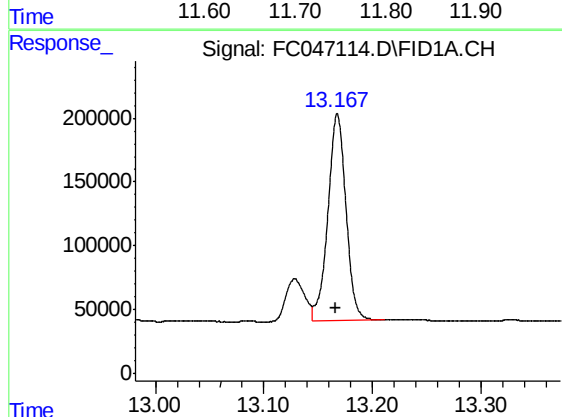


#12 1-chlorooctadecane (SURR)

R.T.: 13.168 min
Delta R.T.: 0.001 min
Response: 1878211
Conc: 21.03 ug/ml

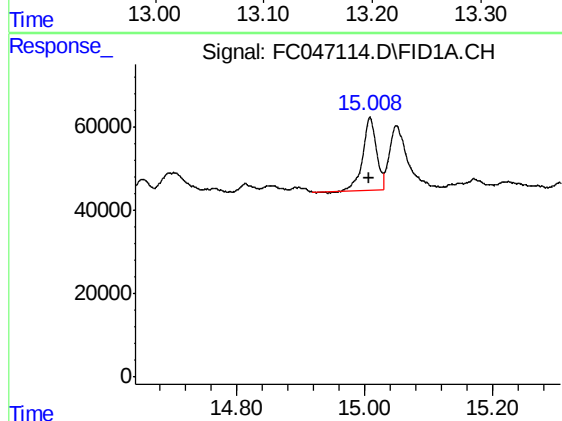


#14 n-Tetracosane (C24)

R.T.: 15.008 min
Delta R.T.: 0.000 min
Response: 256789
Conc: 2.39 ug/ml

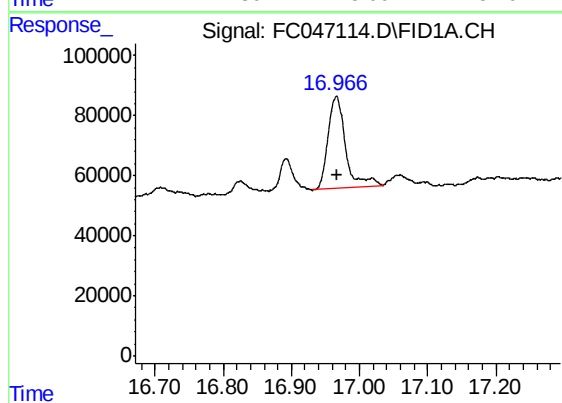

#16 n-Octacosane (C28)


R.T.: 16.966 min
Delta R.T.: -0.001 min
Response: 545786
Conc: 5.11 ug/ml

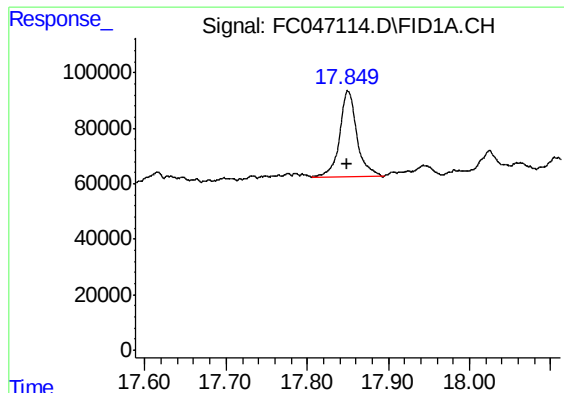

#17 n-Tricontane (C30)

R.T.: 17.851 min
Delta R.T.: 0.000 min
Response: 467665
Conc: 4.67 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-8

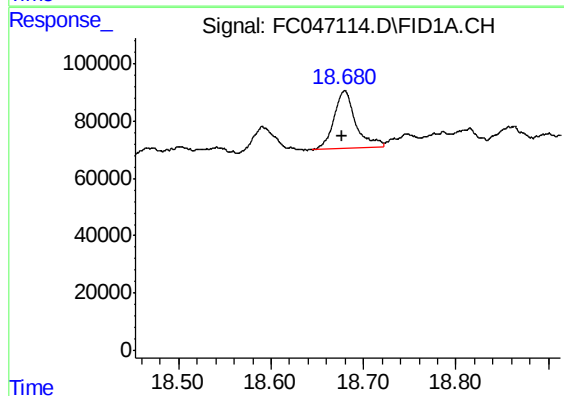

#18 n-Dotriacontane (C32)

R.T.: 18.679 min
Delta R.T.: 0.003 min
Response: 337841
Conc: 4.43 ug/ml