

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042420AL\
 Data File : FC047116.D
 Signal(s) : FID1A.CH
 Acq On : 26 Apr 2020 00:27
 Operator : DD\AJ
 Sample : L2376-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-10

Integration File: autoint1.e
 Quant Time: Apr 27 00:47:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 23 16:30:34 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.754	2209684	19.858 ug/ml
Spiked Amount 50.000		Recovery =	39.72%
12) S 1-chlorooctadecane (S...	13.169	1606457	17.988 ug/ml
Spiked Amount 50.000		Recovery =	35.98%
Target Compounds			
14) T n-Tetracosane (C24)	15.005	374232	3.480 ug/ml
16) T n-Octacosane (C28)	16.963	605766	5.667 ug/ml
17) T n-Tricontane (C30)	17.850	325857	3.256 ug/ml
18) T n-Dotriacontane (C32)	18.677	247591	3.249 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042420AL\
Data File : FC047116.D
Signal(s) : FID1A.CH
Acq On : 26 Apr 2020 00:27
Operator : DD\AJ
Sample : L2376-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :
TP-10

Integration File: autoint1.e
Quant Time: Apr 27 00:47:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042320.M
Quant Title : GC Extractables
QLast Update : Thu Apr 23 16:30:34 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

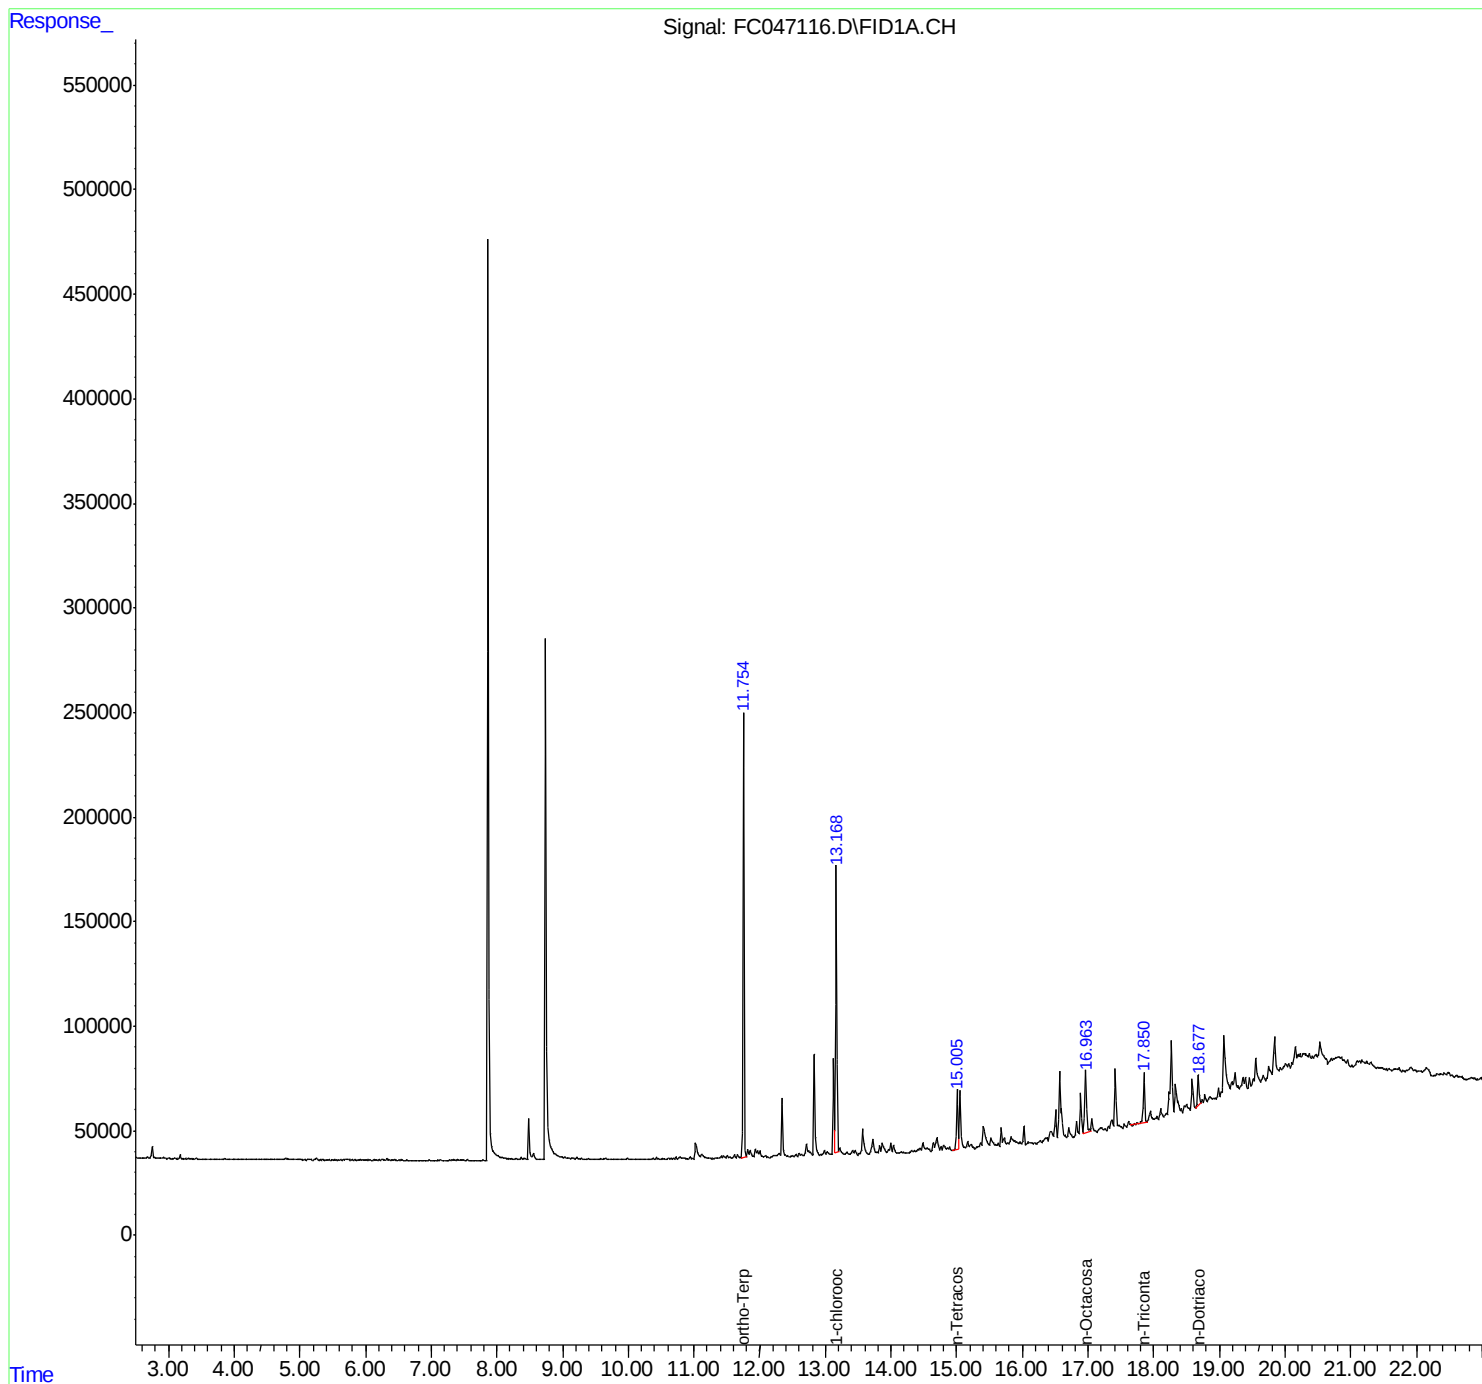


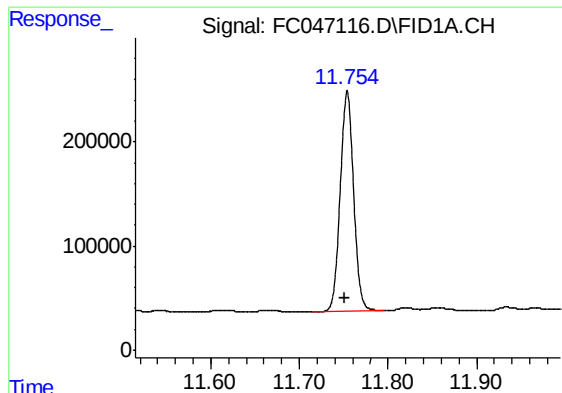

#9 ortho-Terphenyl (SURR)


R.T.: 11.754 min
Delta R.T.: 0.003 min
Response: 2209684
Conc: 19.86 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-10

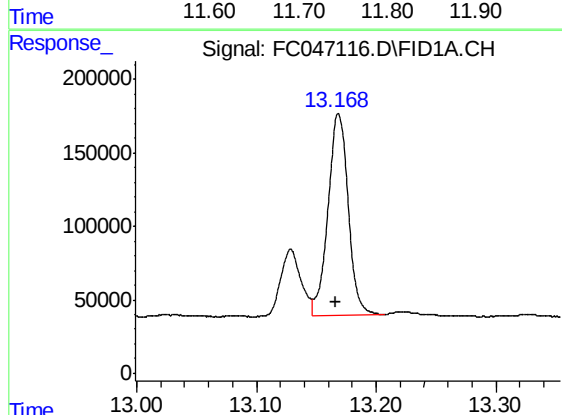


#12 1-chlorooctadecane (SURR)

R.T.: 13.169 min
Delta R.T.: 0.002 min
Response: 1606457
Conc: 17.99 ug/ml

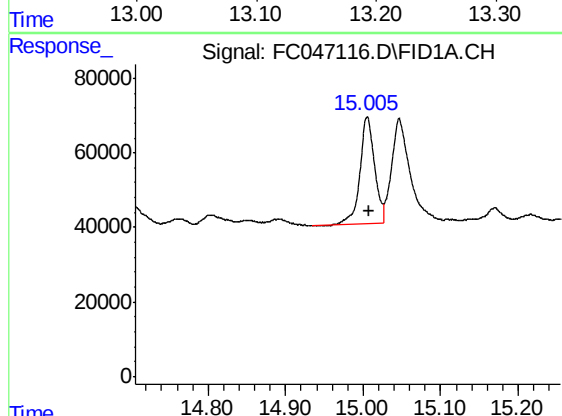


#14 n-Tetracosane (C24)

R.T.: 15.005 min
Delta R.T.: -0.002 min
Response: 374232
Conc: 3.48 ug/ml

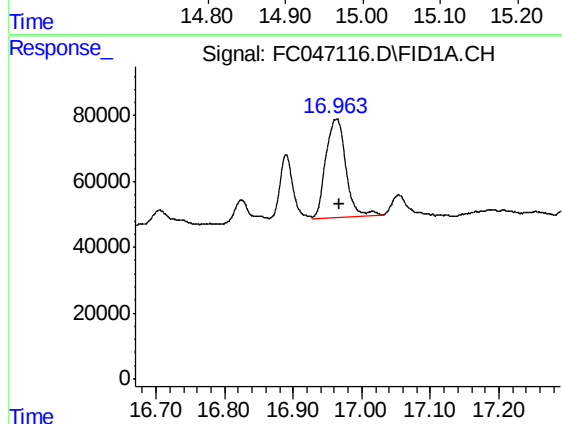

#16 n-Octacosane (C28)


R.T.: 16.963 min
Delta R.T.: -0.004 min
Response: 605766
Conc: 5.67 ug/ml

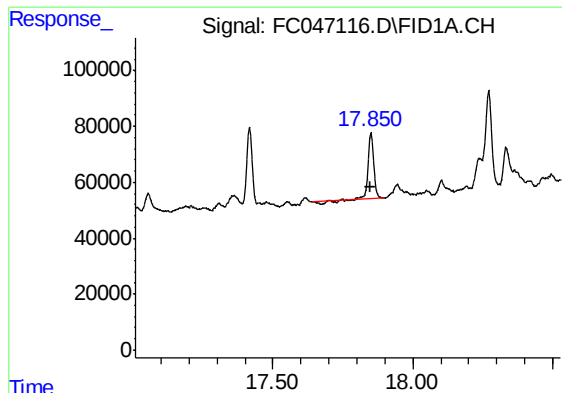

#17 n-Tricontane (C30)

R.T.: 17.850 min
Delta R.T.: 0.000 min
Response: 325857
Conc: 3.26 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-10

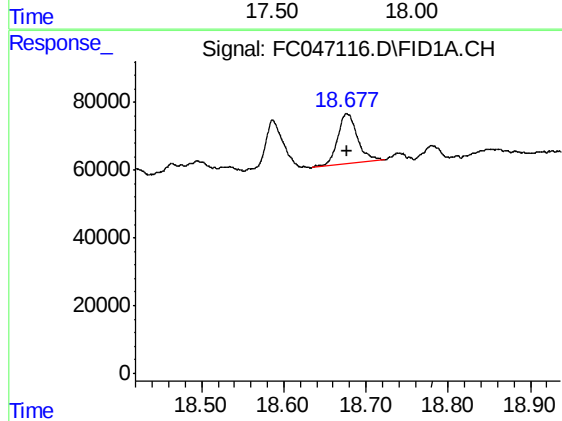

#18 n-Dotriacontane (C32)

R.T.: 18.677 min
Delta R.T.: 0.000 min
Response: 247591
Conc: 3.25 ug/ml