

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042522AL\
 Data File : FC059421.D
 Signal(s) : FID1A.CH
 Acq On : 26 Apr 2022 2:21
 Operator : UA/NP
 Sample : N2548-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 26 06:10:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 042122.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 17:30:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.101	5225682	32.520 ug/ml
Spiked Amount 50.000		Recovery =	65.04%
12) S 1-chlorooctadecane (S...	12.547	4429432	33.920 ug/ml
Spiked Amount 50.000		Recovery =	67.84%
Target Compounds			
10) T n-Eicosane (C20)	12.137	1534802	10.234 ug/ml
11) T n-Heneicosane (C21)	12.771f	123150	0.810 ug/ml
13) T n-Docosane (C22)	13.301	92885	0.606 ug/ml
14) T n-Tetracosane (C24)	14.357	338850	2.188 ug/ml
17) T n-Tricontane (C30)	17.238	93586	0.616 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042522AL\
Data File : FC059421.D
Signal(s) : FID1A.CH
Acq On : 26 Apr 2022 2:21
Operator : UA/NP
Sample : N2548-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 26 06:10:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 042122.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 17:30:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

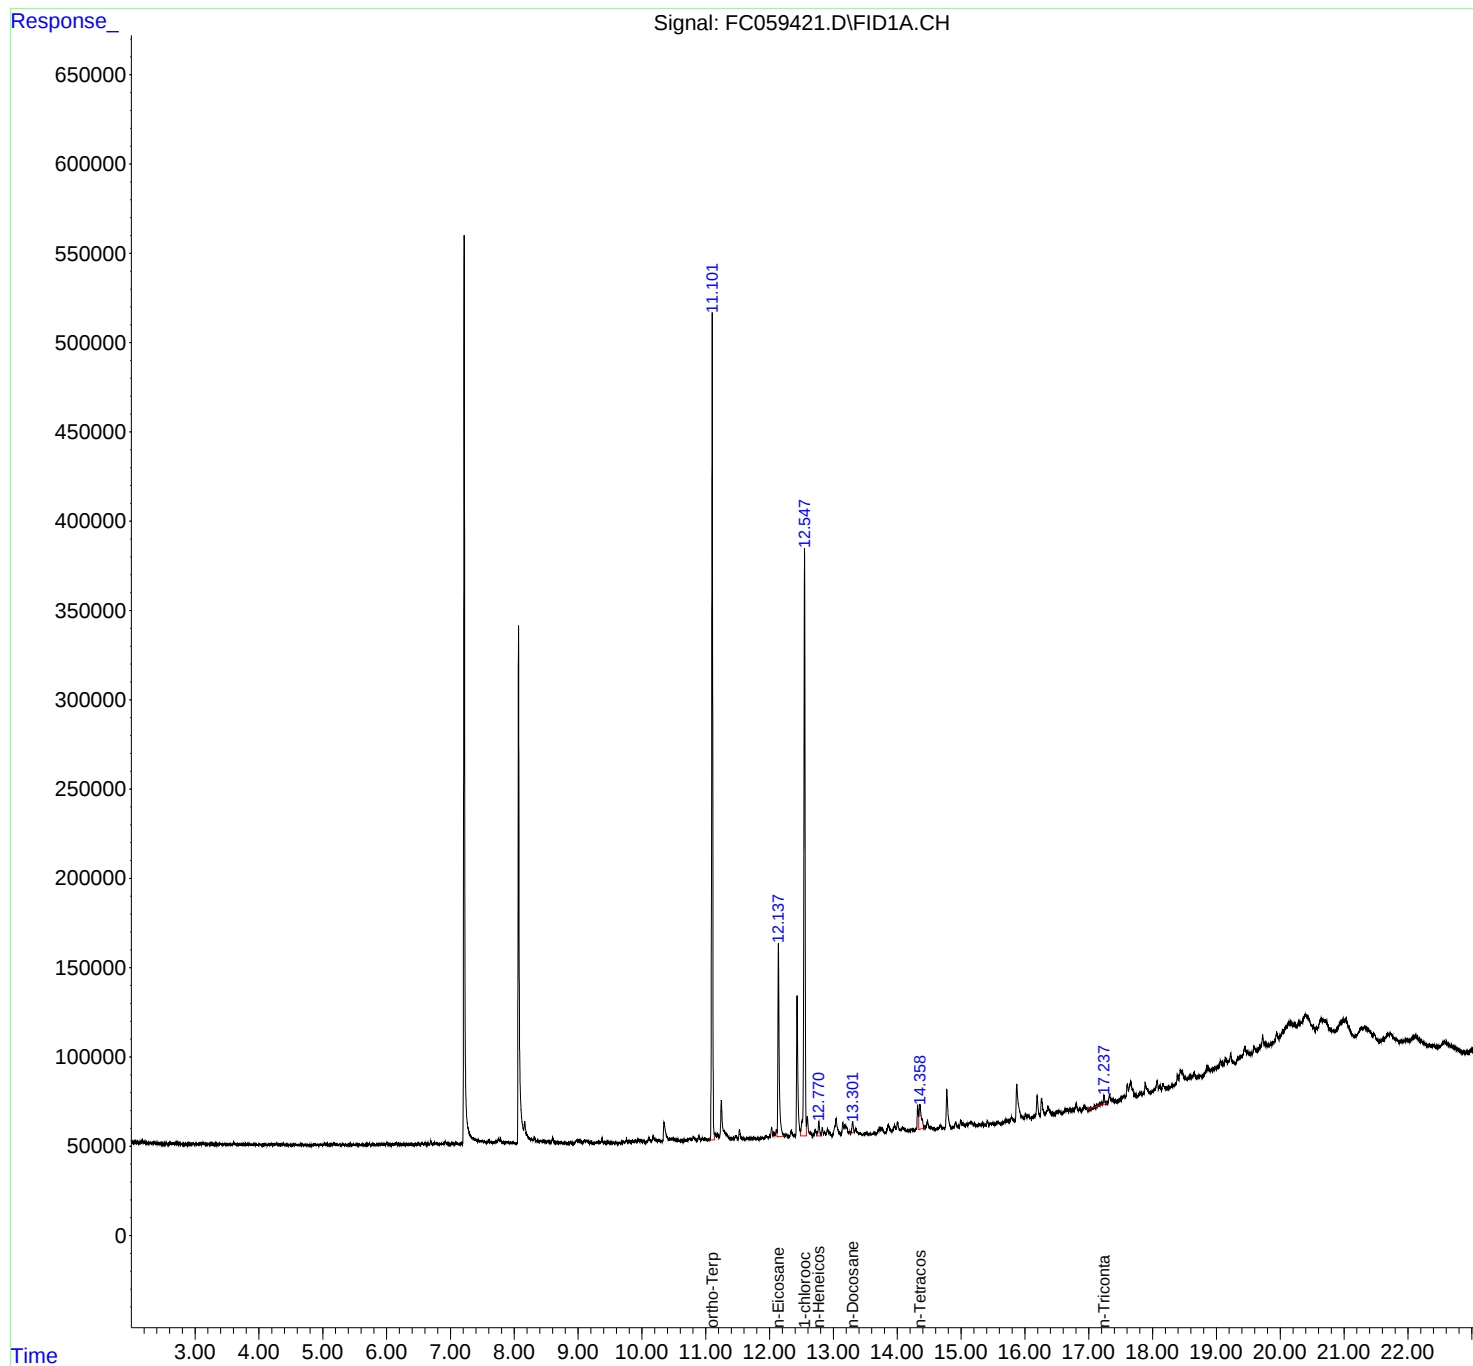


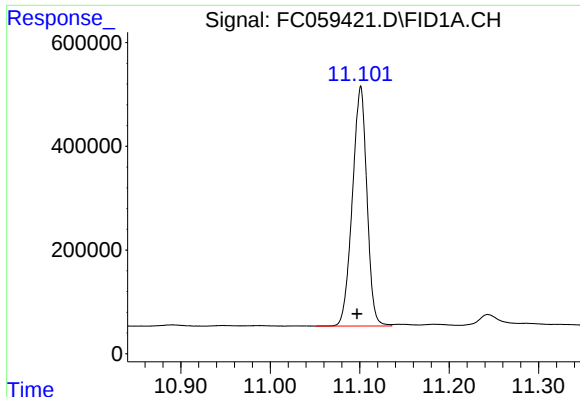

#9 ortho-Terphenyl (SURR)


R.T.: 11.101 min
Delta R.T.: 0.004 min
Response: 5225682
Conc: 32.52 ug/ml

Instrument :
FID_C
ClientSampleId :

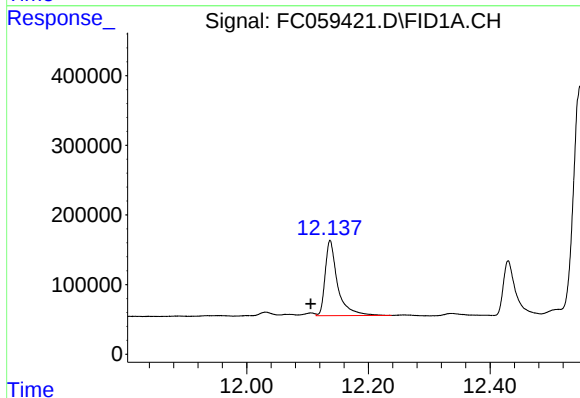


#10 n-Eicosane (C20)

R.T.: 12.137 min
Delta R.T.: 0.032 min
Response: 1534802
Conc: 10.23 ug/ml

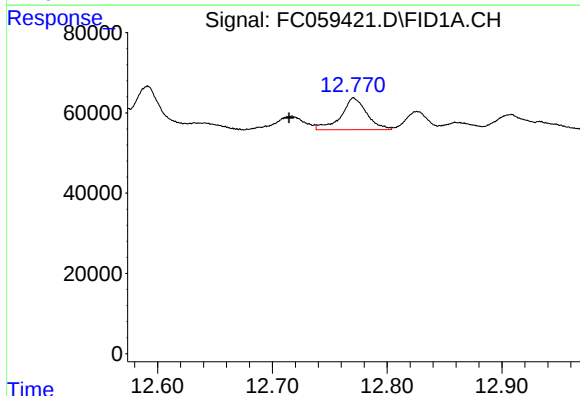


#11 n-Heneicosane (C21)

R.T.: 12.771 min
Delta R.T.: 0.057 min
Response: 123150
Conc: 0.81 ug/ml

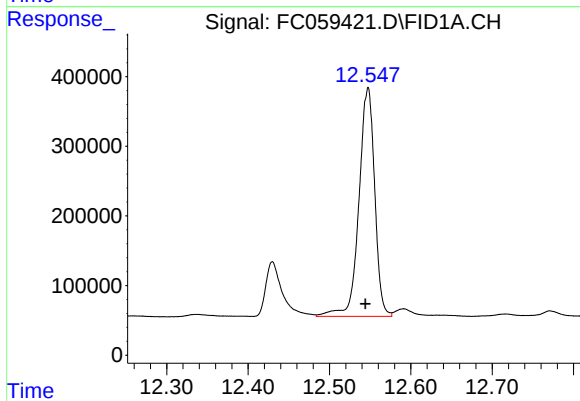

#12 1-chlorooctadecane (SURR)


R.T.: 12.547 min
Delta R.T.: 0.003 min
Response: 4429432
Conc: 33.92 ug/ml

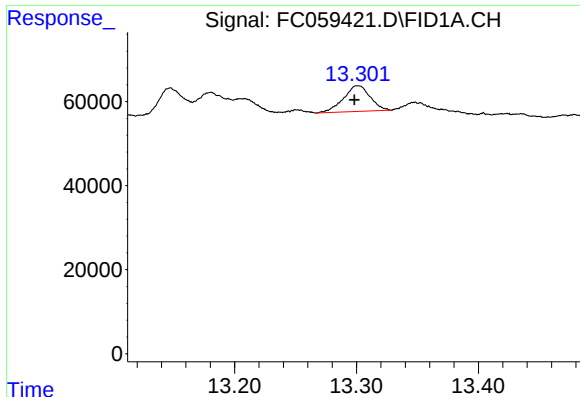

#13 n-Docosane (C22)


R.T.: 13.301 min
Delta R.T.: 0.003 min
Response: 92885
Conc: 0.61 ug/ml

Instrument :
FID_C
ClientSampleId :

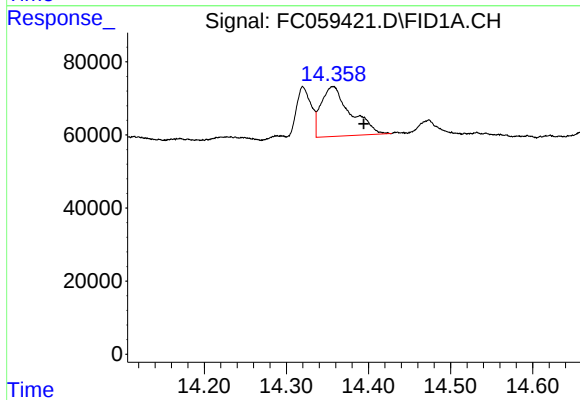

#14 n-Tetracosane (C24)

R.T.: 14.357 min
Delta R.T.: -0.038 min
Response: 338850
Conc: 2.19 ug/ml

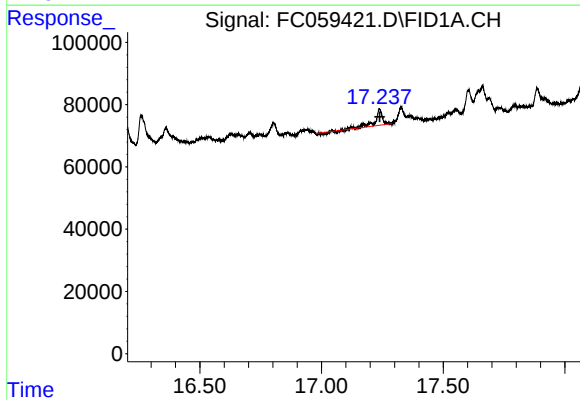

#17 n-Tricontane (C30)

R.T.: 17.238 min
Delta R.T.: 0.000 min
Response: 93586
Conc: 0.62 ug/ml