

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042621AL\
 Data File : FC053389.D
 Signal(s) : FID1A.CH
 Acq On : 26 Apr 2021 9:58
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 26 13:15:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042021.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 21 11:02:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	17.726	199093	1.478 ug/ml
18) T n-Dotriacontane (C32)	18.561	103608	0.755 ug/ml
19) T n-Tetratriacontane (C34)	19.345	586784	4.497 ug/ml
20) T n-Hexatriacontane (C36)	20.110	1627473	13.442 ug/ml
21) T n-Octatriacontane (C38)	20.772	4679550	44.410 ug/ml
22) T n-Tetracontane (C40)	21.670	2251087	21.500 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042621AL\
Data File : FC053389.D
Signal(s) : FID1A.CH
Acq On : 26 Apr 2021 9:58
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :

Integration File: autoint1.e
Quant Time: Apr 26 13:15:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042021.M
Quant Title : GC Extractables
QLast Update : Wed Apr 21 11:02:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

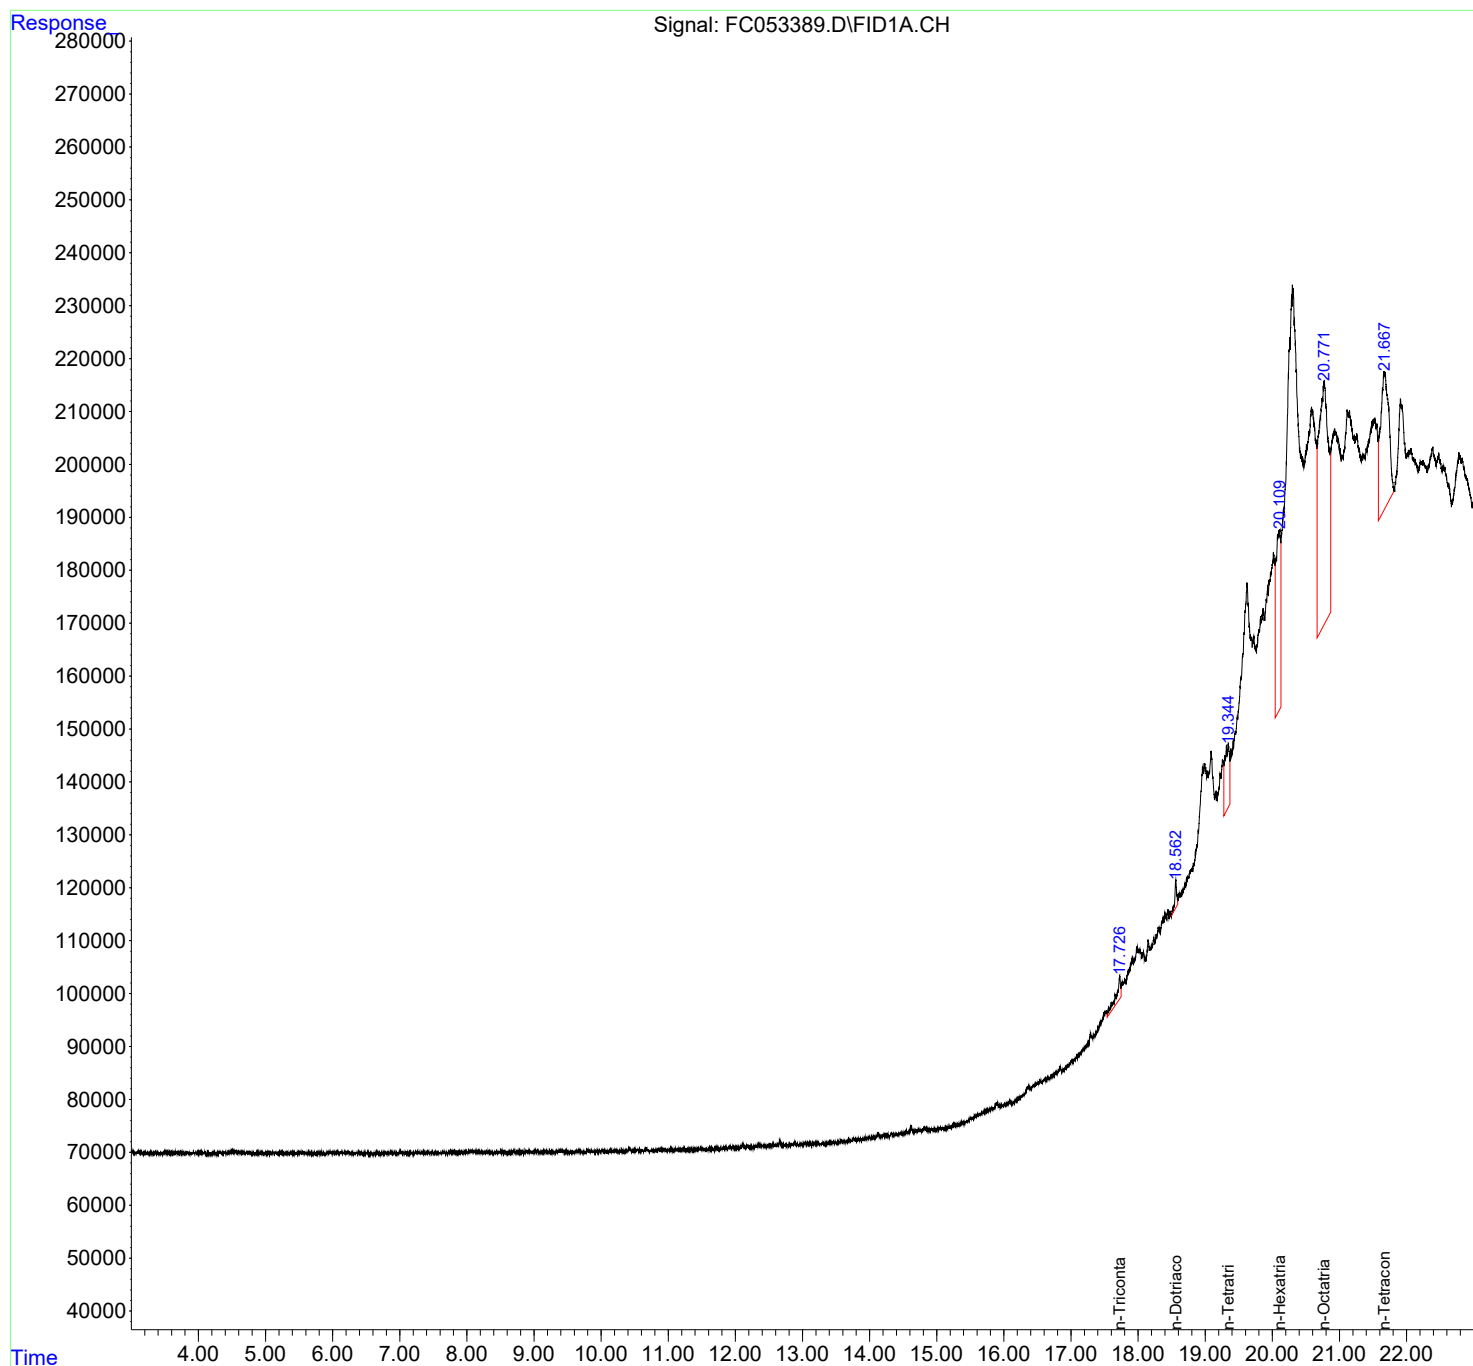


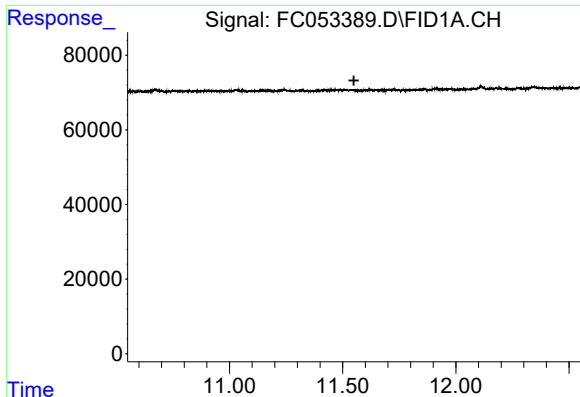

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.550 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

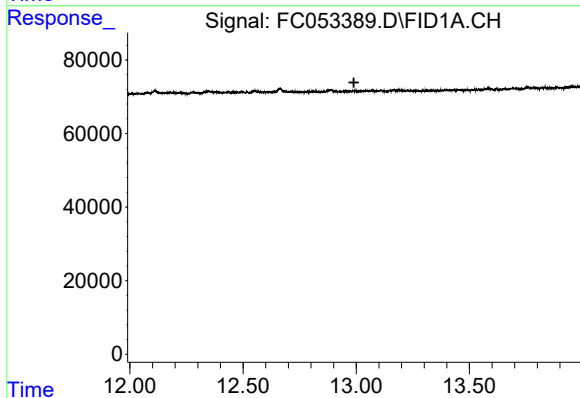


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.990 min
Response: 0
Conc: N.D.

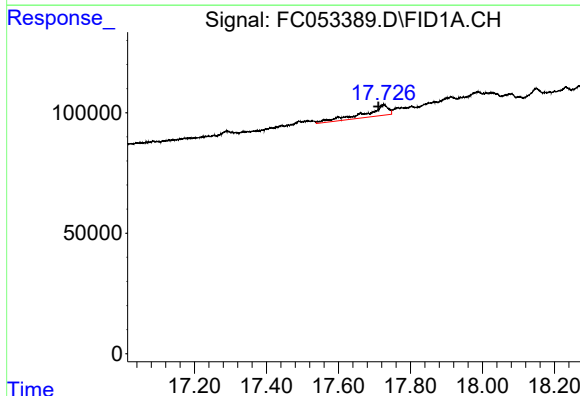


#17 n-Tricontane (C30)

R.T.: 17.726 min
Delta R.T.: 0.015 min
Response: 199093
Conc: 1.48 ug/ml

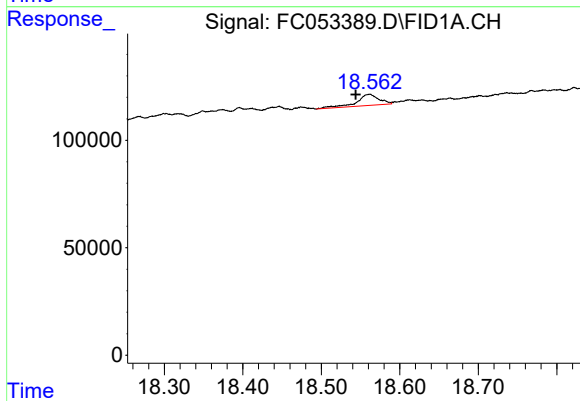

#18 n-Dotriacontane (C32)


R.T.: 18.561 min
Delta R.T.: 0.017 min
Response: 103608
Conc: 0.76 ug/ml

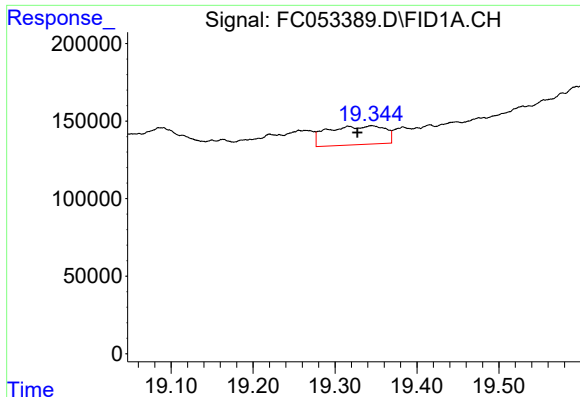

#19 n-Tetratriacontane (C34)


R.T.: 19.345 min
Delta R.T.: 0.017 min
Response: 586784
Conc: 4.50 ug/ml

Instrument :
FID_C
ClientSampleId :

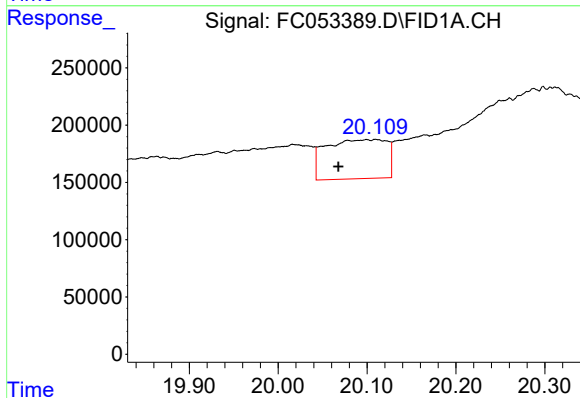


#20 n-Hexatriacontane (C36)

R.T.: 20.110 min
Delta R.T.: 0.043 min
Response: 1627473
Conc: 13.44 ug/ml

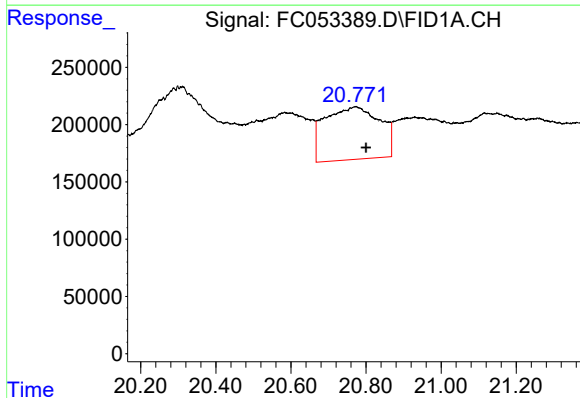

#21 n-Octatriacontane (C38)

R.T.: 20.772 min
Delta R.T.: -0.028 min
Response: 4679550
Conc: 44.41 ug/ml

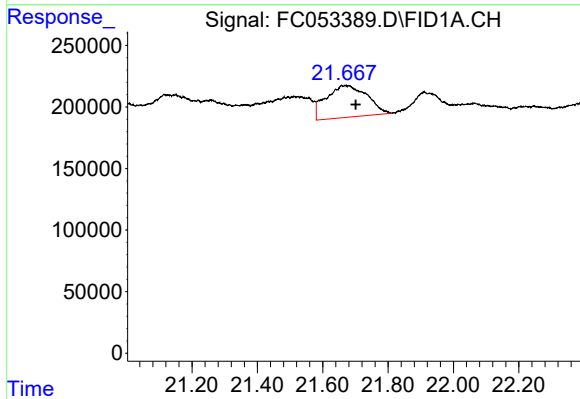

#22 n-Tetracontane (C40)

R.T.: 21.670 min
Delta R.T.: -0.031 min
Response: 2251087
Conc: 21.50 ug/ml