

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042622AL\
 Data File : FC059452.D
 Signal(s) : FID1A.CH
 Acq On : 26 Apr 2022 22:55
 Operator : UA/NP
 Sample : N2349-03DL2 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 27 00:16:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 042122.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 17:30:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.545	96069	0.736 ug/ml
Spiked Amount 50.000		Recovery =	1.47%
Target Compounds			
10) T n-Eicosane (C20)	12.105	211826	1.412 ug/ml
11) T n-Heneicosane (C21)	12.714	324729	2.135 ug/ml
13) T n-Docosane (C22)	13.297	462555	3.019 ug/ml
14) T n-Tetracosane (C24)	14.395	412887	2.667 ug/ml
15) T n-Hexacosane (C26)	15.412	81836	0.531 ug/ml
16) T n-Octacosane (C28)	16.352	205485	1.327 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042622AL\
Data File : FC059452.D
Signal(s) : FID1A.CH
Acq On : 26 Apr 2022 22:55
Operator : UA/NP
Sample : N2349-03DL2 100X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 00:16:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 042122.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 17:30:29 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

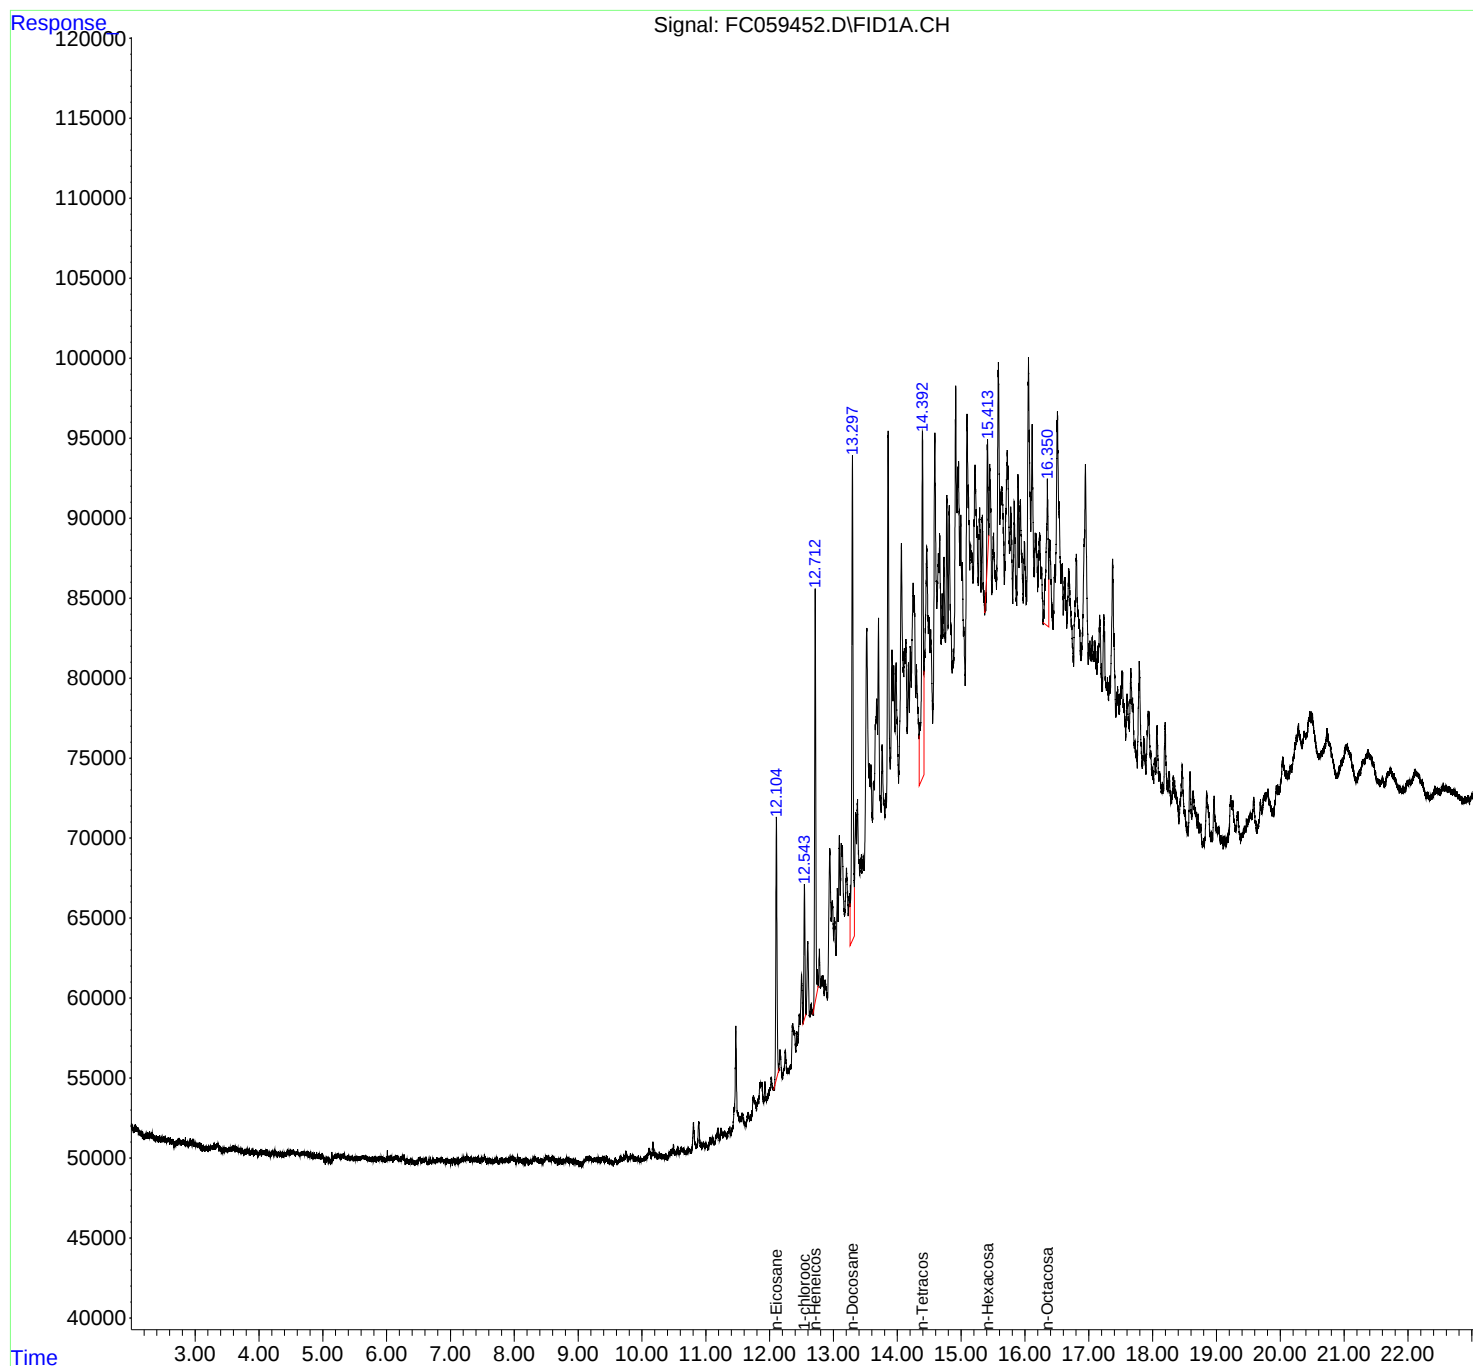


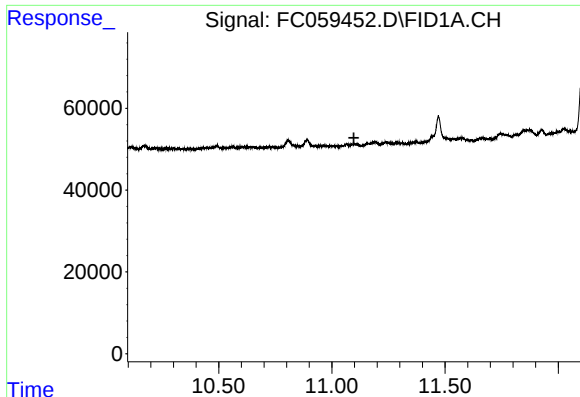

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.097 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

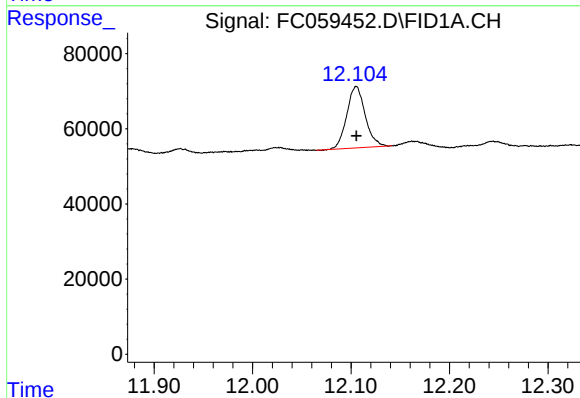


#10 n-Eicosane (C20)

R.T.: 12.105 min
Delta R.T.: 0.000 min
Response: 211826
Conc: 1.41 ug/ml

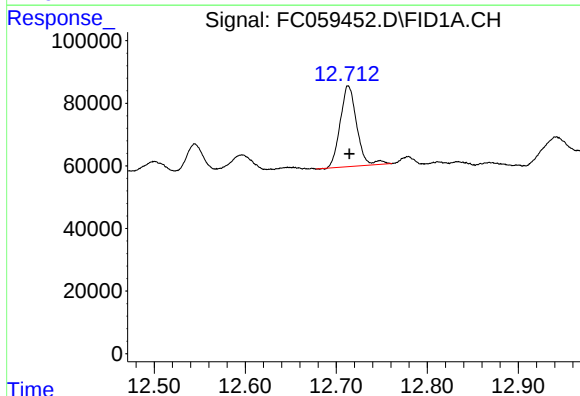


#11 n-Heneicosane (C21)

R.T.: 12.714 min
Delta R.T.: -0.001 min
Response: 324729
Conc: 2.13 ug/ml

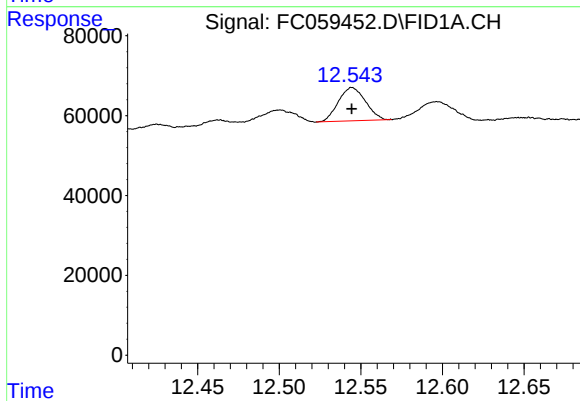

#12 1-chlorooctadecane (SURR)


R.T.: 12.545 min
Delta R.T.: 0.000 min
Response: 96069
Conc: 0.74 ug/ml

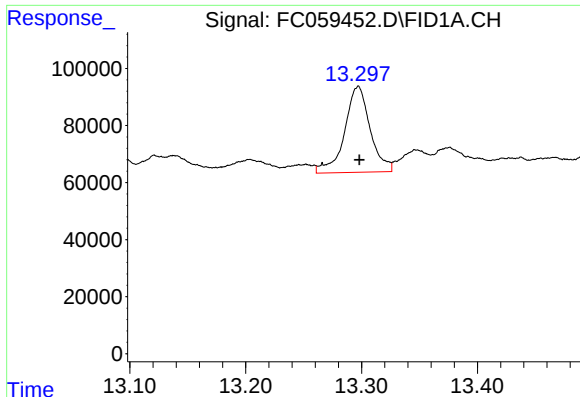

#13 n-Docosane (C22)


R.T.: 13.297 min
Delta R.T.: -0.001 min
Response: 462555
Conc: 3.02 ug/ml

Instrument :
FID_C
ClientSampleId :

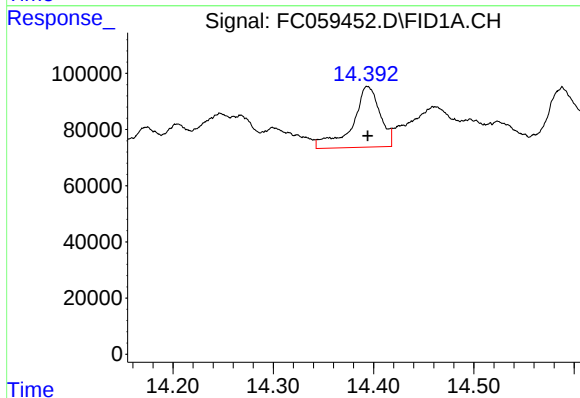


#14 n-Tetracosane (C24)

R.T.: 14.395 min
Delta R.T.: 0.000 min
Response: 412887
Conc: 2.67 ug/ml

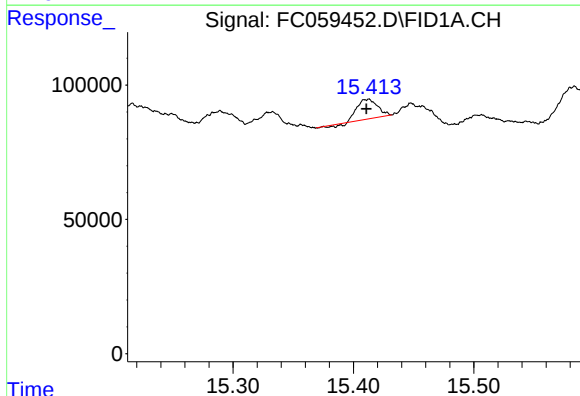

#15 n-Hexacosane (C26)

R.T.: 15.412 min
Delta R.T.: 0.000 min
Response: 81836
Conc: 0.53 ug/ml

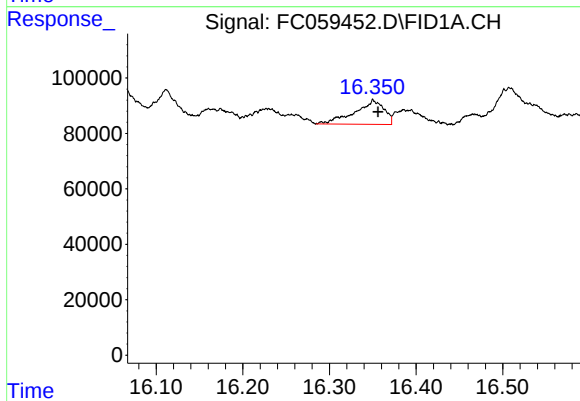

#16 n-Octacosane (C28)

R.T.: 16.352 min
Delta R.T.: -0.005 min
Response: 205485
Conc: 1.33 ug/ml