

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042624AL\
Data File : FC066240.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2024 09:56
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 00:54:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 041524.M
Quant Title : GC Extractables
QLast Update : Tue Apr 16 08:19:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.169	55978	0.473 ug/ml
20) T	n-Hexatriacontane (C36)	20.078	64117	0.621 ug/ml
22) T	n-Tetracontane (C40)	21.721	140238	1.550 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042624AL\
Data File : FC066240.D
Signal(s) : FID1A.ch
Acq On : 26 Apr 2024 09:56
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 27 00:54:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 041524.M
Quant Title : GC Extractables
QLast Update : Tue Apr 16 08:19:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

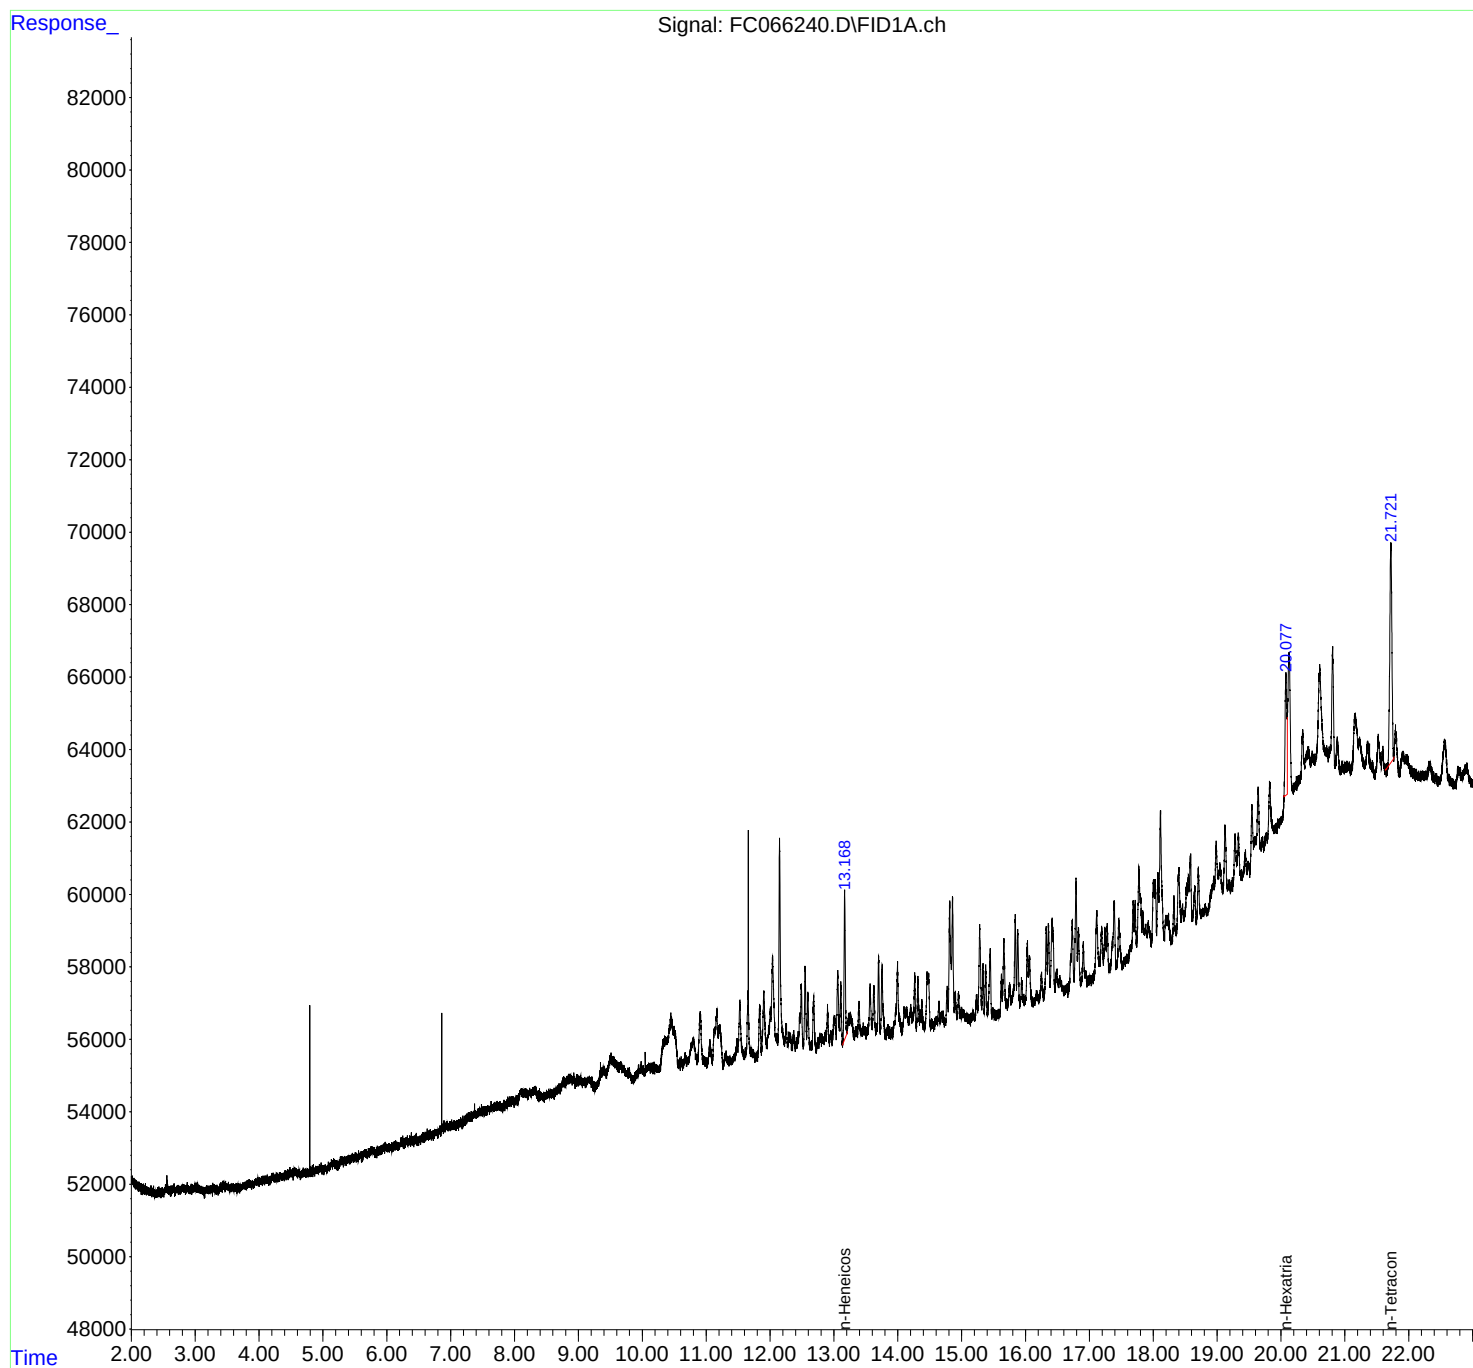


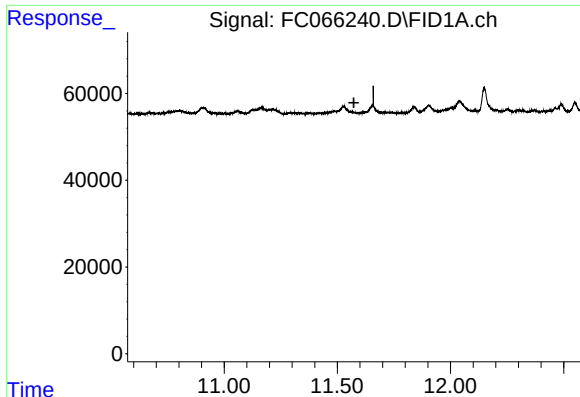

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.573 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

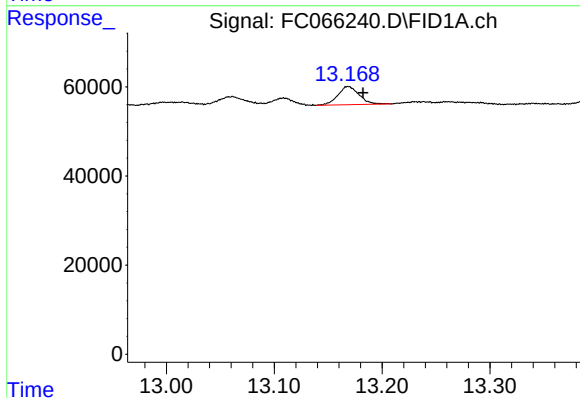


#11 n-Heneicosane (C21)

R.T.: 13.169 min
Delta R.T.: -0.014 min
Response: 55978
Conc: 0.47 ug/ml

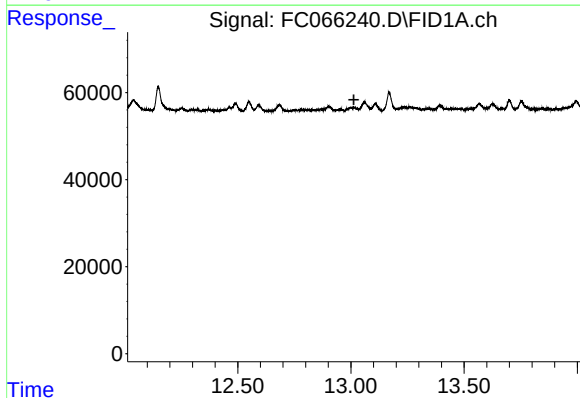


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.013 min
Response: 0
Conc: N.D.

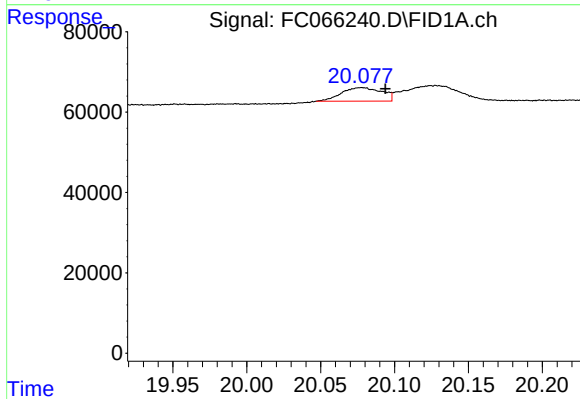

#20 n-Hexatriacontane (C36)

R.T.: 20.078 min
Delta R.T.: -0.016 min
Response: 64117
Conc: 0.62 ug/ml

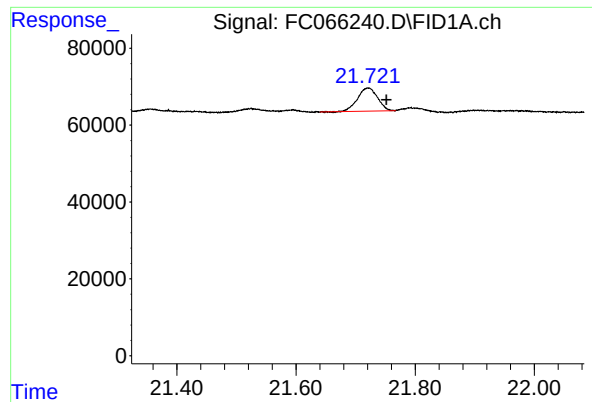

#22 n-Tetracontane (C40)

R.T.: 21.721 min
Delta R.T.: -0.031 min
Response: 140238
Conc: 1.55 ug/ml

Instrument :

FID_C

ClientSampleId :