

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC042723AL\  
 Data File : FC063476.D  
 Signal(s) : FID1A.ch  
 Acq On : 27 Apr 2023 18:35  
 Operator : YP/AJ  
 Sample : PB152444BL  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 PB152444BL

Integration File: autoint1.e  
 Quant Time: Apr 28 02:51:00 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 040523.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Apr 05 07:22:46 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 9) S ortho-Terphenyl (SURR)    | 11.533 | 6387101  | 41.980 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 83.96%     |
| 12) S 1-chlorooctadecane (S... | 12.970 | 4750052  | 42.930 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 85.86%     |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC042723AL\  
Data File : FC063476.D  
Signal(s) : FID1A.ch  
Acq On : 27 Apr 2023 18:35  
Operator : YP/AJ  
Sample : PB152444BL  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
PB152444BL

Integration File: autoint1.e  
Quant Time: Apr 28 02:51:00 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 040523.M  
Quant Title : GC Extractables  
QLast Update : Wed Apr 05 07:22:46 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

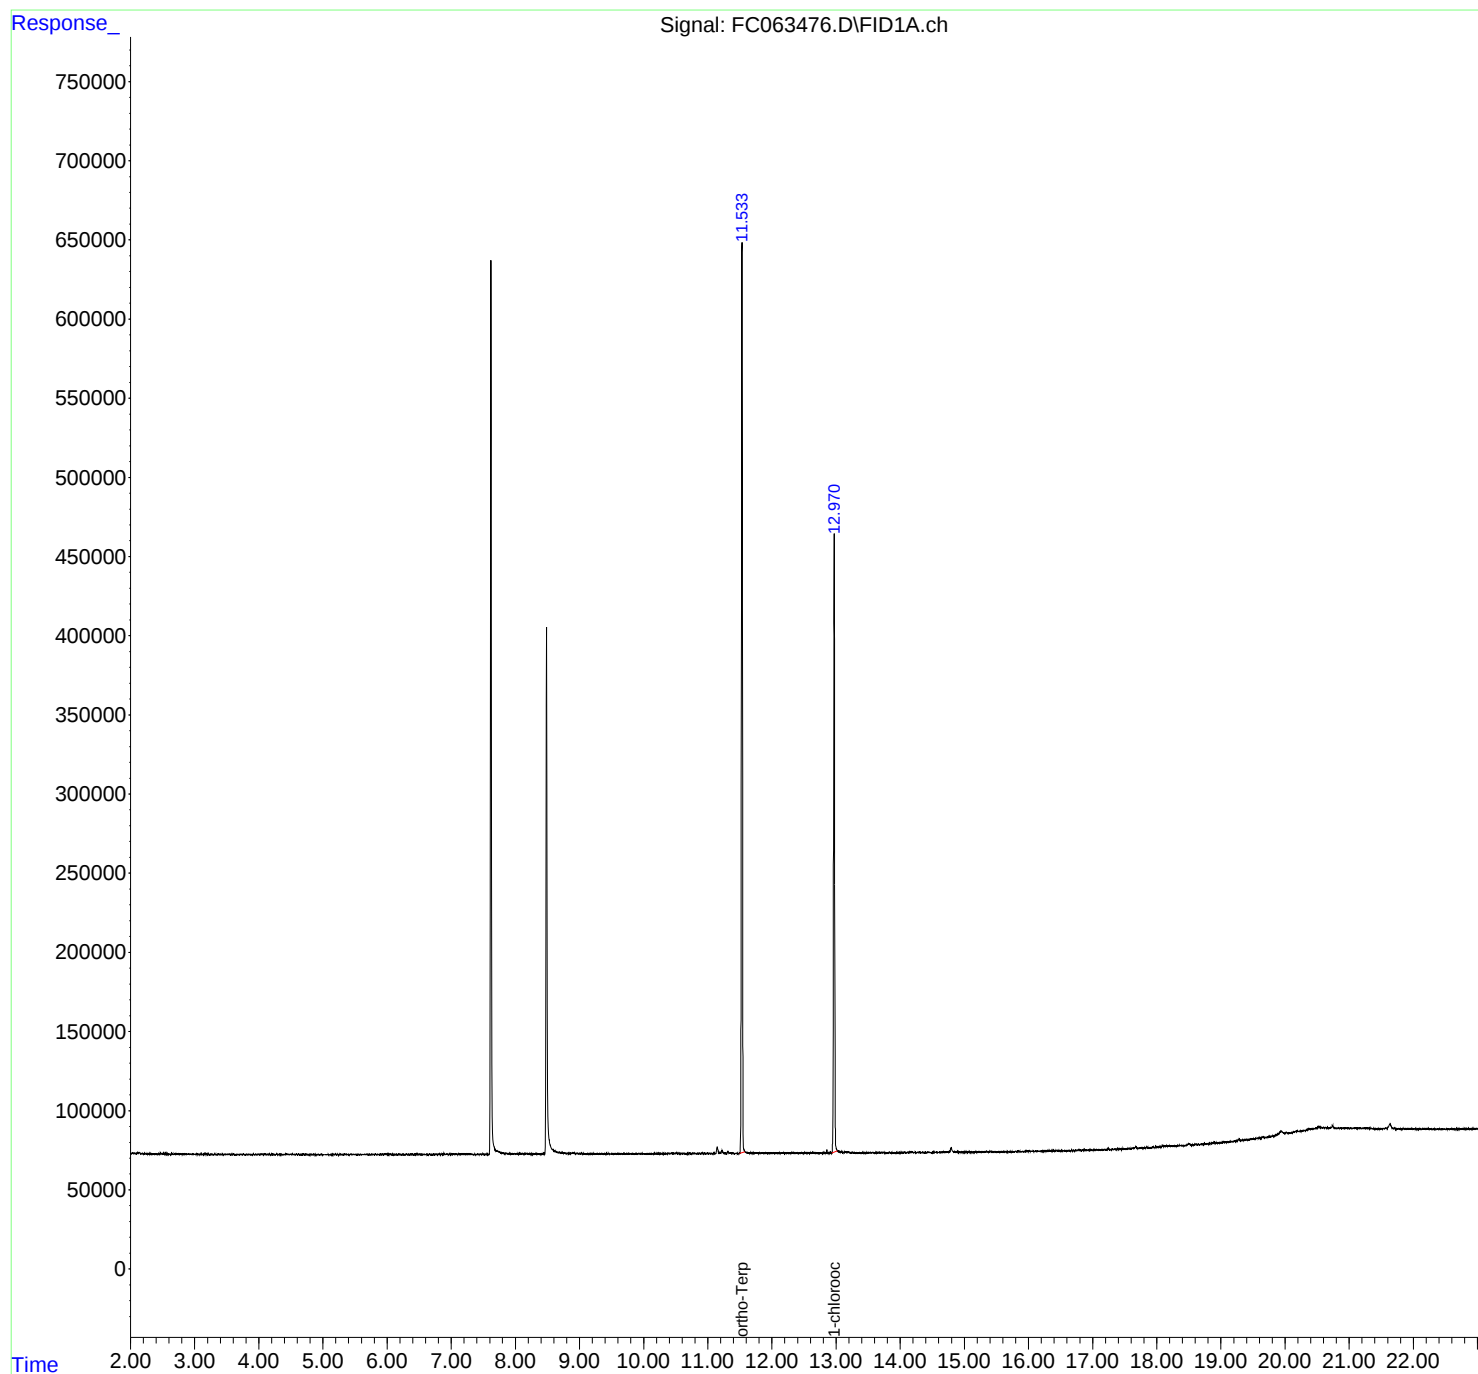


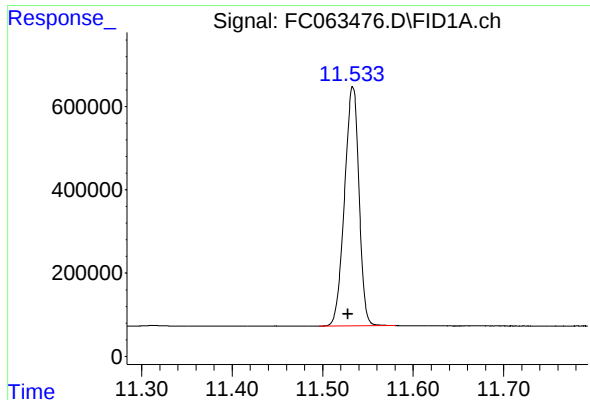

#9 ortho-Terphenyl (SURR)

R.T.: 11.533 min  
Delta R.T.: 0.006 min  
Response: 6387101  
Conc: 41.98 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
PB152444BL

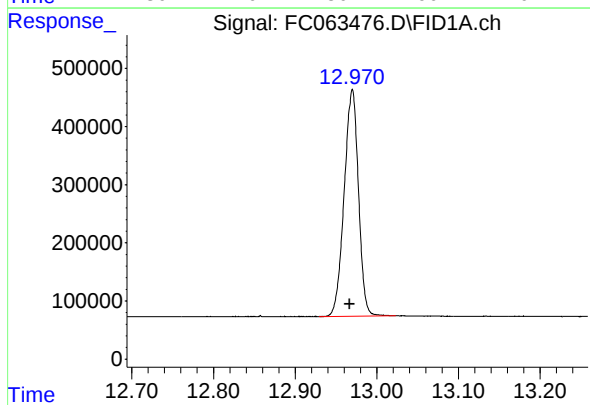

#12 1-chlorooctadecane (SURR)

R.T.: 12.970 min  
Delta R.T.: 0.003 min  
Response: 4750052  
Conc: 42.93 ug/ml