

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042821AL\
 Data File : FC053476.D
 Signal(s) : FID1A.CH
 Acq On : 28 Apr 2021 23:38
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 29 01:55:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042021.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 21 11:02:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.326	45197	0.346 ug/ml
20) T n-Hexatriacontane (C36)	20.136f	516478	4.266 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC042821AL\
Data File : FC053476.D
Signal(s) : FID1A.CH
Acq On : 28 Apr 2021 23:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 29 01:55:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 042021.M
Quant Title : GC Extractables
QLast Update : Wed Apr 21 11:02:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

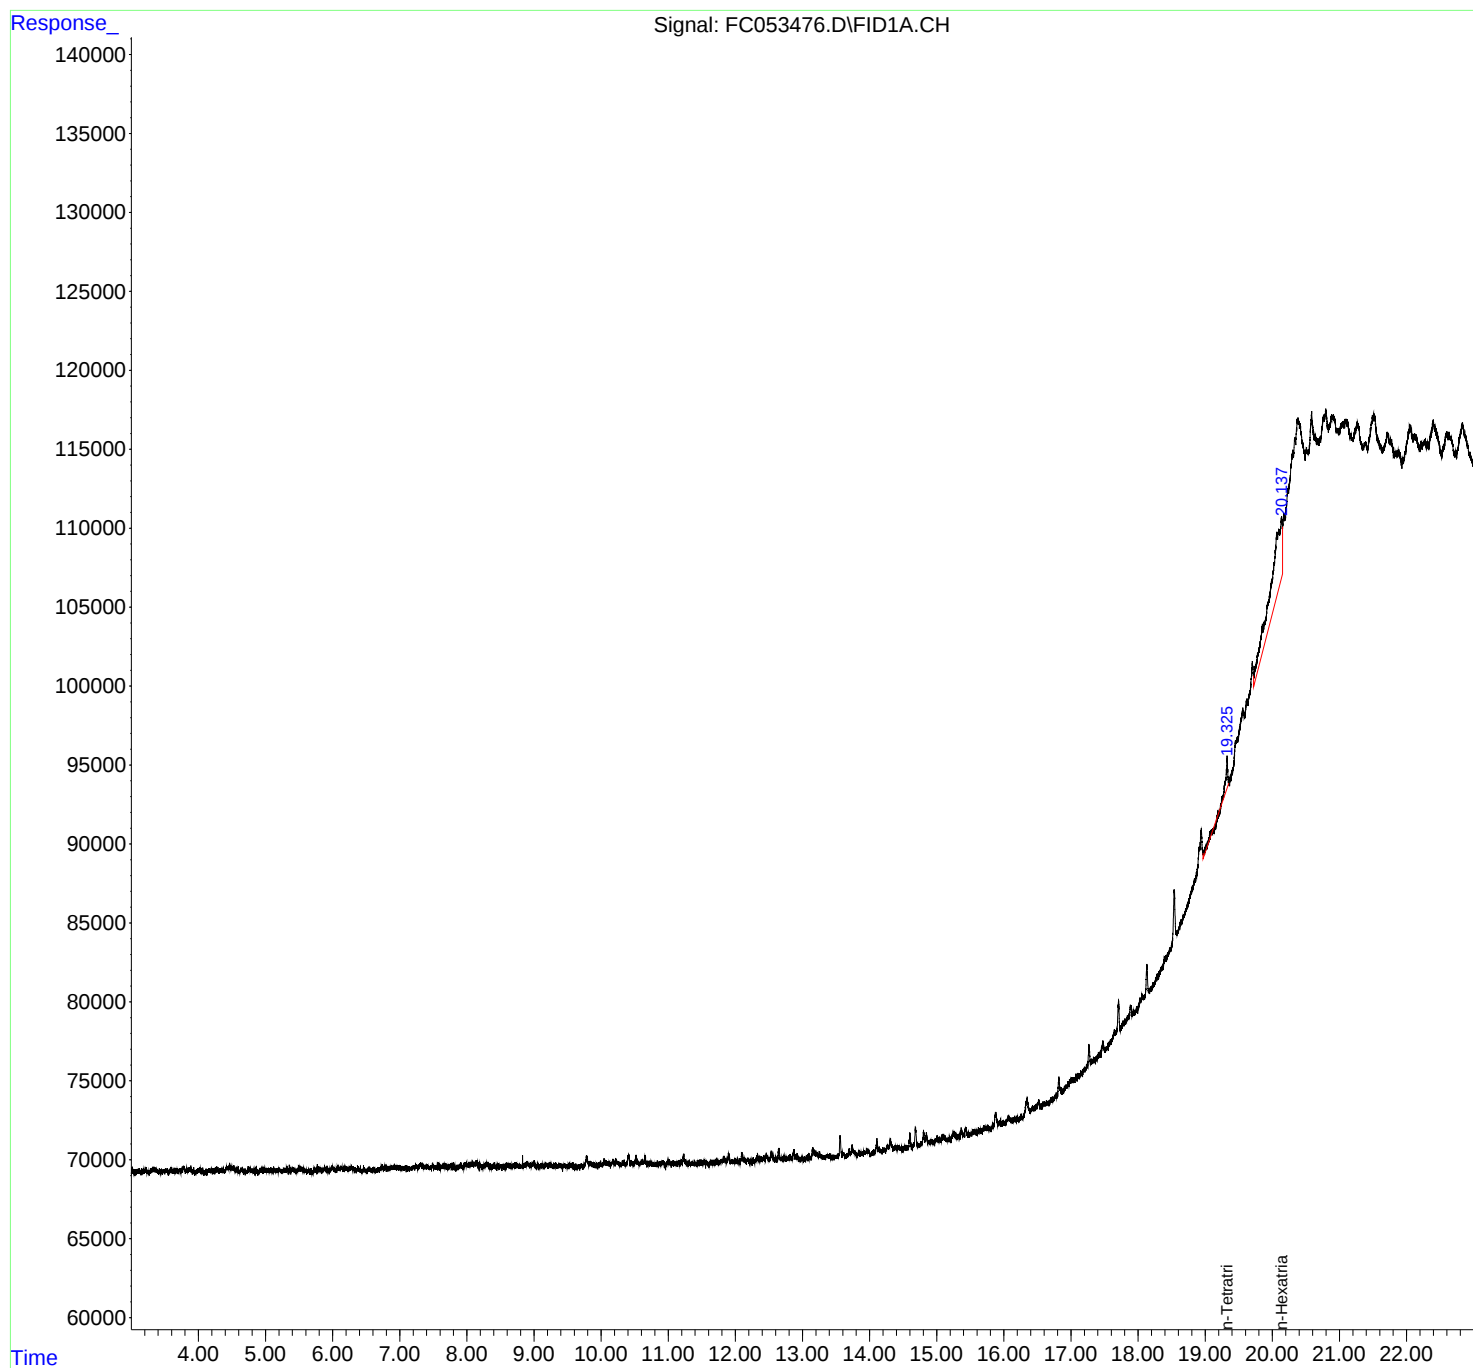


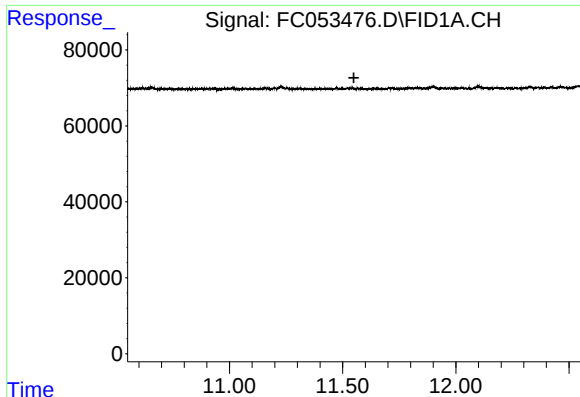

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.550 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

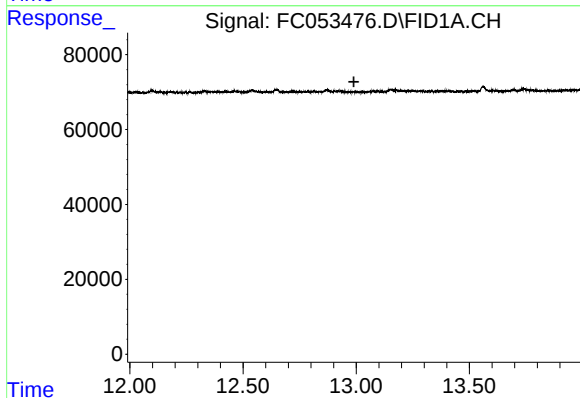


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 12.990 min
Response: 0
Conc: N.D.

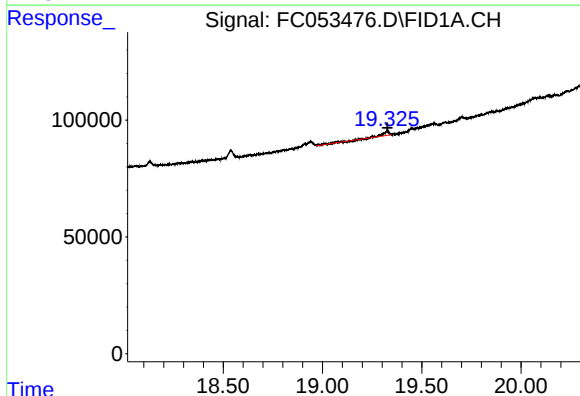

#19 n-Tetratriacontane (C34)

R.T.: 19.326 min
Delta R.T.: -0.002 min
Response: 45197
Conc: 0.35 ug/ml

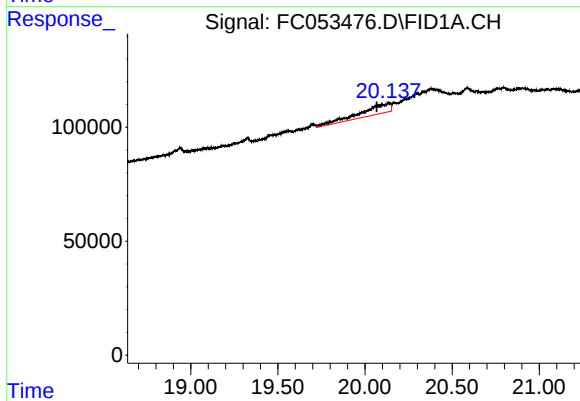

#20 n-Hexatriacontane (C36)

R.T.: 20.136 min
Delta R.T.: 0.069 min
Response: 516478
Conc: 4.27 ug/ml