

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050123AL\
Data File : FC063486.D
Signal(s) : FID1A.ch
Acq On : 01 May 2023 07:42
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 01 11:51:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 07:22:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.129	618569	4.596 ug/ml
13) T	n-Docosane (C22)	13.715	396980	2.977 ug/ml
14) T	n-Tetracosane (C24)	14.792	6704636	49.865 ug/ml
15) T	n-Hexacosane (C26)	15.846	437566	3.269 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050123AL\
Data File : FC063486.D
Signal(s) : FID1A.ch
Acq On : 01 May 2023 07:42
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 01 11:51:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 07:22:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

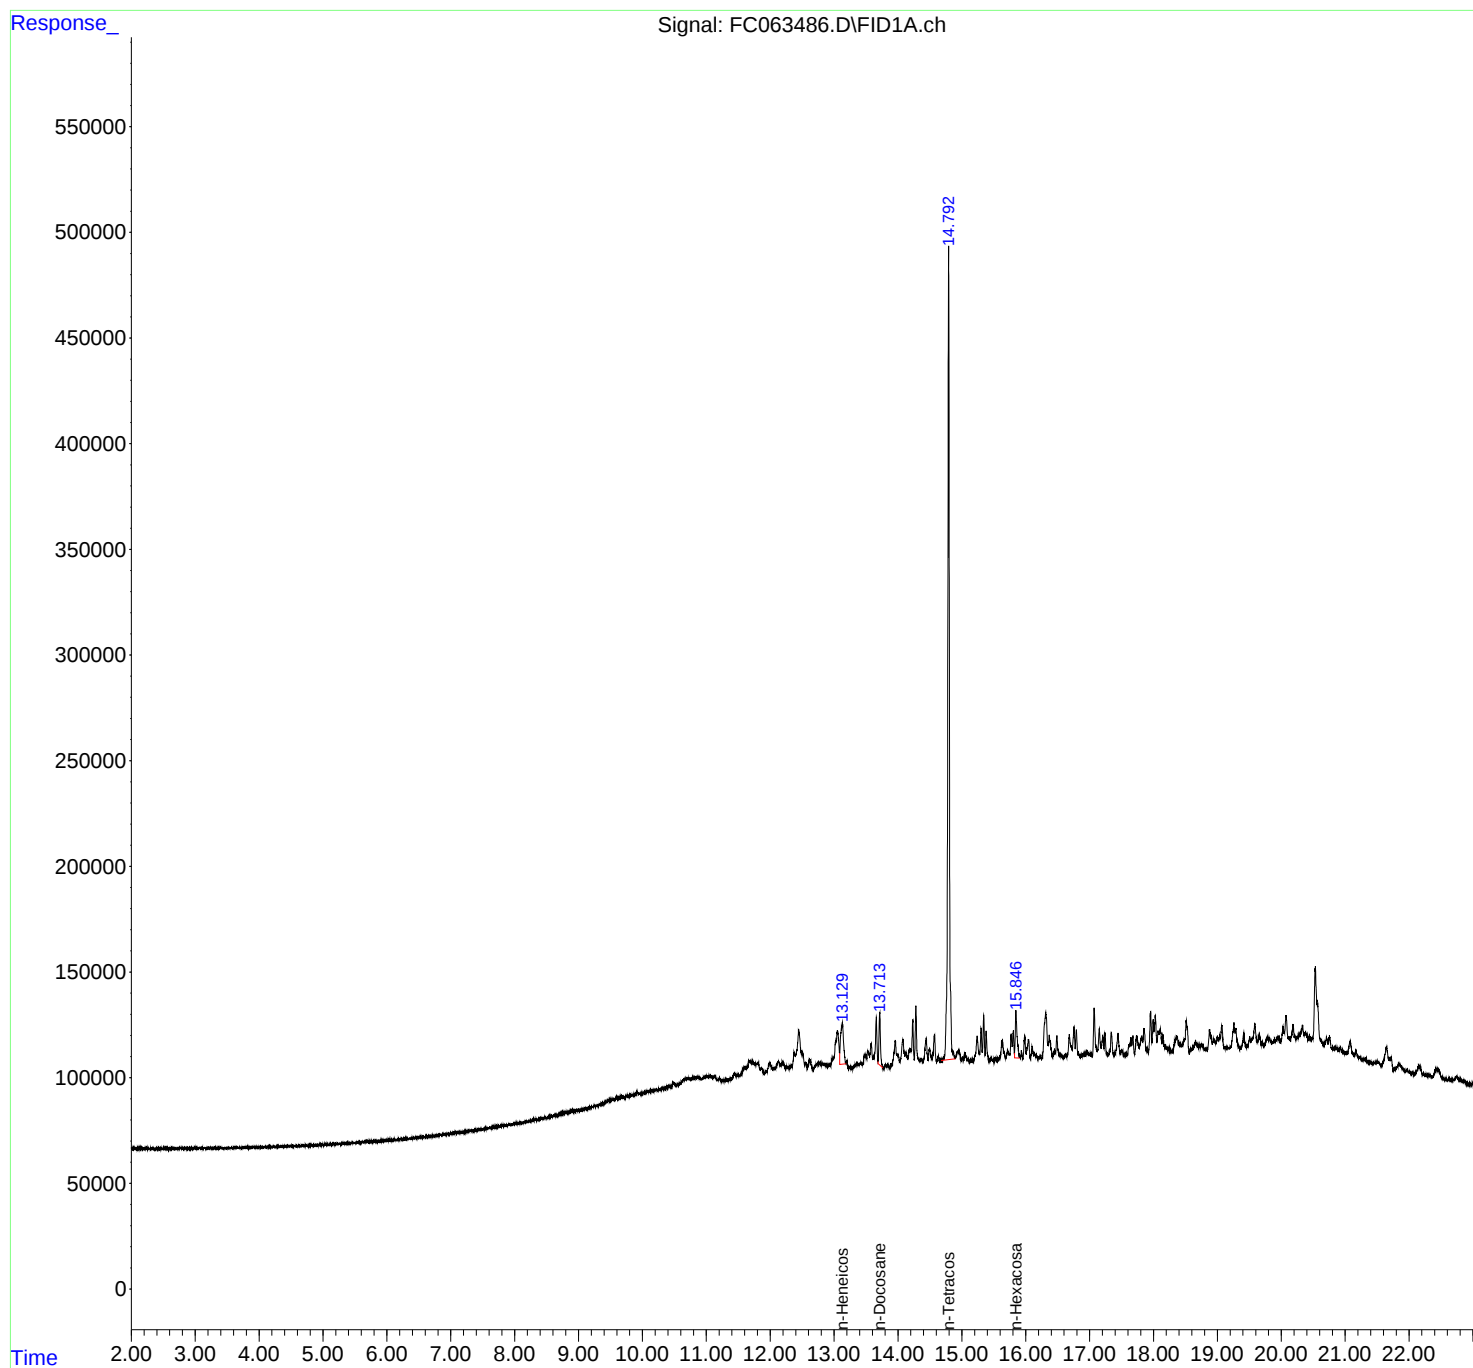


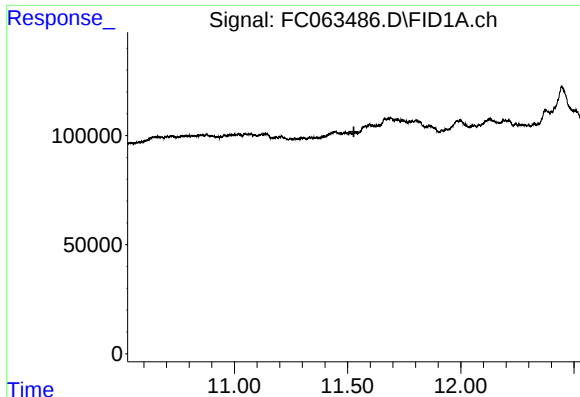

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.528 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

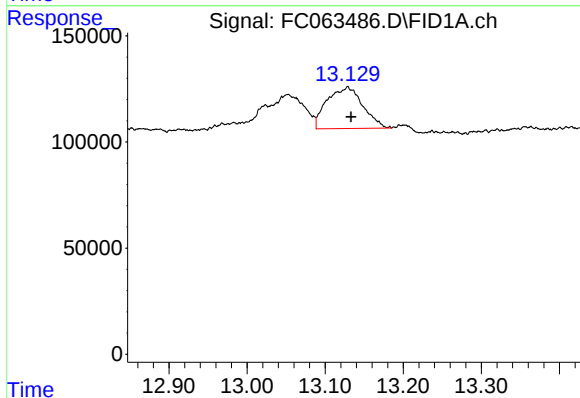


#11 n-Heneicosane (C21)

R.T.: 13.129 min
Delta R.T.: -0.004 min
Response: 618569
Conc: 4.60 ug/ml

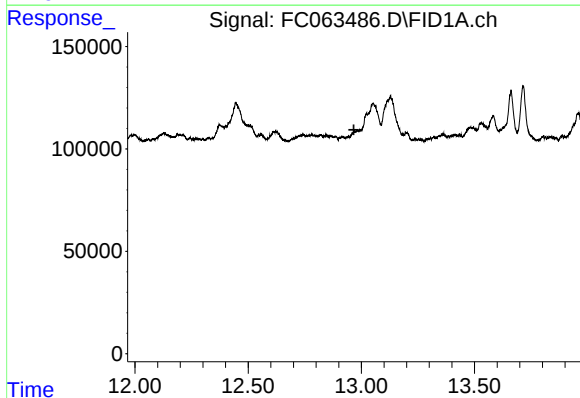


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.967 min
Response: 0
Conc: N.D.

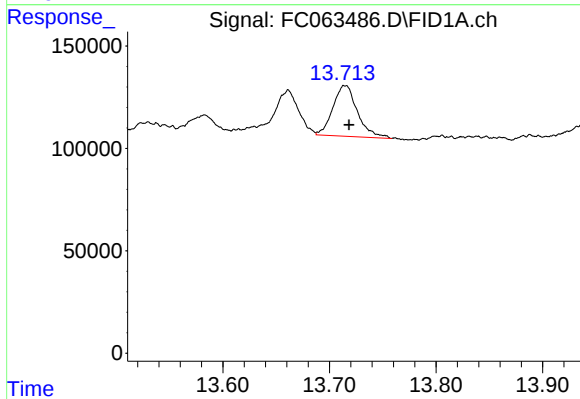

#13 n-Docosane (C22)


R.T.: 13.715 min
Delta R.T.: -0.004 min
Response: 396980
Conc: 2.98 ug/ml

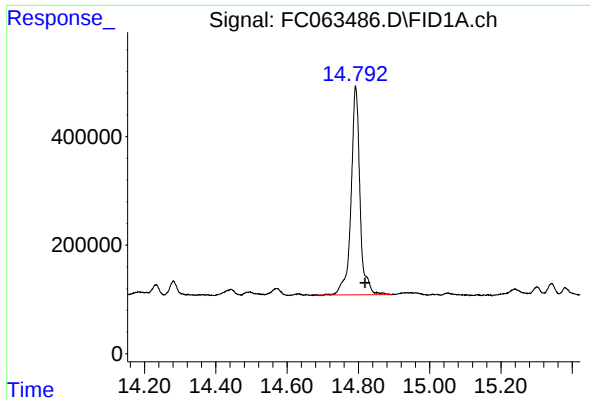

#14 n-Tetracosane (C24)

R.T.: 14.792 min
Delta R.T.: -0.026 min
Response: 6704636
Conc: 49.87 ug/ml

Instrument :
FID_C
ClientSampleId :

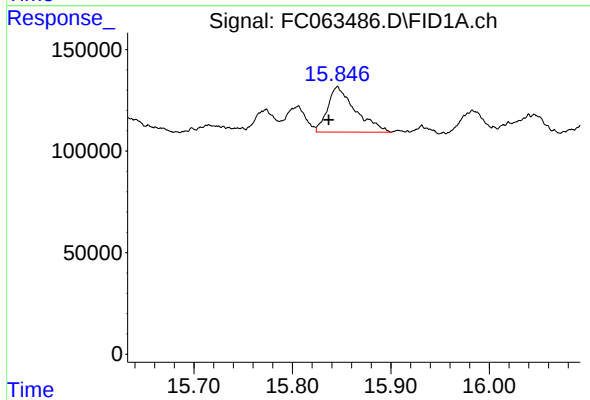

#15 n-Hexacosane (C26)

R.T.: 15.846 min
Delta R.T.: 0.009 min
Response: 437566
Conc: 3.27 ug/ml