

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC050224AL\  
 Data File : FC066295.D  
 Signal(s) : FID1A.ch  
 Acq On : 02 May 2024 22:21  
 Operator : YP/AJ  
 Sample : P2327-02  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: May 03 02:27:30 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 050124.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 02 09:03:15 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.000 | 3712663    | 30.268 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 60.54%       |
|                                |        |            |              |
| Target Compounds               |        |            |              |
| 2) T n-Decane (C10)            | 4.388  | 32268      | 0.210 ug/ml  |
| 4) T n-Dodecane (C12)          | 6.406  | 103247     | 0.672 ug/ml  |
| 6) T n-Tetradecane (C14)       | 8.201  | 51444      | 0.340 ug/ml  |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC050224AL\  
Data File : FC066295.D  
Signal(s) : FID1A.ch  
Acq On : 02 May 2024 22:21  
Operator : YP/AJ  
Sample : P2327-02  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: May 03 02:27:30 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 050124.M  
Quant Title : GC Extractables  
QLast Update : Thu May 02 09:03:15 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 u1  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

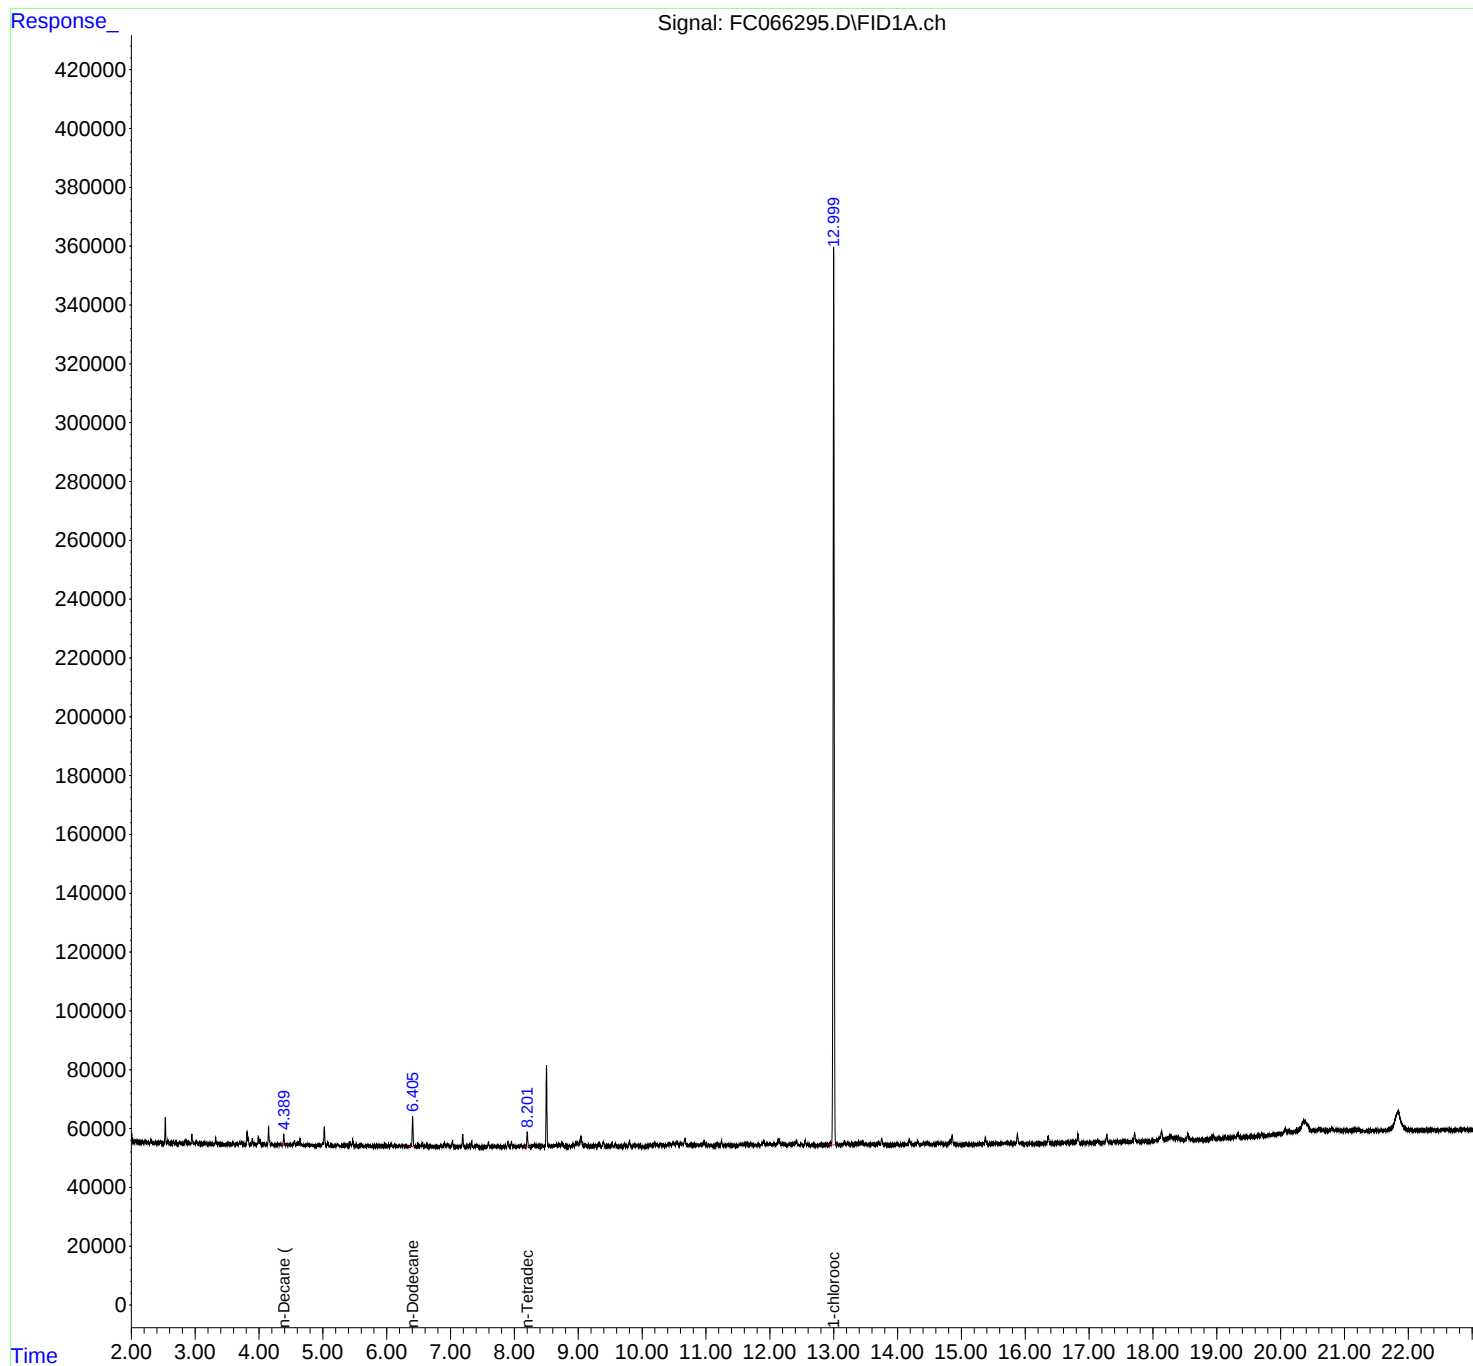


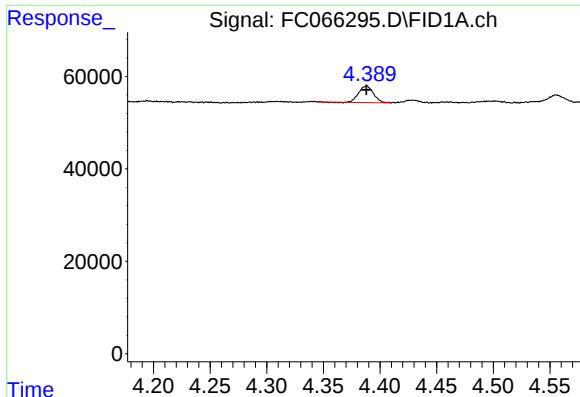

#2 n-Decane (C10)


R.T.: 4.388 min  
Delta R.T.: 0.000 min  
Response: 32268  
Conc: 0.21 ug/ml

Instrument :  
FID\_C  
ClientSampleId :

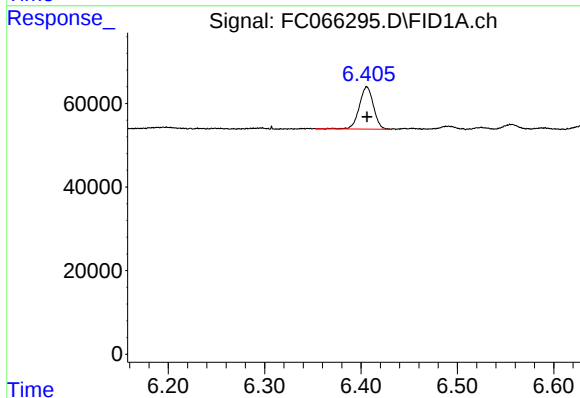


#4 n-Dodecane (C12)

R.T.: 6.406 min  
Delta R.T.: 0.000 min  
Response: 103247  
Conc: 0.67 ug/ml

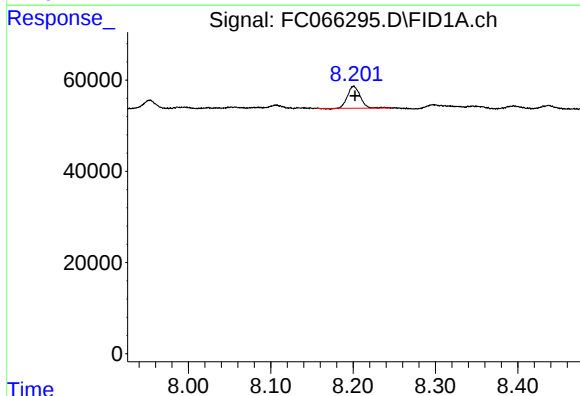


#6 n-Tetradecane (C14)

R.T.: 8.201 min  
Delta R.T.: -0.002 min  
Response: 51444  
Conc: 0.34 ug/ml

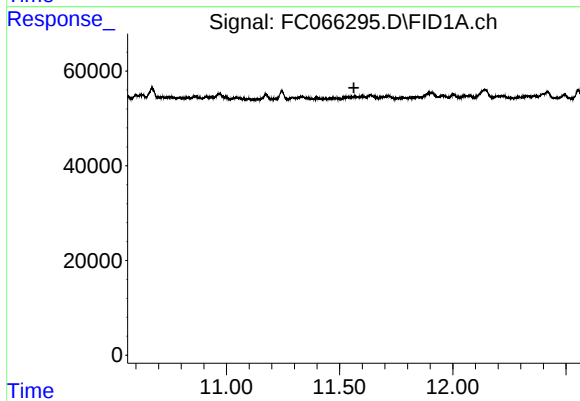

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 11.563 min  
Response: 0  
Conc: N.D.

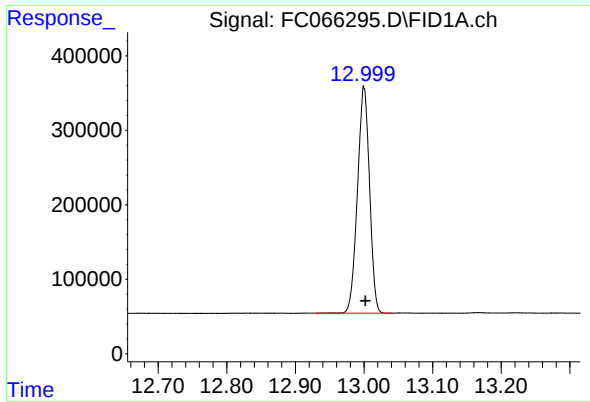

#12 1-chlorooctadecane (SURR)

R.T.: 13.000 min  
Delta R.T.: -0.002 min  
Response: 3712663  
Conc: 30.27 ug/ml

Instrument :  
FID\_C  
ClientSampleId :