

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050224AL\
 Data File : FC066299.D
 Signal(s) : FID1A.ch
 Acq On : 03 May 2024 01:43
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 03 02:28:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050124.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:03:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.576	103960	0.807 ug/ml
20) T n-Hexatriacontane (C36)	20.128f	136431	1.187 ug/ml
22) T n-Tetracontane (C40)	21.791	275544	2.570 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050224AL\
Data File : FC066299.D
Signal(s) : FID1A.ch
Acq On : 03 May 2024 01:43
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 03 02:28:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050124.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:03:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

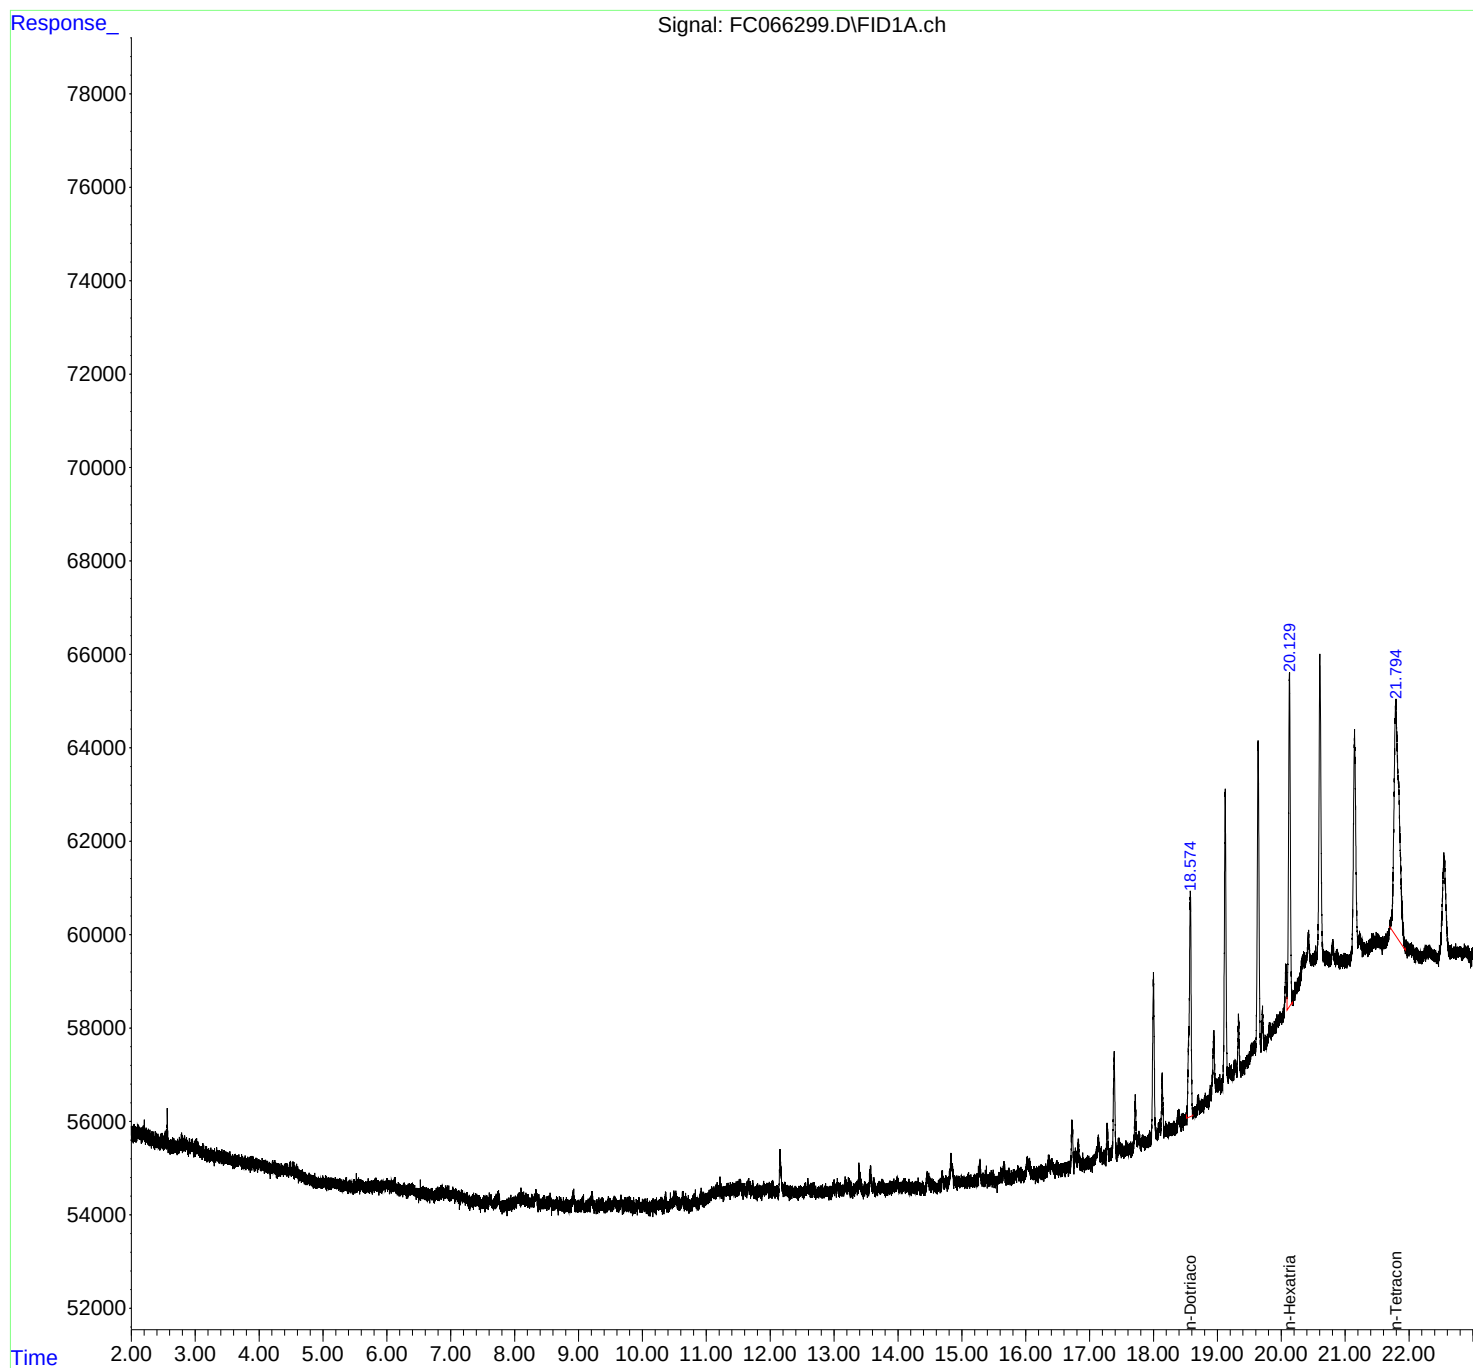


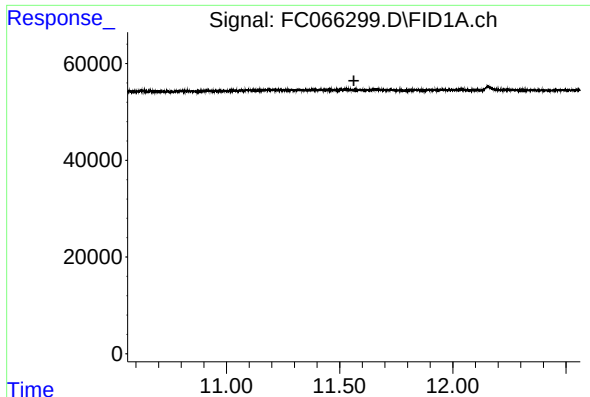

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.563 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

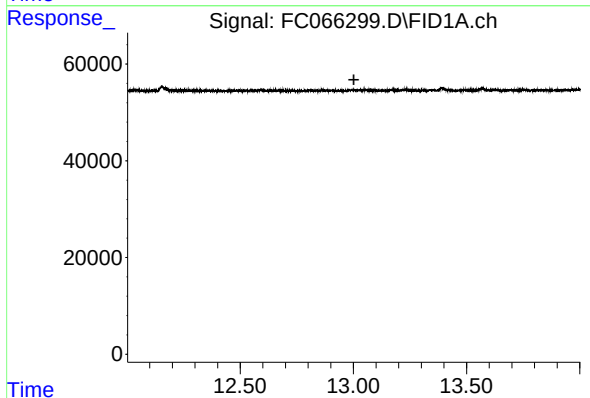


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.002 min
Response: 0
Conc: N.D.

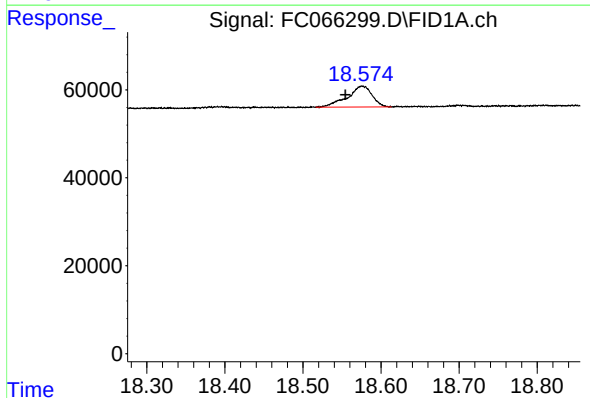


#18 n-Dotriacontane (C32)

R.T.: 18.576 min
Delta R.T.: 0.022 min
Response: 103960
Conc: 0.81 ug/ml

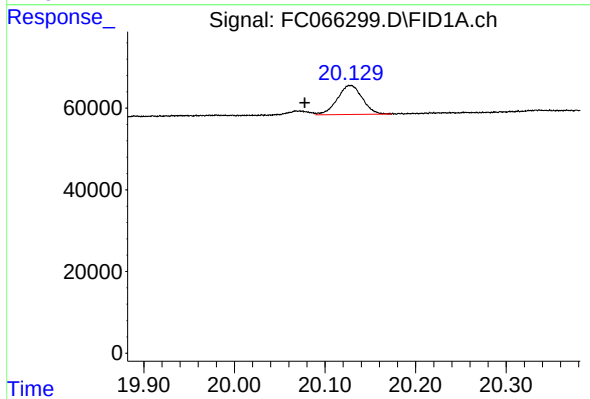

#20 n-Hexatriacontane (C36)

R.T.: 20.128 min
Delta R.T.: 0.050 min
Response: 136431
Conc: 1.19 ug/ml

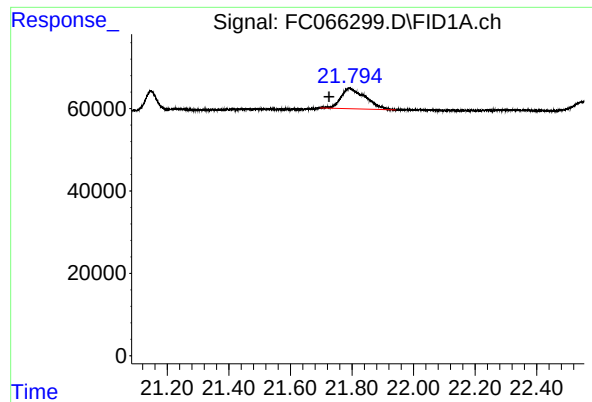

#22 n-Tetracontane (C40)

R.T.: 21.791 min
Delta R.T.: 0.065 min
Response: 275544
Conc: 2.57 ug/ml

Instrument :
FID_C
ClientSampleId :