

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC050324AL\  
Data File : FC066305.D  
Signal(s) : FID1A.ch  
Acq On : 03 May 2024 08:35  
Operator : YP/AJ  
Sample : P2327-03DL 25X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
PE-3(3.5-4)DL

Integration File: autoint1.e  
Quant Time: May 03 11:24:05 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 050124.M  
Quant Title : GC Extractables  
QLast Update : Thu May 02 09:03:15 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 12) S 1-chlorooctadecane (S... | 12.996 | 229574     | 1.872 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 3.74%       |
| Target Compounds               |        |            |             |
| -----                          |        |            |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC050324AL\  
Data File : FC066305.D  
Signal(s) : FID1A.ch  
Acq On : 03 May 2024 08:35  
Operator : YP/AJ  
Sample : P2327-03DL 25X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
PE-3(3.5-4)DL

Integration File: autoint1.e  
Quant Time: May 03 11:24:05 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 050124.M  
Quant Title : GC Extractables  
QLast Update : Thu May 02 09:03:15 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

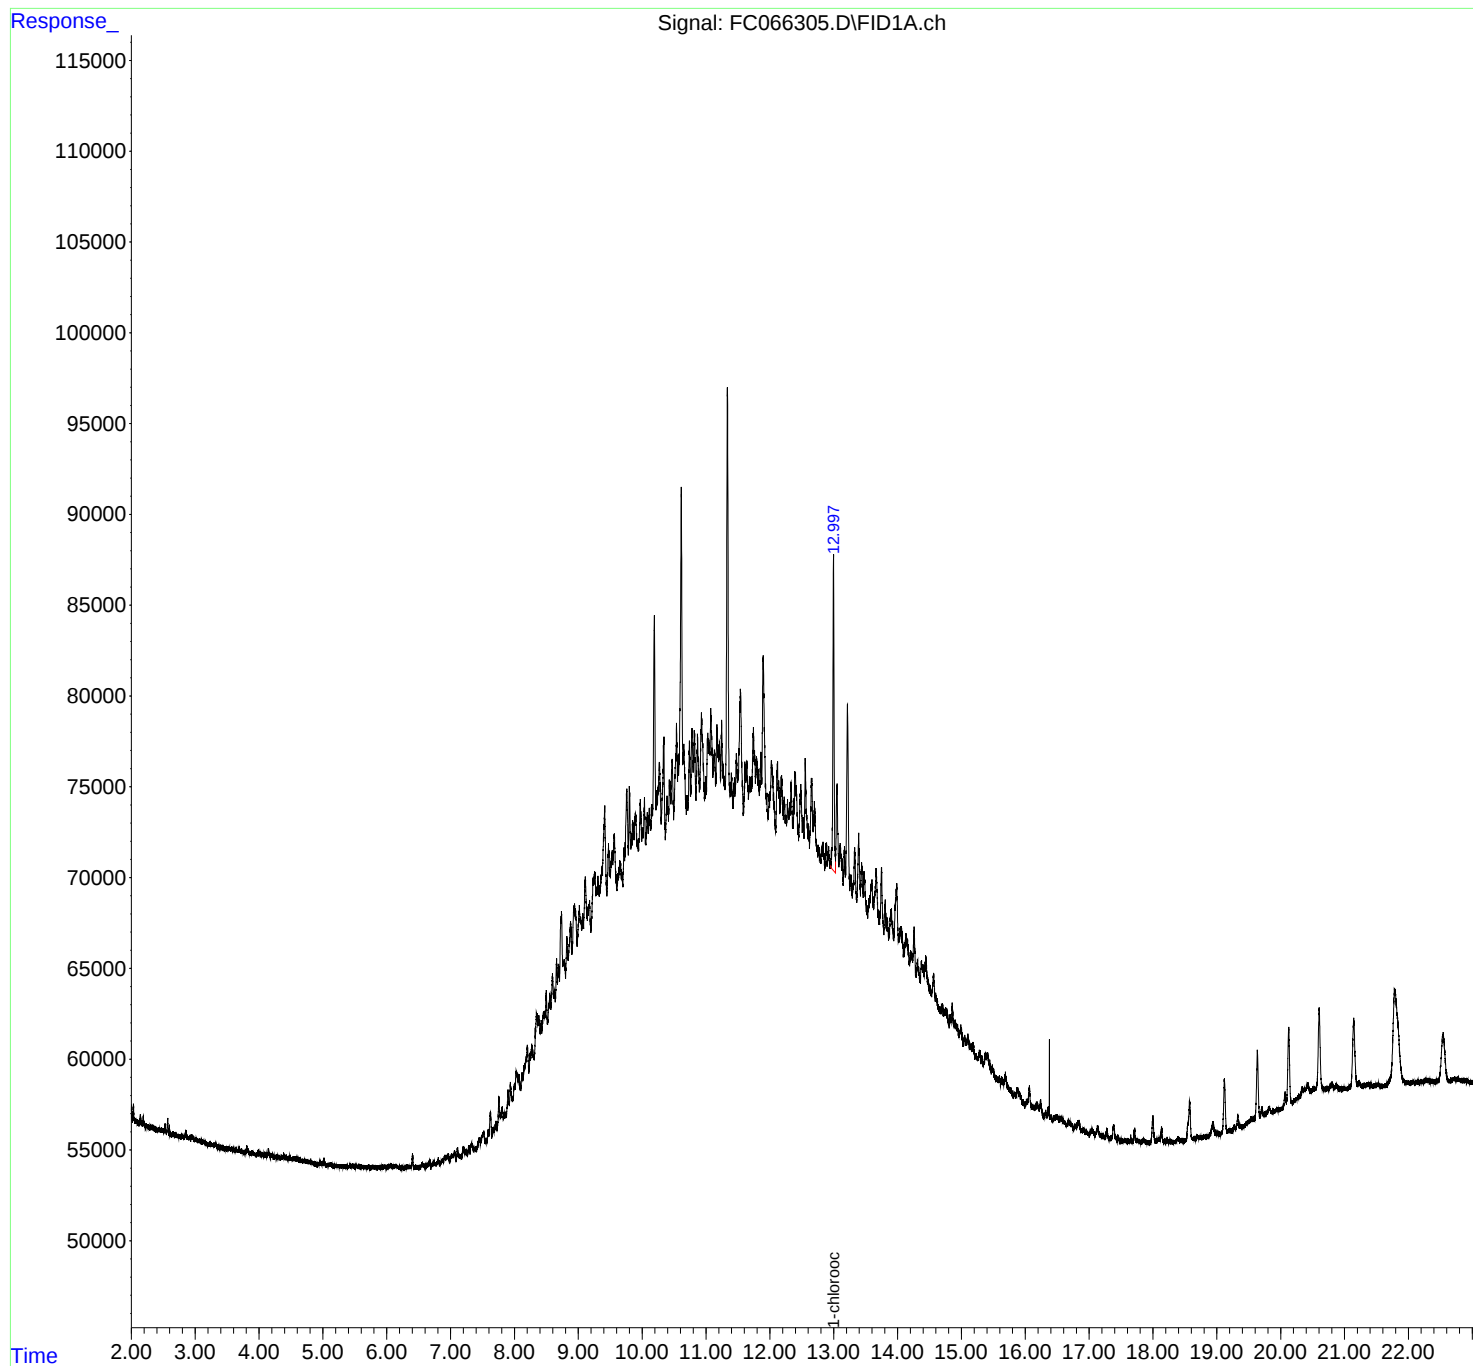


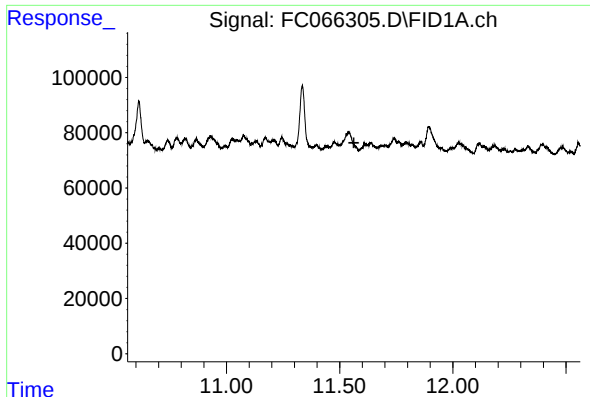

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.563 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
PE-3(3.5-4)DL

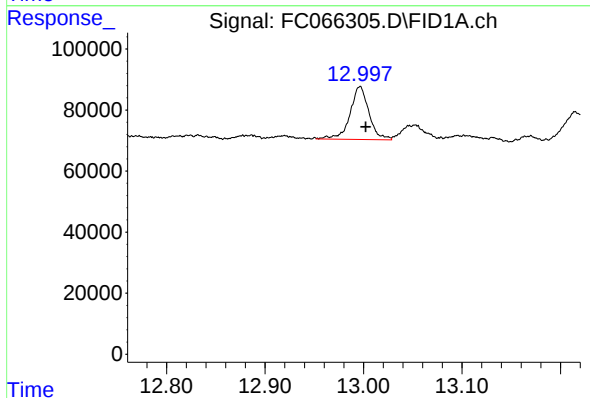

#12 1-chlorooctadecane (SURR)

R.T.: 12.996 min  
Delta R.T.: -0.006 min  
Response: 229574  
Conc: 1.87 ug/ml