

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050621AL\
 Data File : FC053535.D
 Signal(s) : FID1A.CH
 Acq On : 06 May 2021 15:13
 Operator : DD\AJ
 Sample : M2279-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 07 05:07:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
 Quant Title : GC Extractables
 QLast Update : Tue May 04 11:44:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.975	2548426	22.849 ug/ml
Spiked Amount 50.000		Recovery =	45.70%
Target Compounds			
4) T n-Dodecane (C12)	6.375	137654	1.138 ug/ml
14) T n-Tetracosane (C24)	14.833	106834	0.800 ug/ml
15) T n-Hexacosane (C26)	15.856	179210	1.355 ug/ml
16) T n-Octacosane (C28)	16.807	174121	1.330 ug/ml
17) T n-Tricontane (C30)	17.694	209012	1.602 ug/ml
18) T n-Dotriacontane (C32)	18.527	127819	1.013 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050621AL\
Data File : FC053535.D
Signal(s) : FID1A.CH
Acq On : 06 May 2021 15:13
Operator : DD\AJ
Sample : M2279-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 07 05:07:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
Quant Title : GC Extractables
QLast Update : Tue May 04 11:44:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

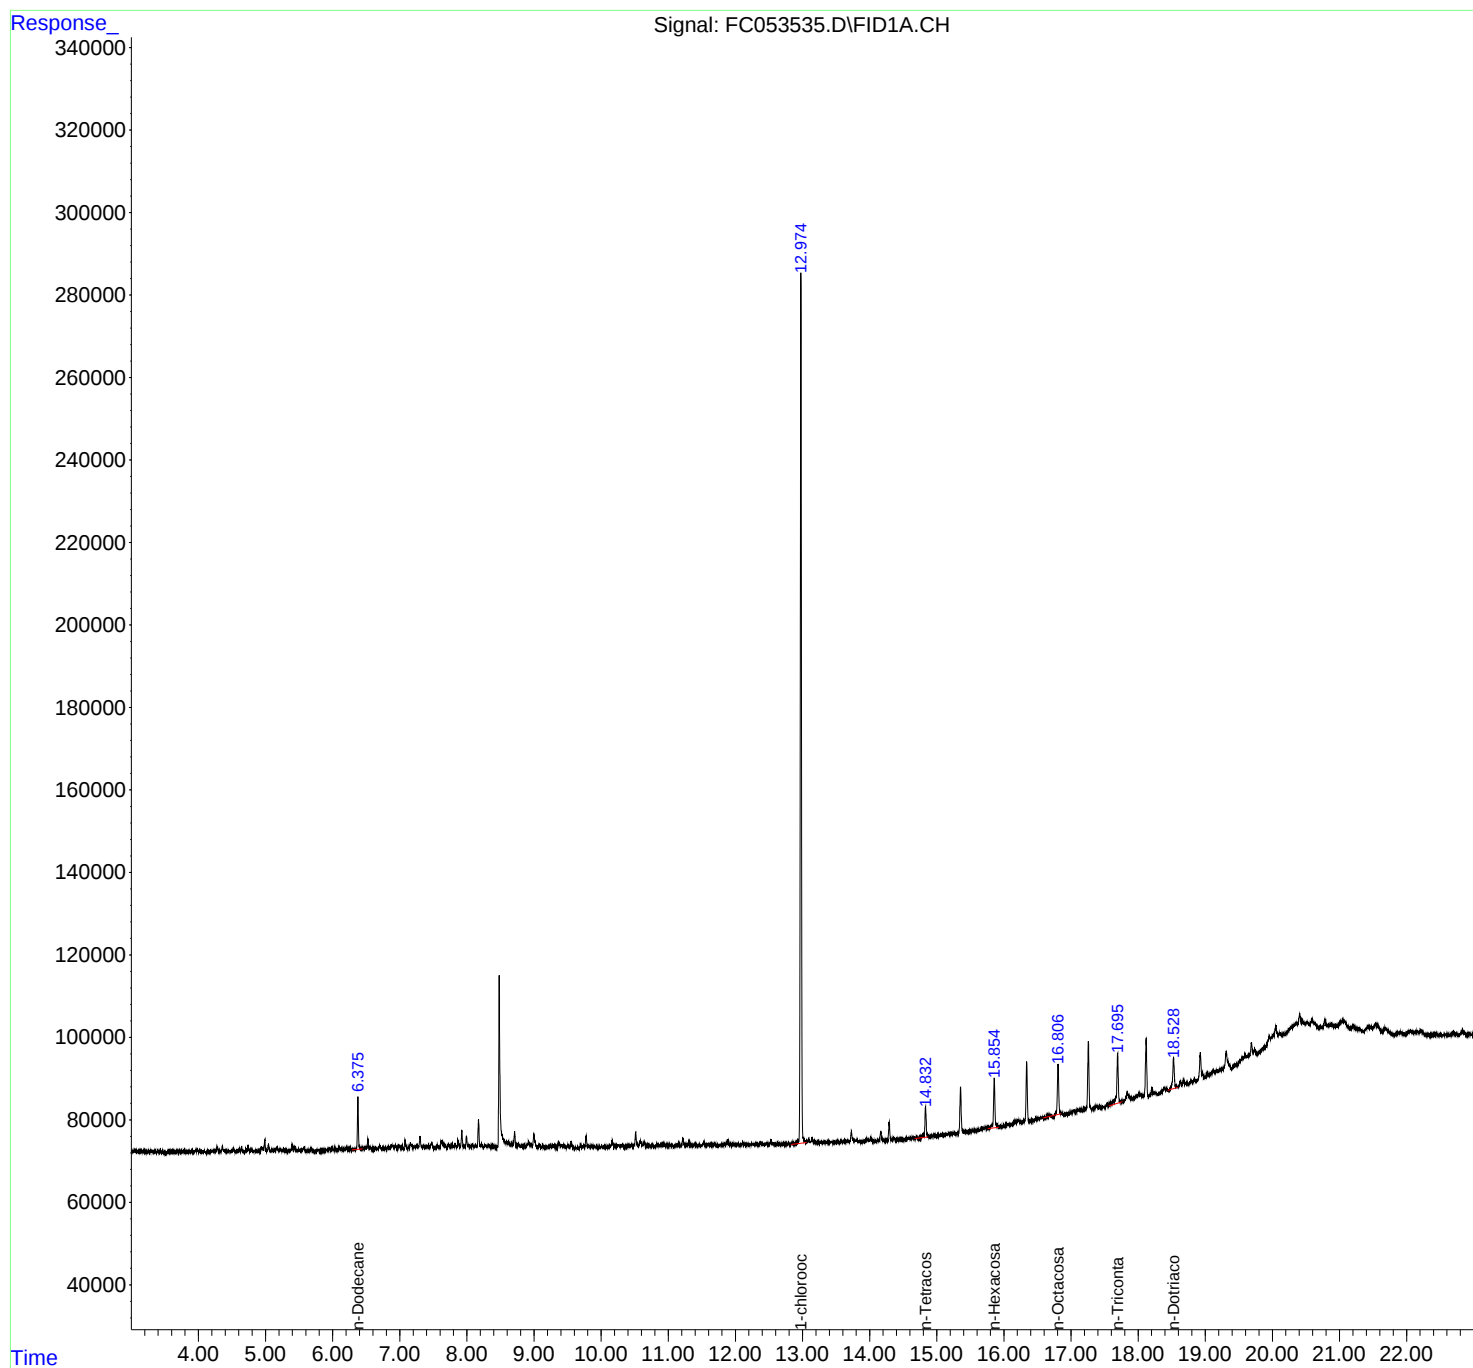


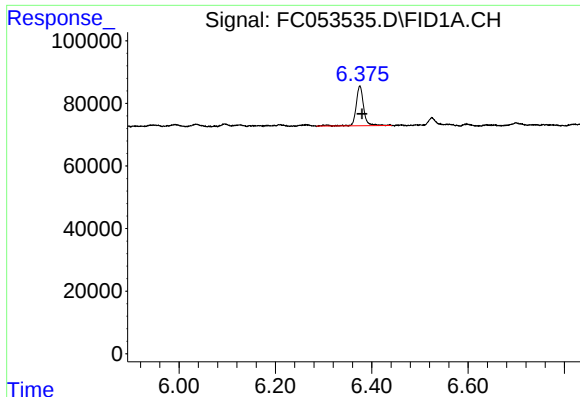

#4 n-Dodecane (C12)


R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 137654
Conc: 1.14 ug/ml

Instrument :
FID_C
ClientSampleId :

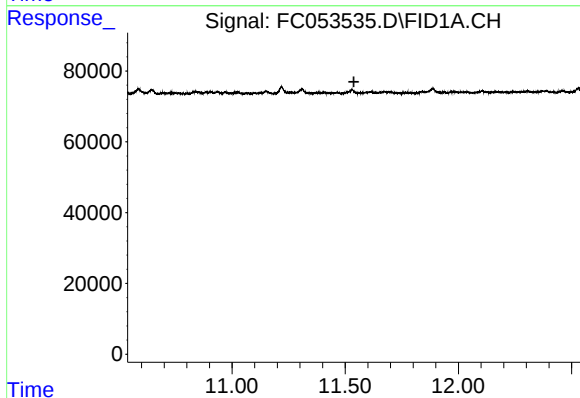


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.538 min
Response: 0
Conc: N.D.

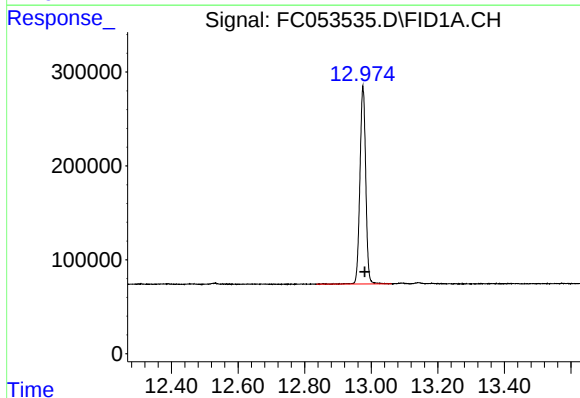


#12 1-chlorooctadecane (SURR)

R.T.: 12.975 min
Delta R.T.: -0.005 min
Response: 2548426
Conc: 22.85 ug/ml

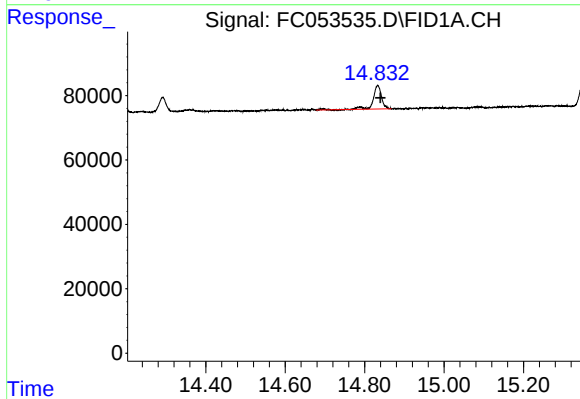

#14 n-Tetracosane (C24)


R.T.: 14.833 min
Delta R.T.: -0.007 min
Response: 106834
Conc: 0.80 ug/ml

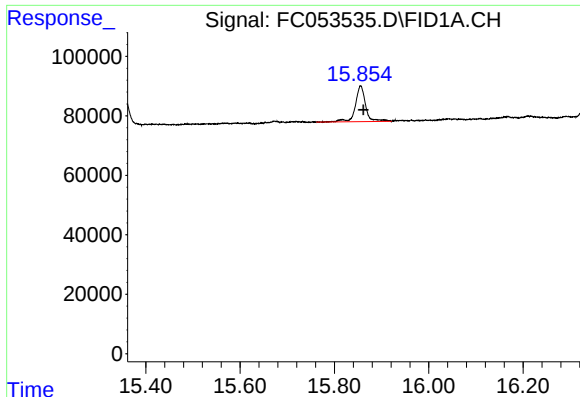

#15 n-Hexacosane (C26)


R.T.: 15.856 min
Delta R.T.: -0.006 min
Response: 179210
Conc: 1.36 ug/ml

Instrument :
FID_C
ClientSampleId :

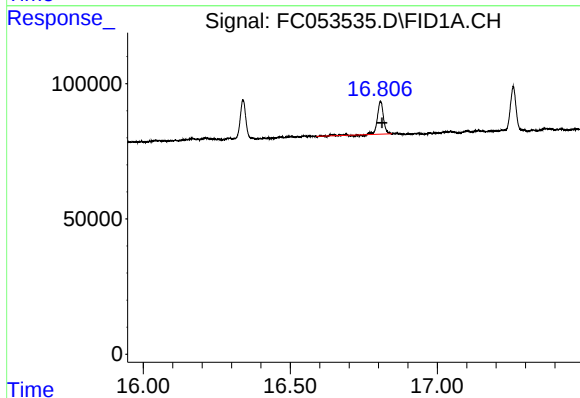


#16 n-Octacosane (C28)

R.T.: 16.807 min
Delta R.T.: -0.005 min
Response: 174121
Conc: 1.33 ug/ml

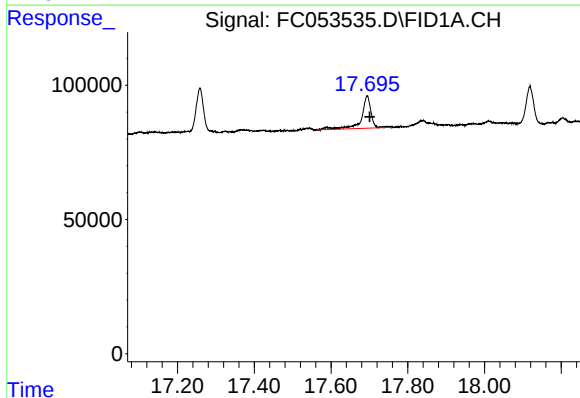

#17 n-Tricontane (C30)

R.T.: 17.694 min
Delta R.T.: -0.007 min
Response: 209012
Conc: 1.60 ug/ml

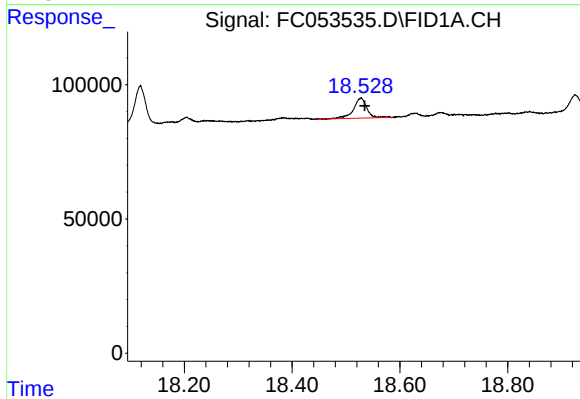

#18 n-Dotriacontane (C32)

R.T.: 18.527 min
Delta R.T.: -0.007 min
Response: 127819
Conc: 1.01 ug/ml