

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050621AL\
 Data File : FC053536.D
 Signal(s) : FID1A.CH
 Acq On : 06 May 2021 15:51
 Operator : DD\AJ
 Sample : M2279-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 07 05:07:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
 Quant Title : GC Extractables
 QLast Update : Tue May 04 11:44:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.977	3881245	34.799 ug/ml
Spiked Amount 50.000		Recovery =	69.60%
Target Compounds			
4) T n-Dodecane (C12)	6.376	191427	1.582 ug/ml
6) T n-Tetradecane (C14)	8.173	76085	0.625 ug/ml
14) T n-Tetracosane (C24)	14.834	95085	0.712 ug/ml
15) T n-Hexacosane (C26)	15.856	161176	1.219 ug/ml
16) T n-Octacosane (C28)	16.806	176233	1.346 ug/ml
17) T n-Tricontane (C30)	17.696	200567	1.538 ug/ml
18) T n-Dotriacontane (C32)	18.529	120452	0.955 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050621AL\
Data File : FC053536.D
Signal(s) : FID1A.CH
Acq On : 06 May 2021 15:51
Operator : DD\AJ
Sample : M2279-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 07 05:07:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
Quant Title : GC Extractables
QLast Update : Tue May 04 11:44:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

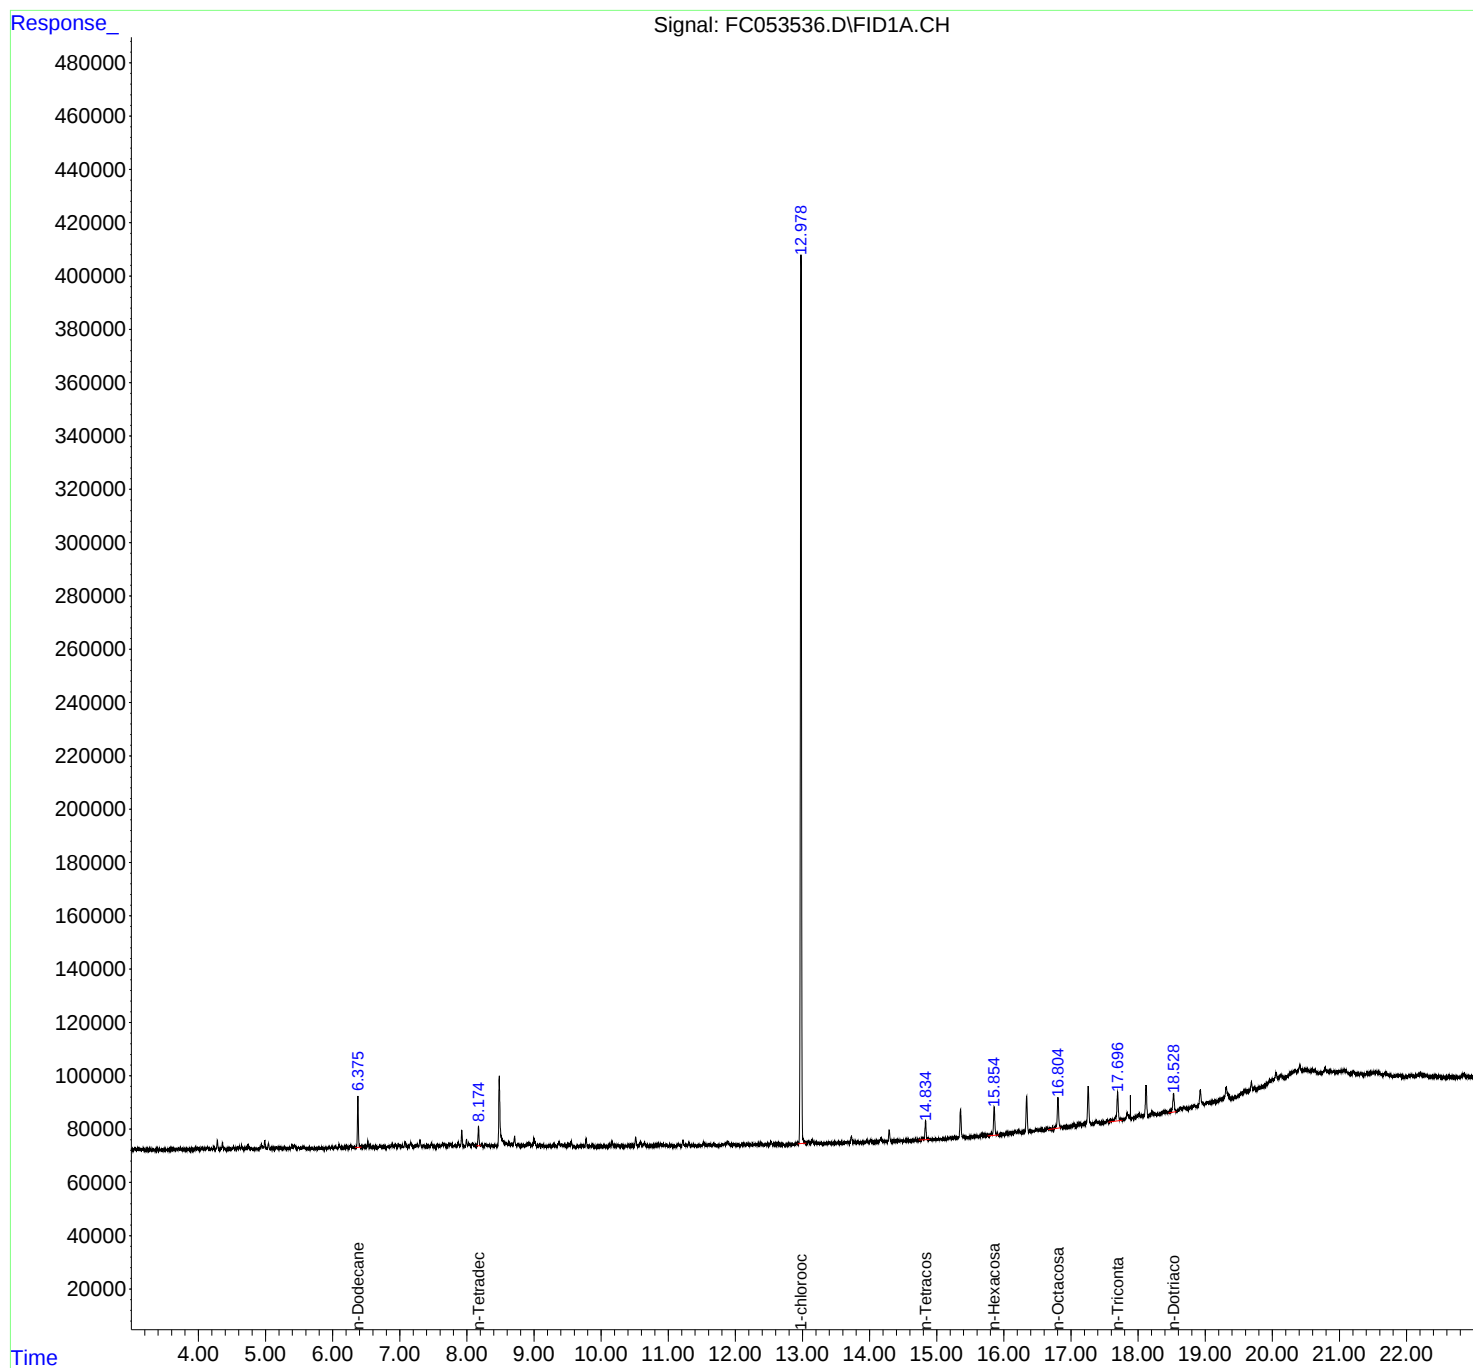


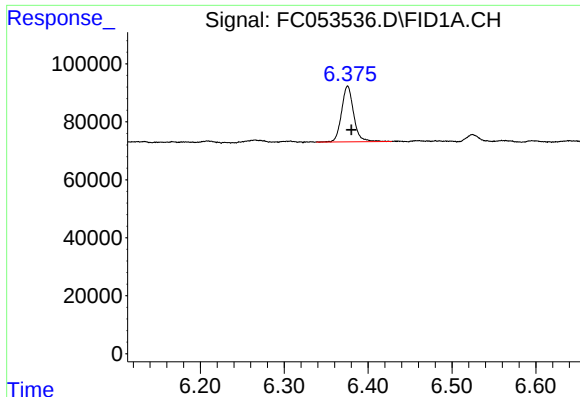

#4 n-Dodecane (C12)


R.T.: 6.376 min
Delta R.T.: -0.005 min
Response: 191427
Conc: 1.58 ug/ml

Instrument :
FID_C
ClientSampleId :

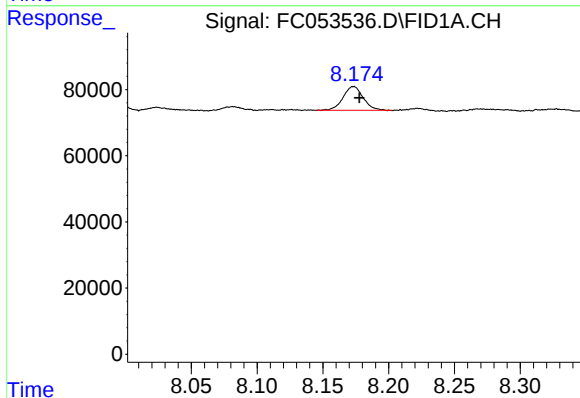


#6 n-Tetradecane (C14)

R.T.: 8.173 min
Delta R.T.: -0.005 min
Response: 76085
Conc: 0.62 ug/ml

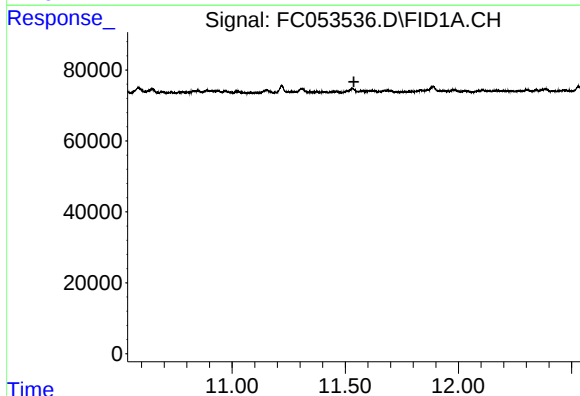


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.538 min
Response: 0
Conc: N.D.

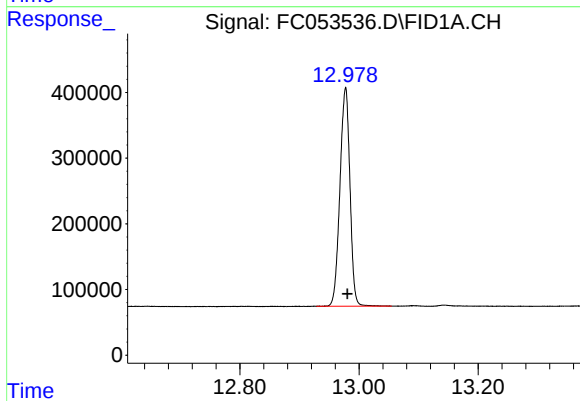

#12 1-chlorooctadecane (SURR)


R.T.: 12.977 min
Delta R.T.: -0.003 min
Response: 3881245
Conc: 34.80 ug/ml

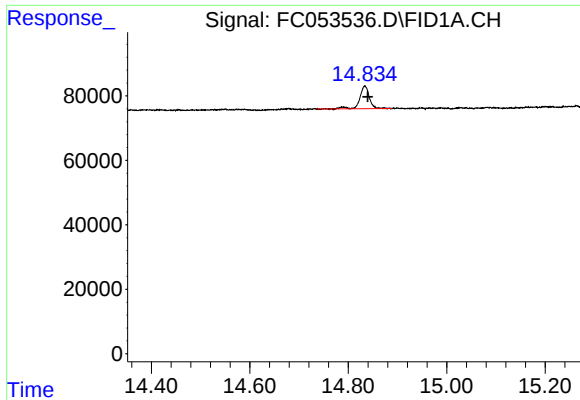

#14 n-Tetracosane (C24)


R.T.: 14.834 min
Delta R.T.: -0.006 min
Response: 95085
Conc: 0.71 ug/ml

Instrument :
FID_C
ClientSampleId :

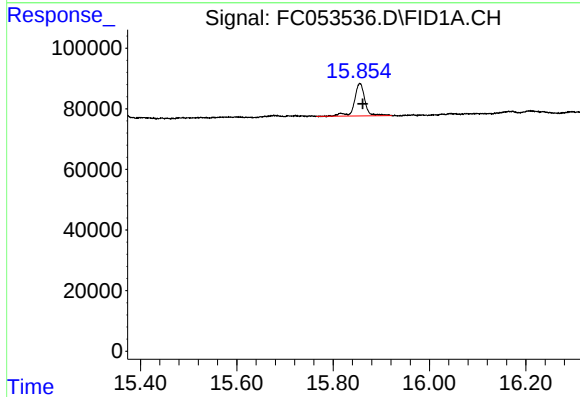


#15 n-Hexacosane (C26)

R.T.: 15.856 min
Delta R.T.: -0.006 min
Response: 161176
Conc: 1.22 ug/ml

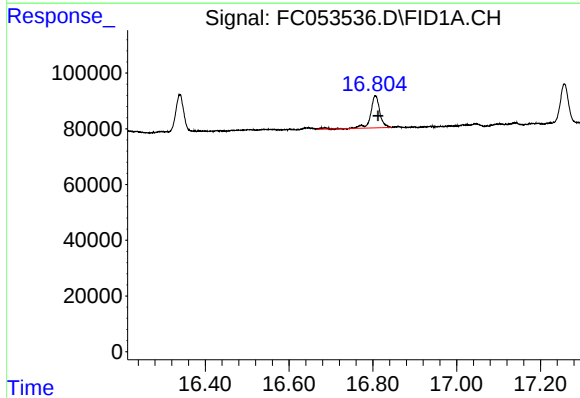


#16 n-Octacosane (C28)

R.T.: 16.806 min
Delta R.T.: -0.006 min
Response: 176233
Conc: 1.35 ug/ml

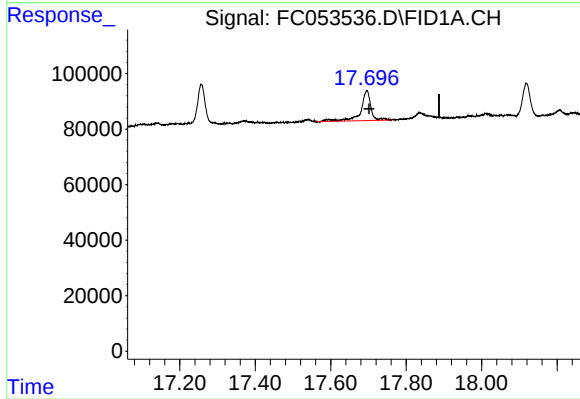

#17 n-Tricontane (C30)

R.T.: 17.696 min
Delta R.T.: -0.006 min
Response: 200567
Conc: 1.54 ug/ml

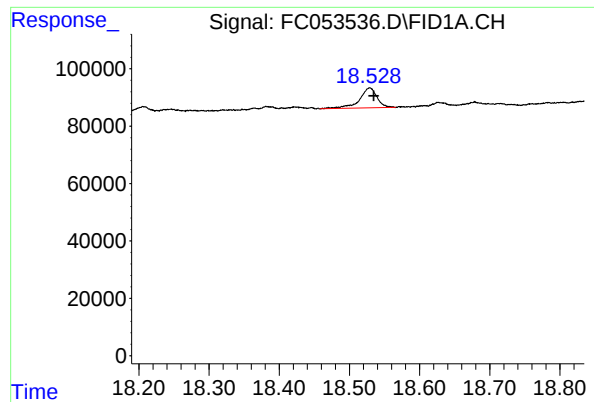

#18 n-Dotriacontane (C32)

R.T.: 18.529 min
Delta R.T.: -0.006 min
Response: 120452
Conc: 0.95 ug/ml

Instrument :
FID_C
ClientSampleId :