

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050622AL\
 Data File : FC059590.D
 Signal(s) : FID1A.CH
 Acq On : 06 May 2022 12:13
 Operator : UA/NP
 Sample : N2637-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 06 14:15:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050522.M
 Quant Title : GC Extractables
 QLast Update : Thu May 05 15:50:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.075	461032	4.006 ug/ml
Spiked Amount 50.000		Recovery =	8.01%
Target Compounds			
14) T n-Tetracosane (C24)	13.888	88475	0.703 ug/ml
15) T n-Hexacosane (C26)	14.886	119492	1.001 ug/ml
16) T n-Octacosane (C28)	15.816	264223	2.321 ug/ml
17) T n-Tricontane (C30)	16.683	225041	2.047 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050622AL\
Data File : FC059590.D
Signal(s) : FID1A.CH
Acq On : 06 May 2022 12:13
Operator : UA/NP
Sample : N2637-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 06 14:15:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050522.M
Quant Title : GC Extractables
QLast Update : Thu May 05 15:50:37 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

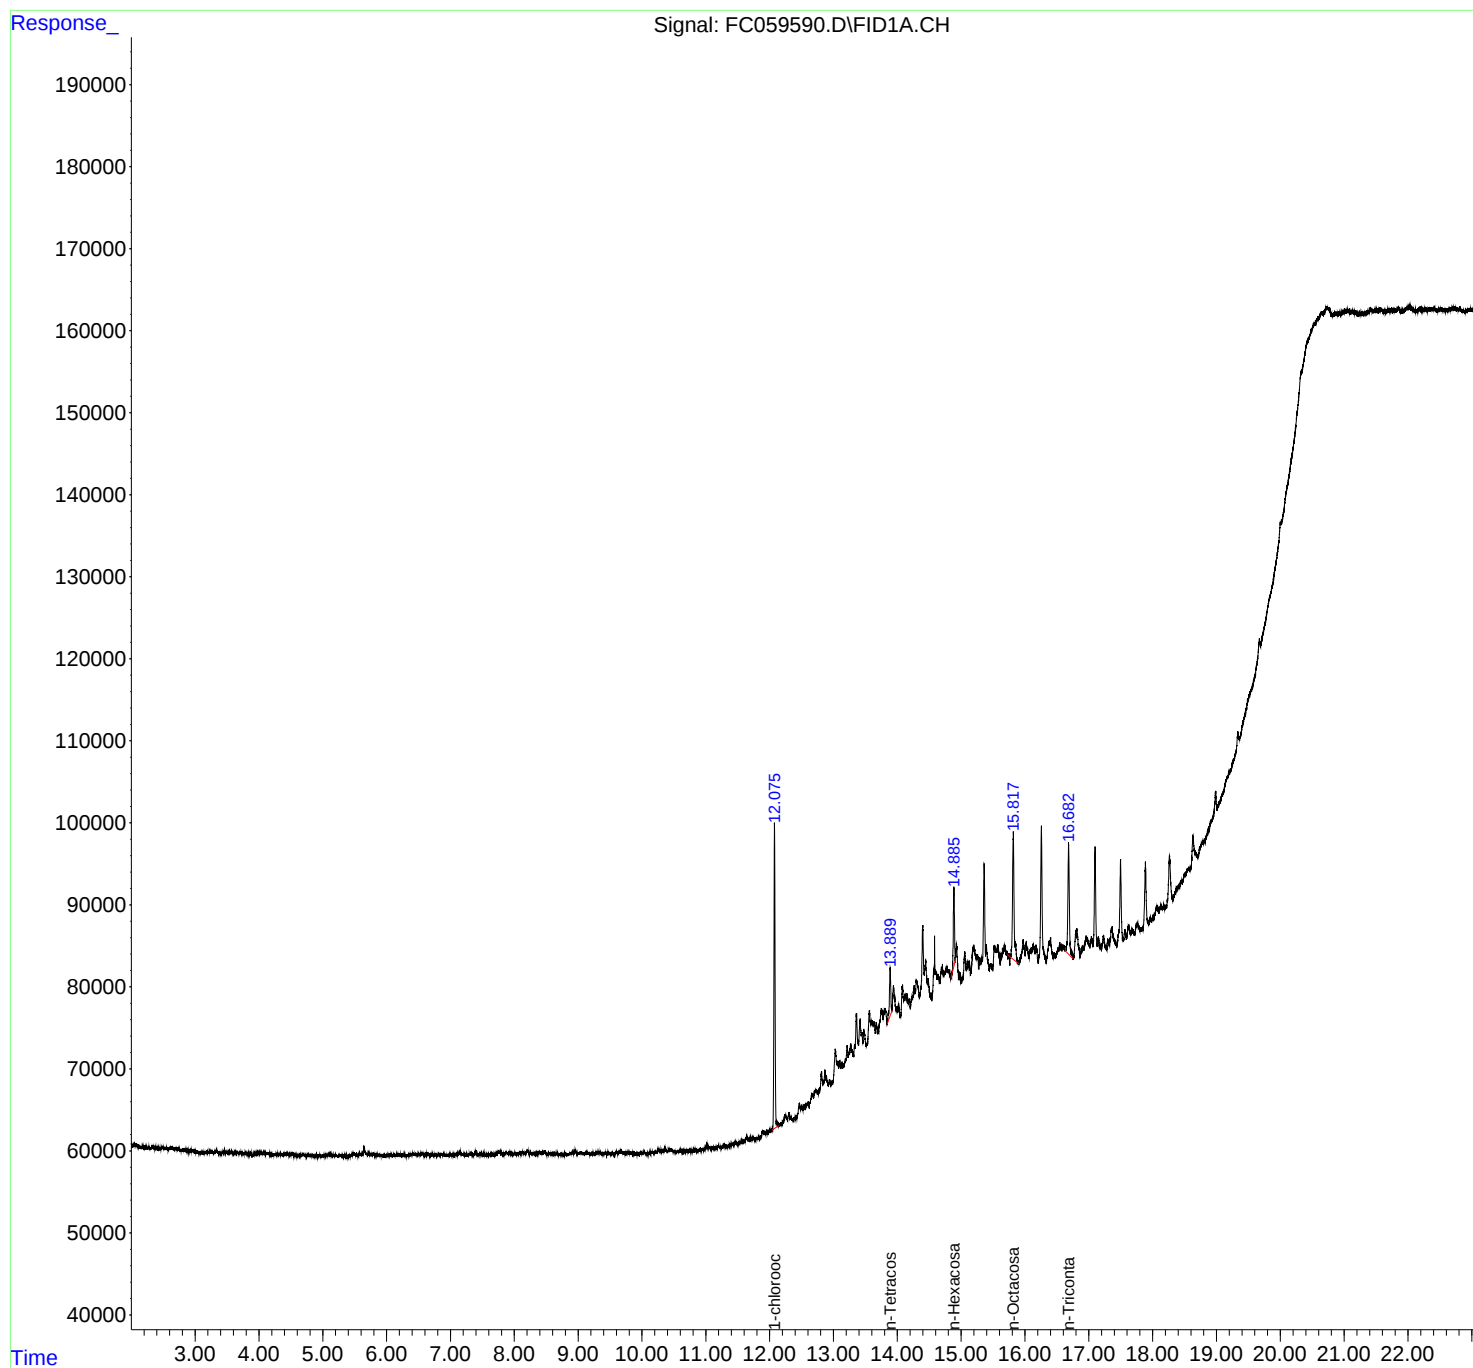


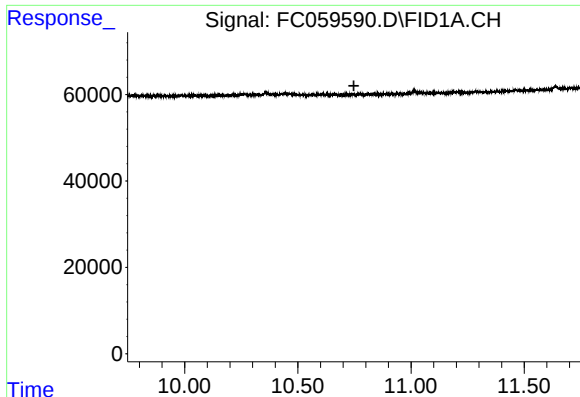

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.747 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

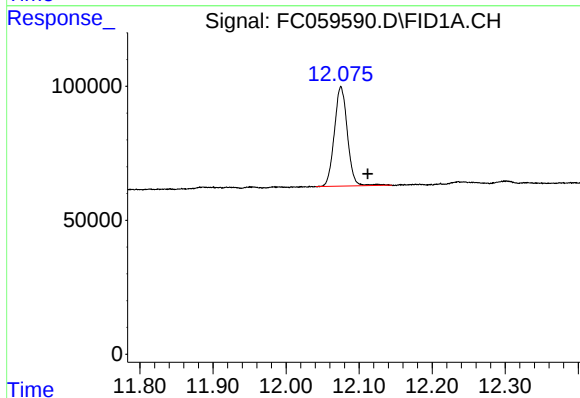


#12 1-chlorooctadecane (SURR)

R.T.: 12.075 min
Delta R.T.: -0.037 min
Response: 461032
Conc: 4.01 ug/ml

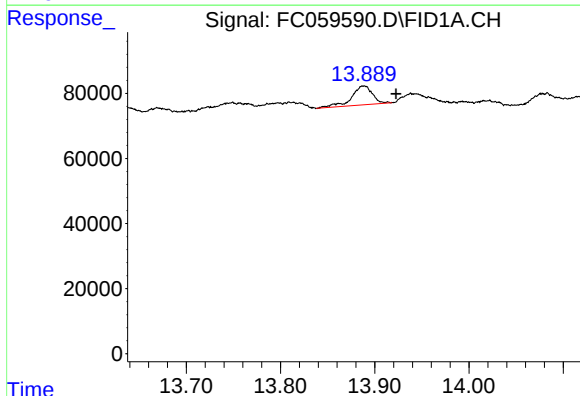


#14 n-Tetracosane (C24)

R.T.: 13.888 min
Delta R.T.: -0.034 min
Response: 88475
Conc: 0.70 ug/ml

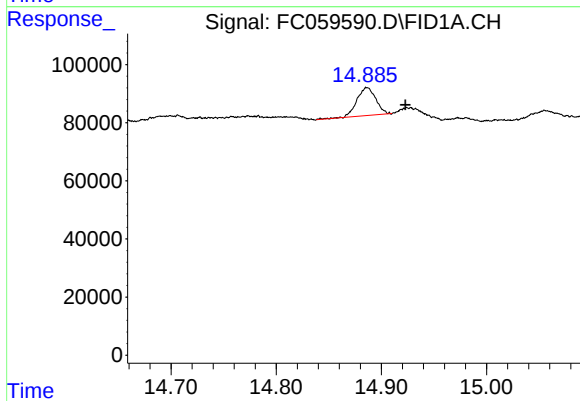

#15 n-Hexacosane (C26)


R.T.: 14.886 min
Delta R.T.: -0.037 min
Response: 119492
Conc: 1.00 ug/ml

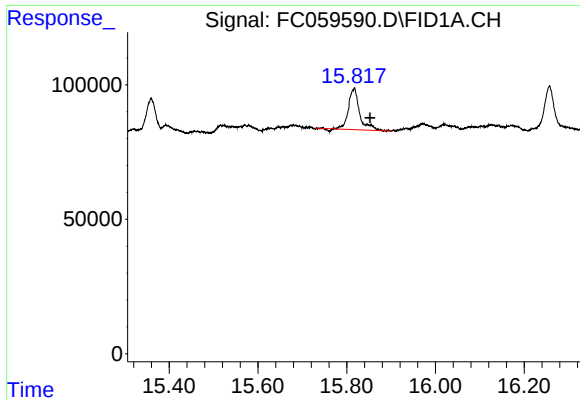

#16 n-Octacosane (C28)

R.T.: 15.816 min
Delta R.T.: -0.037 min
Response: 264223
Conc: 2.32 ug/ml

Instrument :
FID_C
ClientSampleId :

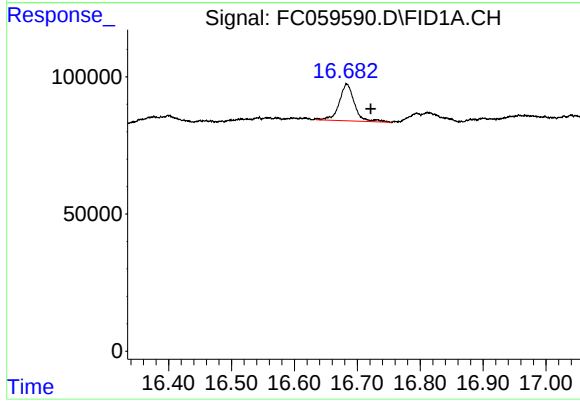

#17 n-Tricontane (C30)

R.T.: 16.683 min
Delta R.T.: -0.038 min
Response: 225041
Conc: 2.05 ug/ml