

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050724AL\
 Data File : FC066323.D
 Signal(s) : FID1A.ch
 Acq On : 07 May 2024 15:21
 Operator : YP/AJ
 Sample : P2390-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 08 02:35:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050124.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:03:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.003	5383441	43.889 ug/ml
Spiked Amount 50.000		Recovery =	87.78%
Target Compounds			
4) T n-Dodecane (C12)	6.406	85962	0.559 ug/ml
6) T n-Tetradecane (C14)	8.201	46002	0.304 ug/ml
14) T n-Tetracosane (C24)	14.856	66575	0.473 ug/ml
15) T n-Hexacosane (C26)	15.877	63131	0.462 ug/ml
16) T n-Octacosane (C28)	16.828	57125	0.427 ug/ml
17) T n-Tricontane (C30)	17.717	49276	0.366 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC050724AL\
Data File : FC066323.D
Signal(s) : FID1A.ch
Acq On : 07 May 2024 15:21
Operator : YP/AJ
Sample : P2390-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 08 02:35:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050124.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:03:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

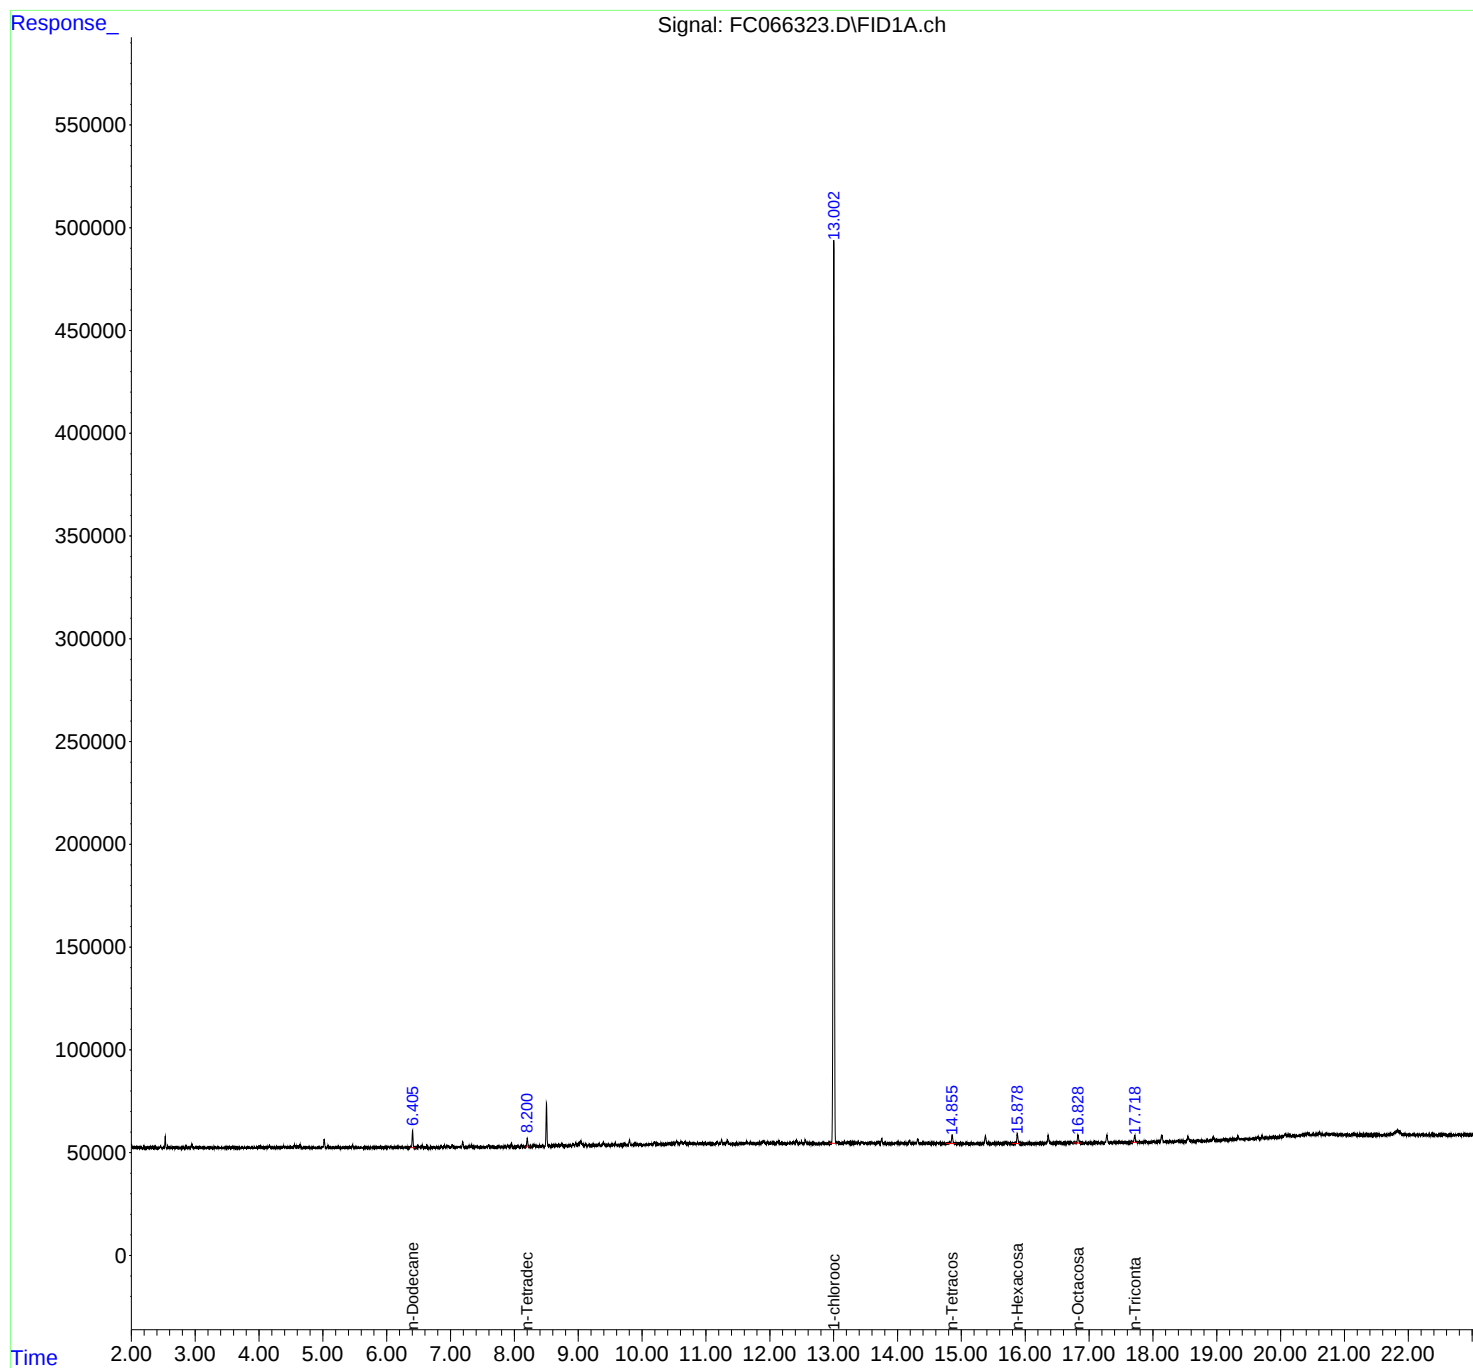


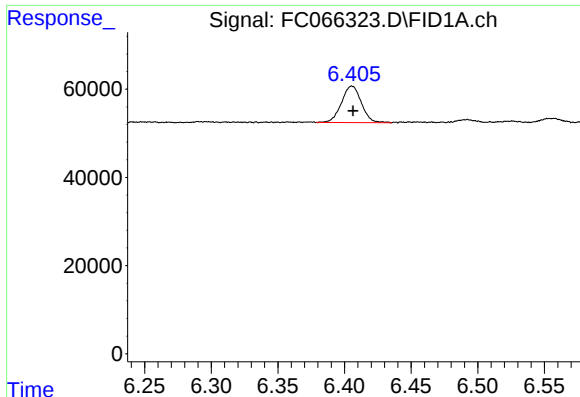

#4 n-Dodecane (C12)


R.T.: 6.406 min
Delta R.T.: 0.000 min
Response: 85962
Conc: 0.56 ug/ml

Instrument :
FID_C
ClientSampleId :

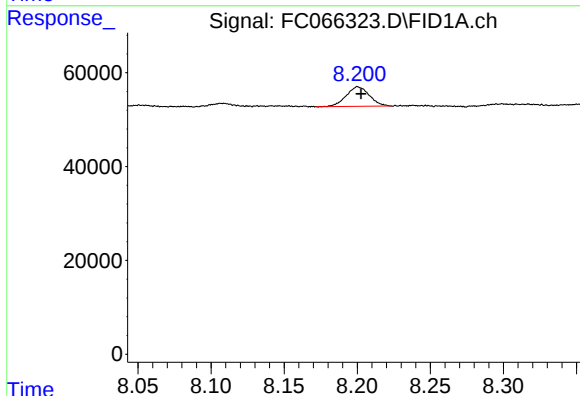


#6 n-Tetradecane (C14)

R.T.: 8.201 min
Delta R.T.: -0.002 min
Response: 46002
Conc: 0.30 ug/ml

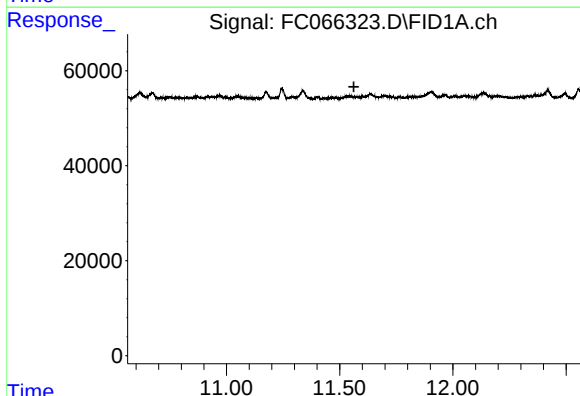


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.563 min
Response: 0
Conc: N.D.

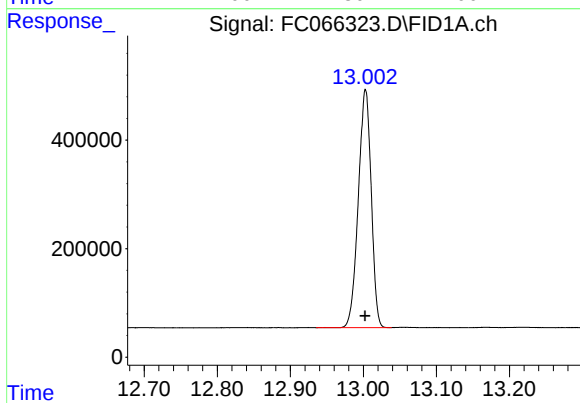

#12 1-chlorooctadecane (SURR)


R.T.: 13.003 min
Delta R.T.: 0.000 min
Response: 5383441
Conc: 43.89 ug/ml

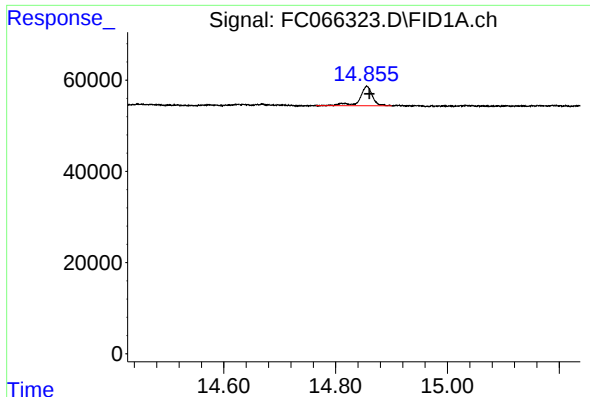

#14 n-Tetracosane (C24)


R.T.: 14.856 min
Delta R.T.: -0.004 min
Response: 66575
Conc: 0.47 ug/ml

Instrument :
FID_C
ClientSampleId :

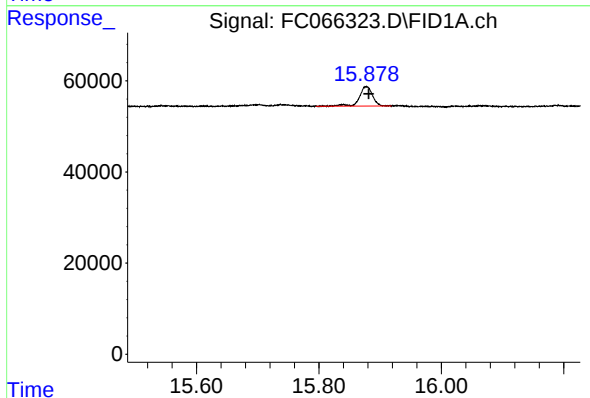


#15 n-Hexacosane (C26)

R.T.: 15.877 min
Delta R.T.: -0.004 min
Response: 63131
Conc: 0.46 ug/ml

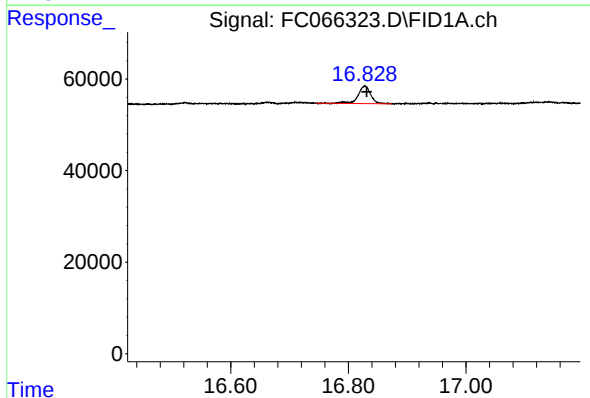

#16 n-Octacosane (C28)

R.T.: 16.828 min
Delta R.T.: -0.003 min
Response: 57125
Conc: 0.43 ug/ml

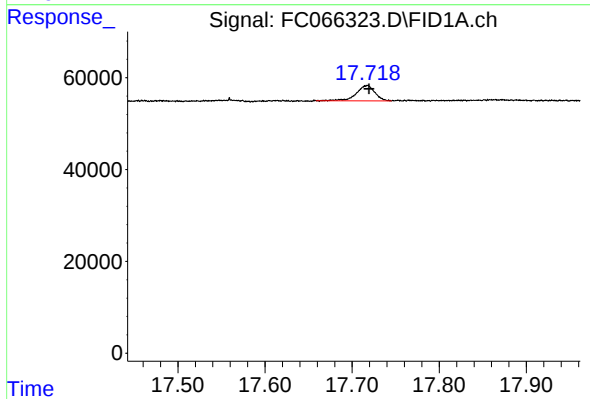

#17 n-Tricontane (C30)

R.T.: 17.717 min
Delta R.T.: -0.003 min
Response: 49276
Conc: 0.37 ug/ml