

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051021AL\
 Data File : FC053640.D
 Signal(s) : FID1A.CH
 Acq On : 10 May 2021 23:58
 Operator : DD\AJ
 Sample : M2335-01DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 11 03:23:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
 Quant Title : GC Extractables
 QLast Update : Tue May 04 11:44:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.530	876808	6.333 ug/ml
Spiked Amount 50.000		Recovery =	12.67%
12) S 1-chlorooctadecane (S...	12.972	752113	6.743 ug/ml
Spiked Amount 50.000		Recovery =	13.49%
Target Compounds			
10) T n-Eicosane (C20)	12.585	331129	2.502 ug/ml
14) T n-Tetracosane (C24)	14.809	193434	1.449 ug/ml
17) T n-Tricontane (C30)	17.693	66248	0.508 ug/ml
19) T n-Tetratriacontane (C34)	19.341	124119	1.019 ug/ml
21) T n-Octatriacontane (C38)	20.781	1514514	14.722 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051021AL\
Data File : FC053640.D
Signal(s) : FID1A.CH
Acq On : 10 May 2021 23:58
Operator : DD\AJ
Sample : M2335-01DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 11 03:23:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
Quant Title : GC Extractables
QLast Update : Tue May 04 11:44:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

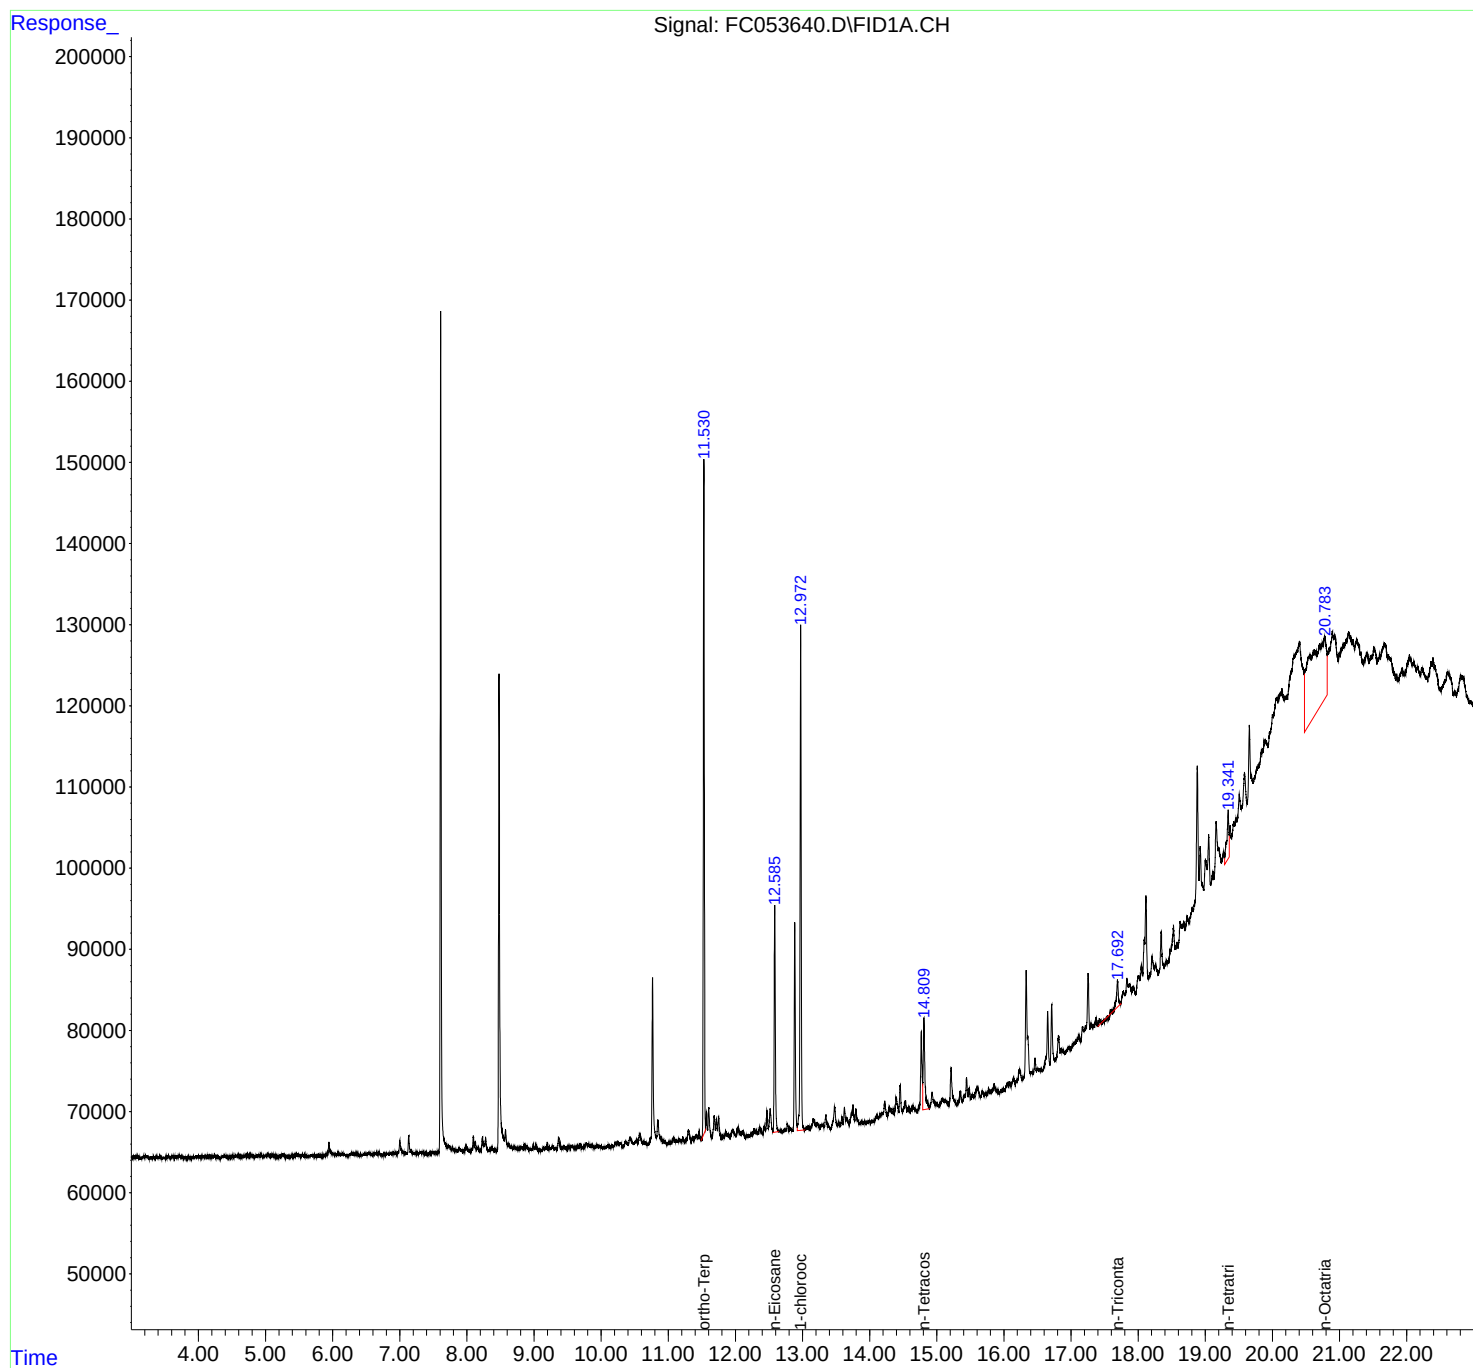


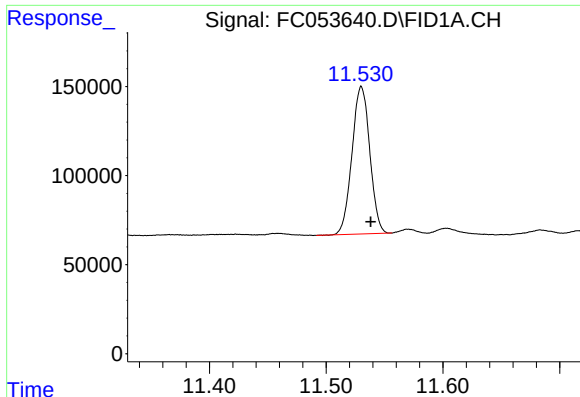

#9 ortho-Terphenyl (SURR)


R.T.: 11.530 min
Delta R.T.: -0.008 min
Response: 876808
Conc: 6.33 ug/ml

Instrument :
FID_C
ClientSampleId :

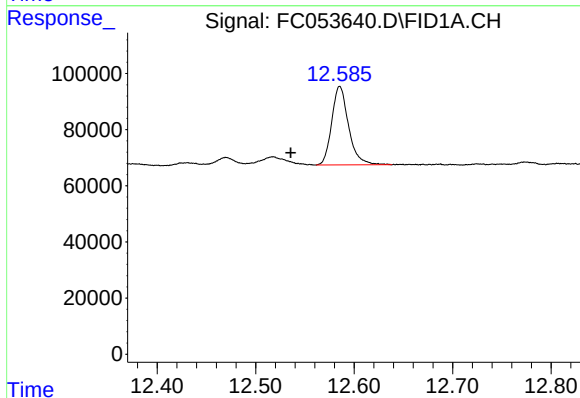


#10 n-Eicosane (C20)

R.T.: 12.585 min
Delta R.T.: 0.050 min
Response: 331129
Conc: 2.50 ug/ml

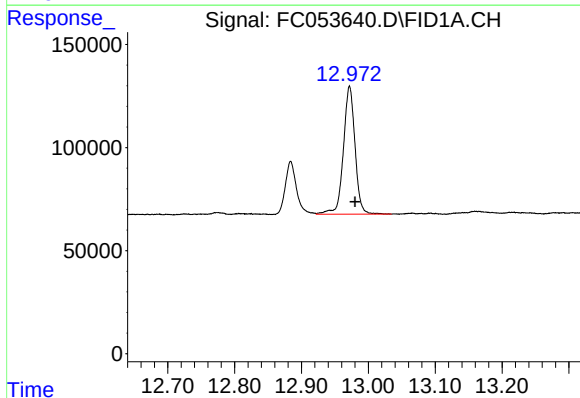


#12 1-chlorooctadecane (SURR)

R.T.: 12.972 min
Delta R.T.: -0.008 min
Response: 752113
Conc: 6.74 ug/ml

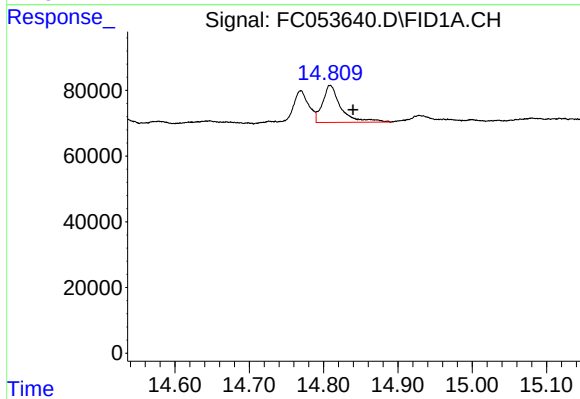

#14 n-Tetracosane (C24)


R.T.: 14.809 min
Delta R.T.: -0.030 min
Response: 193434
Conc: 1.45 ug/ml

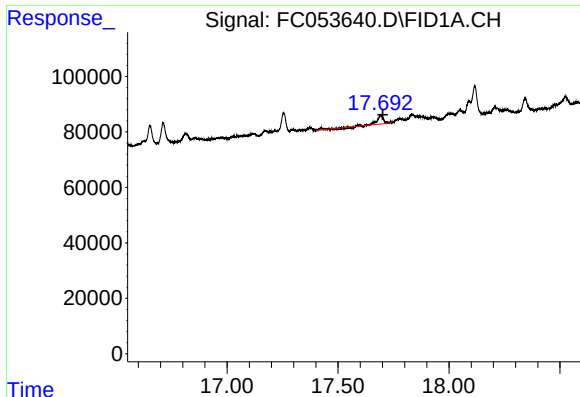

#17 n-Tricontane (C30)


R.T.: 17.693 min
Delta R.T.: -0.008 min
Response: 66248
Conc: 0.51 ug/ml

Instrument :
FID_C
ClientSampleId :

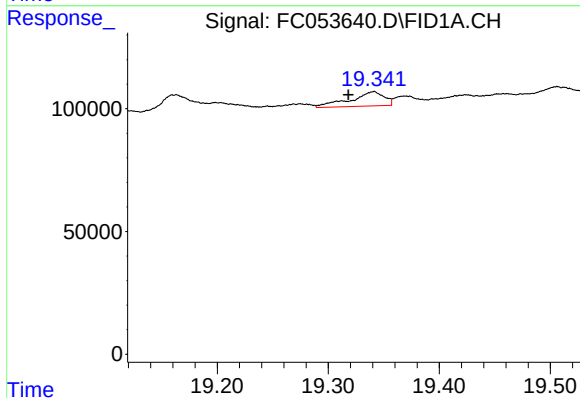

#19 n-Tetratriacontane (C34)

R.T.: 19.341 min
Delta R.T.: 0.022 min
Response: 124119
Conc: 1.02 ug/ml

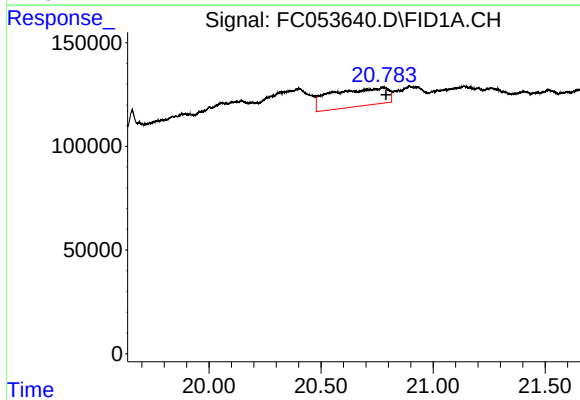

#21 n-Octatriacontane (C38)

R.T.: 20.781 min
Delta R.T.: -0.009 min
Response: 1514514
Conc: 14.72 ug/ml