

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051021AL\
 Data File : FC053642.D
 Signal(s) : FID1A.CH
 Acq On : 11 May 2021 1:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 11 03:24:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050321.M
 Quant Title : GC Extractables
 QLast Update : Tue May 04 11:44:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	13.679f	81908	0.616 ug/ml
14) T	n-Tetracosane (C24)	14.830	117117	0.877 ug/ml
15) T	n-Hexacosane (C26)	15.853	129123	0.977 ug/ml
16) T	n-Octacosane (C28)	16.804	154169	1.178 ug/ml
17) T	n-Tricontane (C30)	17.691	150168	1.151 ug/ml
18) T	n-Dotriacontane (C32)	18.526	150975	1.197 ug/ml
19) T	n-Tetratriacontane (C34)	19.310	131440	1.079 ug/ml
20) T	n-Hexatriacontane (C36)	20.050	547517	4.683 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051021AL\
Data File : FC053642.D
Signal(s) : FID1A.CH
Acq On : 11 May 2021 1:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :

Integration File: autoint1.e
Quant Time: May 11 03:24:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050321.M
Quant Title : GC Extractables
QLast Update : Tue May 04 11:44:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

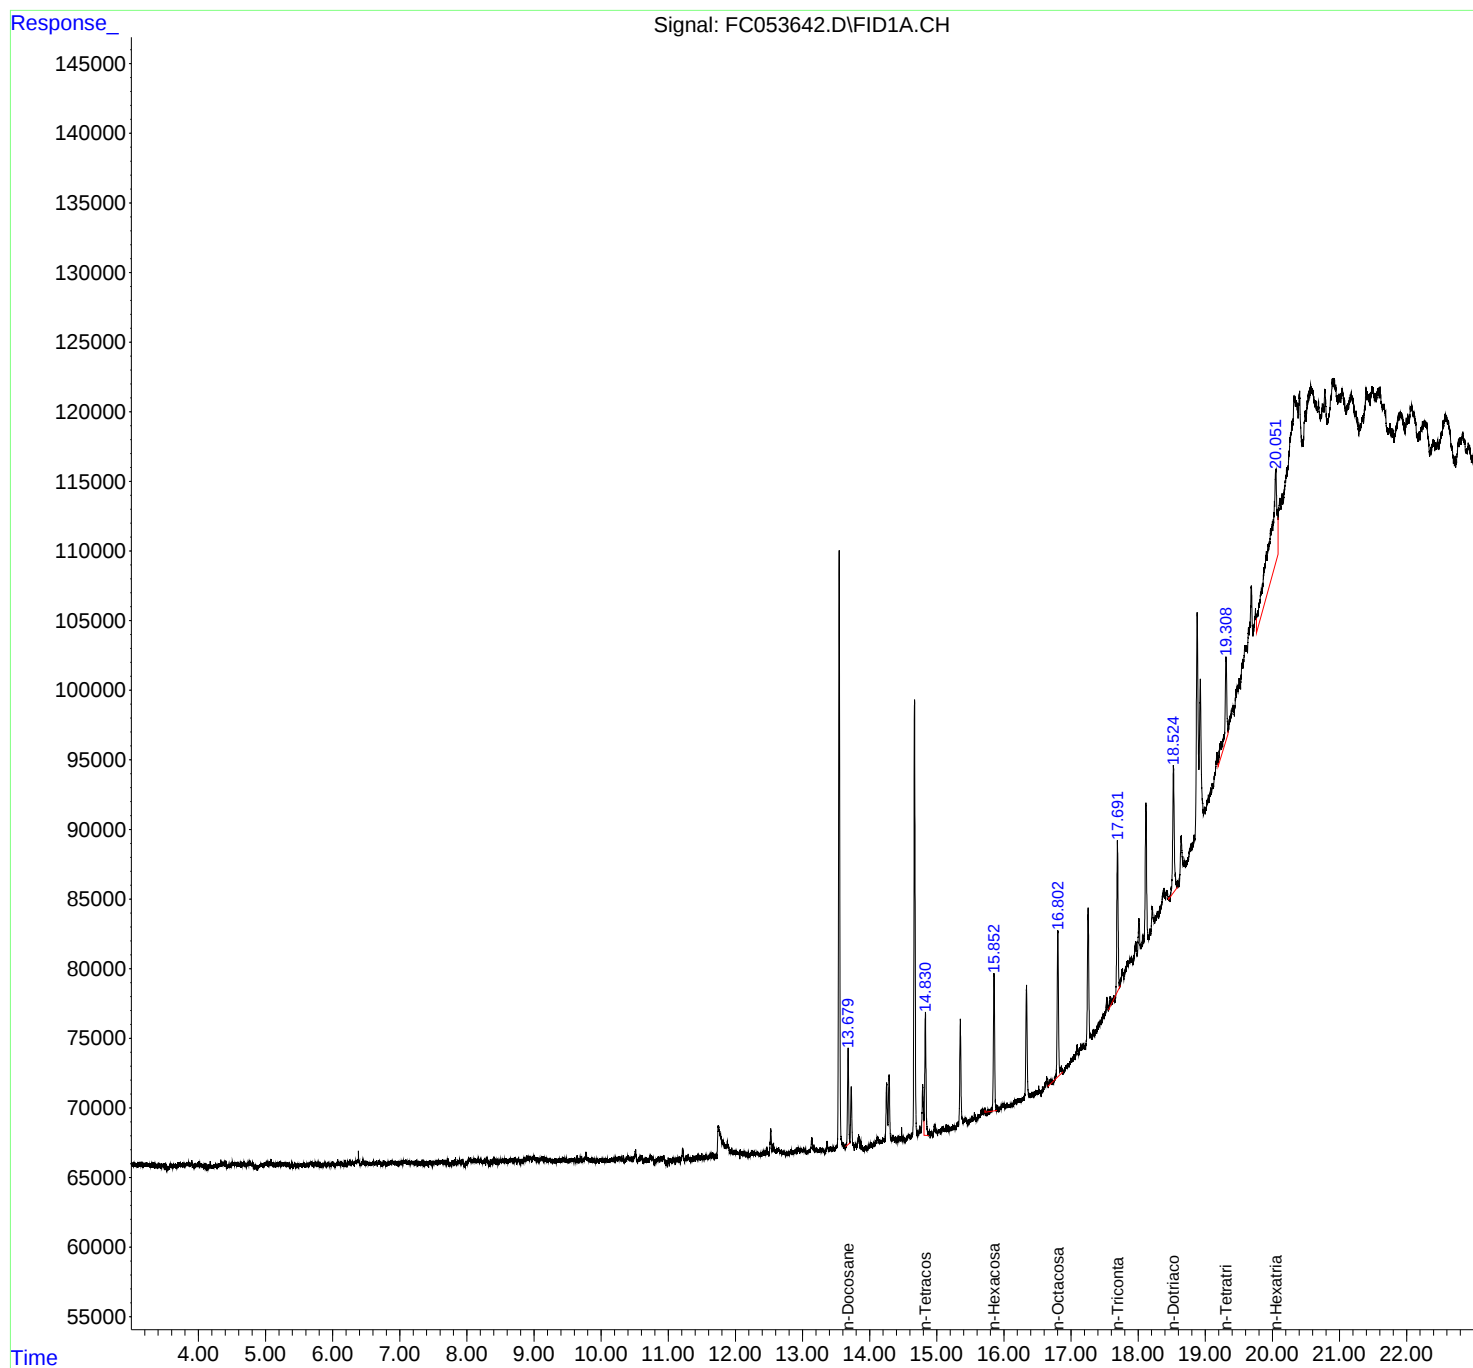


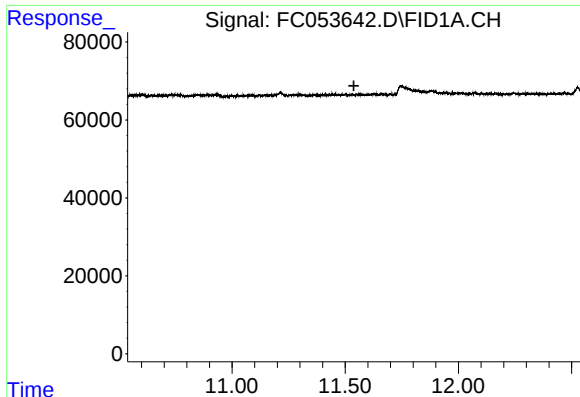

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.538 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

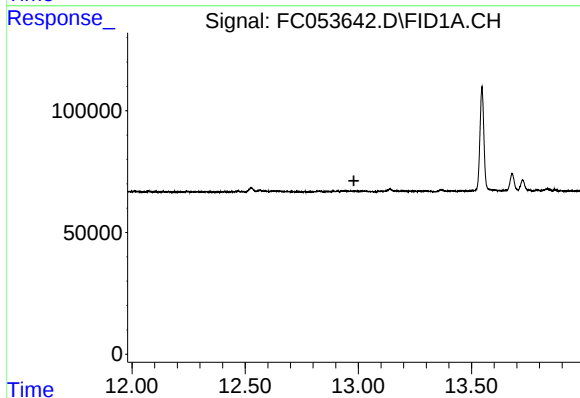


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.980 min
Response: 0
Conc: N.D.

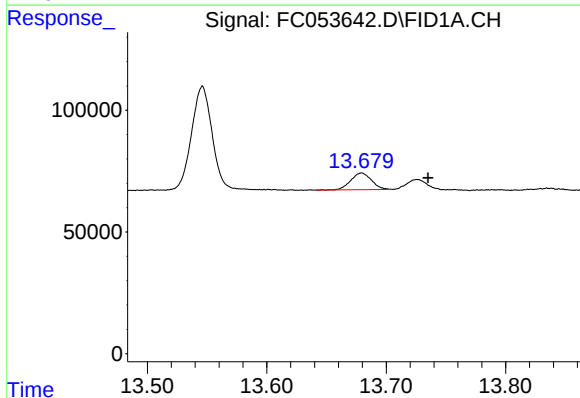


#13 n-Docosane (C22)

R.T.: 13.679 min
Delta R.T.: -0.056 min
Response: 81908
Conc: 0.62 ug/ml

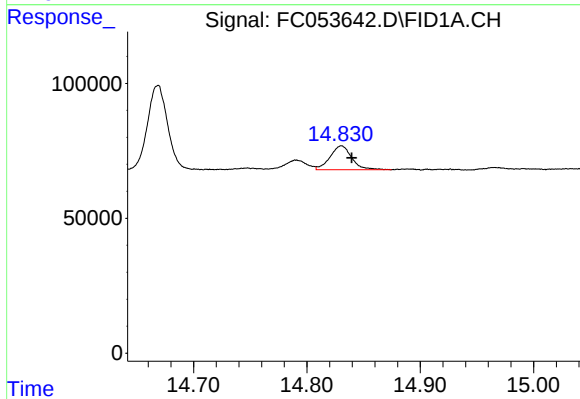

#14 n-Tetracosane (C24)


R.T.: 14.830 min
Delta R.T.: -0.009 min
Response: 117117
Conc: 0.88 ug/ml

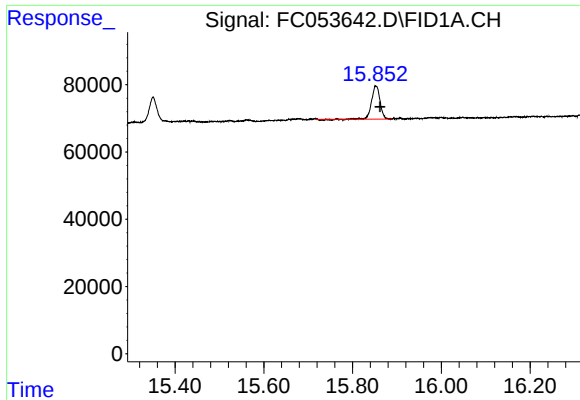

#15 n-Hexacosane (C26)


R.T.: 15.853 min
Delta R.T.: -0.009 min
Response: 129123
Conc: 0.98 ug/ml

Instrument :
FID_C
ClientSampleId :

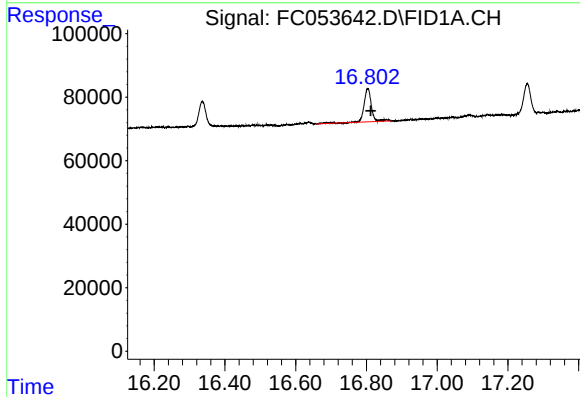


#16 n-Octacosane (C28)

R.T.: 16.804 min
Delta R.T.: -0.009 min
Response: 154169
Conc: 1.18 ug/ml

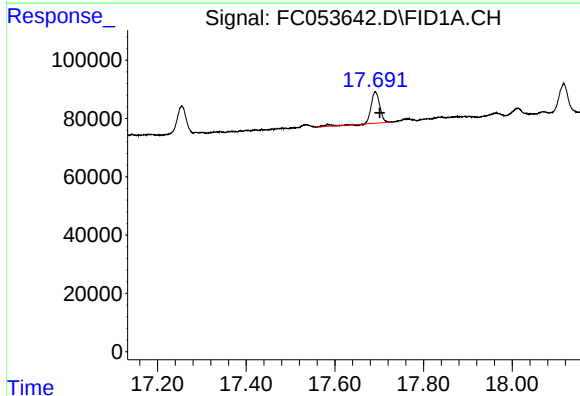


#17 n-Tricontane (C30)

R.T.: 17.691 min
Delta R.T.: -0.010 min
Response: 150168
Conc: 1.15 ug/ml

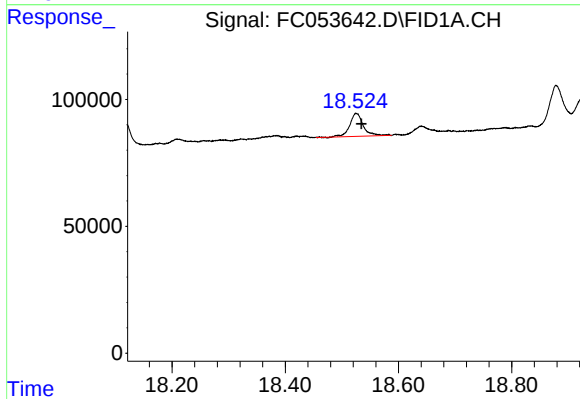

#18 n-Dotriacontane (C32)


R.T.: 18.526 min
Delta R.T.: -0.009 min
Response: 150975
Conc: 1.20 ug/ml

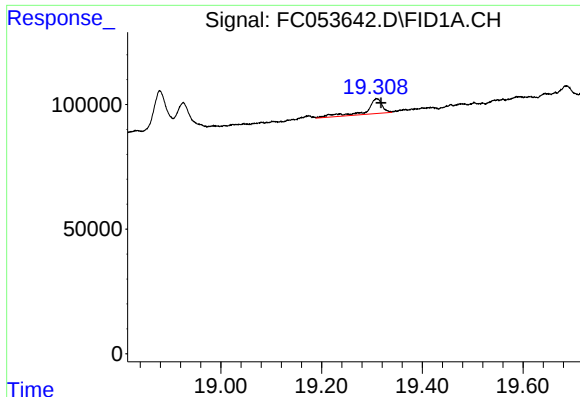

#19 n-Tetratriacontane (C34)

R.T.: 19.310 min
Delta R.T.: -0.009 min
Response: 131440
Conc: 1.08 ug/ml

Instrument :
FID_C
ClientSampleId :

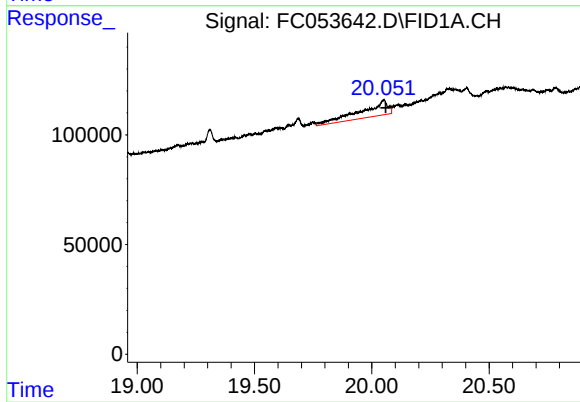

#20 n-Hexatriacontane (C36)

R.T.: 20.050 min
Delta R.T.: -0.009 min
Response: 547517
Conc: 4.68 ug/ml