

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC051420AL\  
 Data File : FC047449.D  
 Signal(s) : FID1A.CH  
 Acq On : 15 May 2020 2:39  
 Operator : DD\AJ  
 Sample : L2636-02D  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 AST-2

Integration File: autoint1.e  
 Quant Time: May 15 07:23:10 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Alaphatic EPH 050820.M  
 Quant Title : GC Extractables  
 QLast Update : Fri May 08 16:49:27 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 12) S 1-chlorooctadecane (S... | 13.157 | 1245123    | 12.695 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 25.39%       |
| Target Compounds               |        |            |              |
| -----                          |        |            |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC051420AL\  
Data File : FC047449.D  
Signal(s) : FID1A.CH  
Acq On : 15 May 2020 2:39  
Operator : DD\AJ  
Sample : L2636-02D  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
AST-2

Integration File: autoint1.e  
Quant Time: May 15 07:23:10 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Alaphatic EPH 050820.M  
Quant Title : GC Extractables  
QLast Update : Fri May 08 16:49:27 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

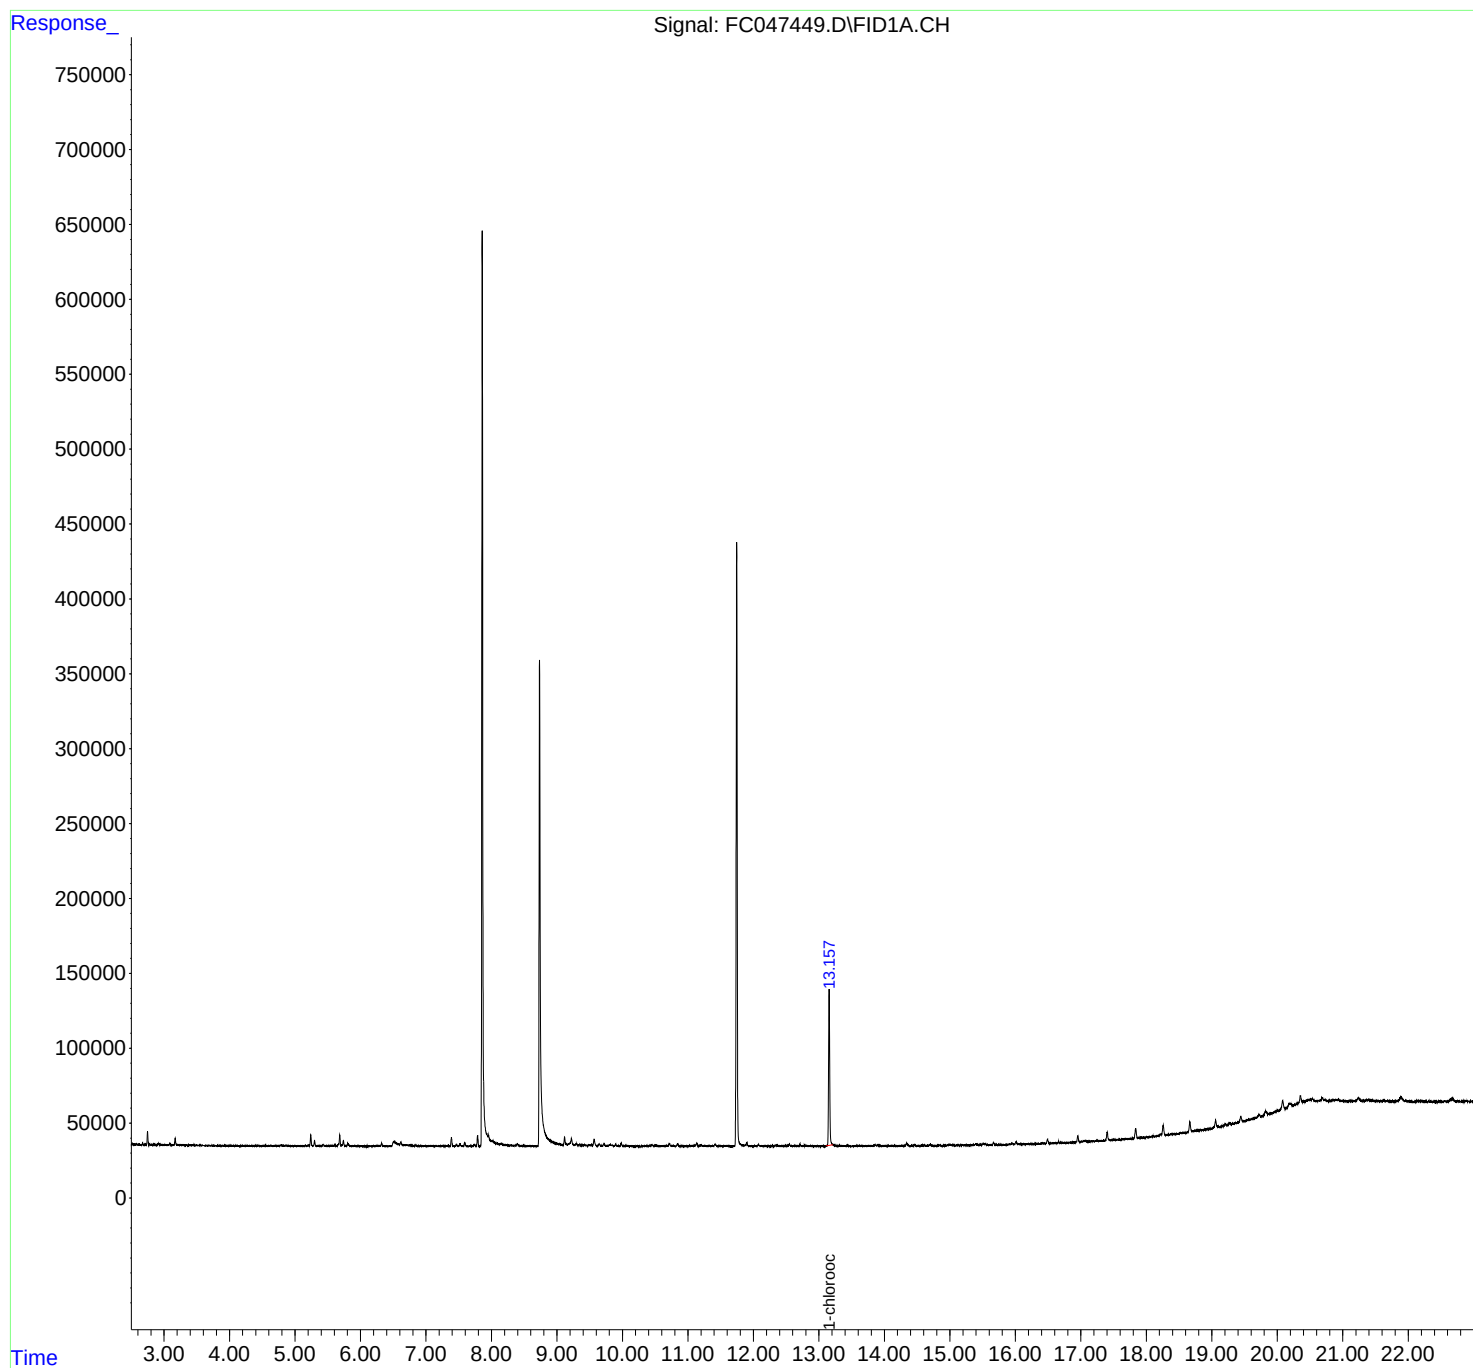


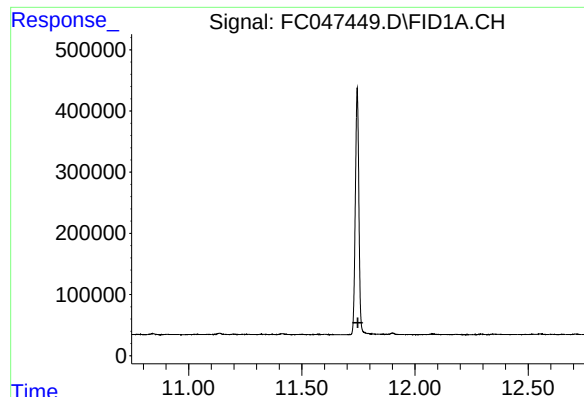

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.748 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
AST-2

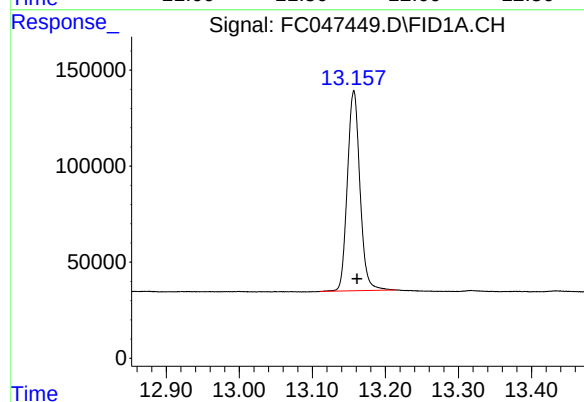

#12 1-chlorooctadecane (SURR)

R.T.: 13.157 min  
Delta R.T.: -0.004 min  
Response: 1245123  
Conc: 12.69 ug/ml