

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051923AL\
 Data File : FC063662.D
 Signal(s) : FID1A.ch
 Acq On : 20 May 2023 13:48
 Operator : YP/AJ
 Sample : 02837-02DL2 250X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 21 01:52:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050523.M
 Quant Title : GC Extractables
 QLast Update : Fri May 05 18:15:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.561	129656	0.692 ug/ml
Spiked Amount 50.000		Recovery =	1.38%
Target Compounds			
6) T n-Tetradecane (C14)	8.183	338451	2.143 ug/ml
7) T n-Hexadecane (C16)	9.780	166926	1.041 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC051923AL\
Data File : FC063662.D
Signal(s) : FID1A.ch
Acq On : 20 May 2023 13:48
Operator : YP/AJ
Sample : 02837-02DL2 250X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 21 01:52:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050523.M
Quant Title : GC Extractables
QLast Update : Fri May 05 18:15:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

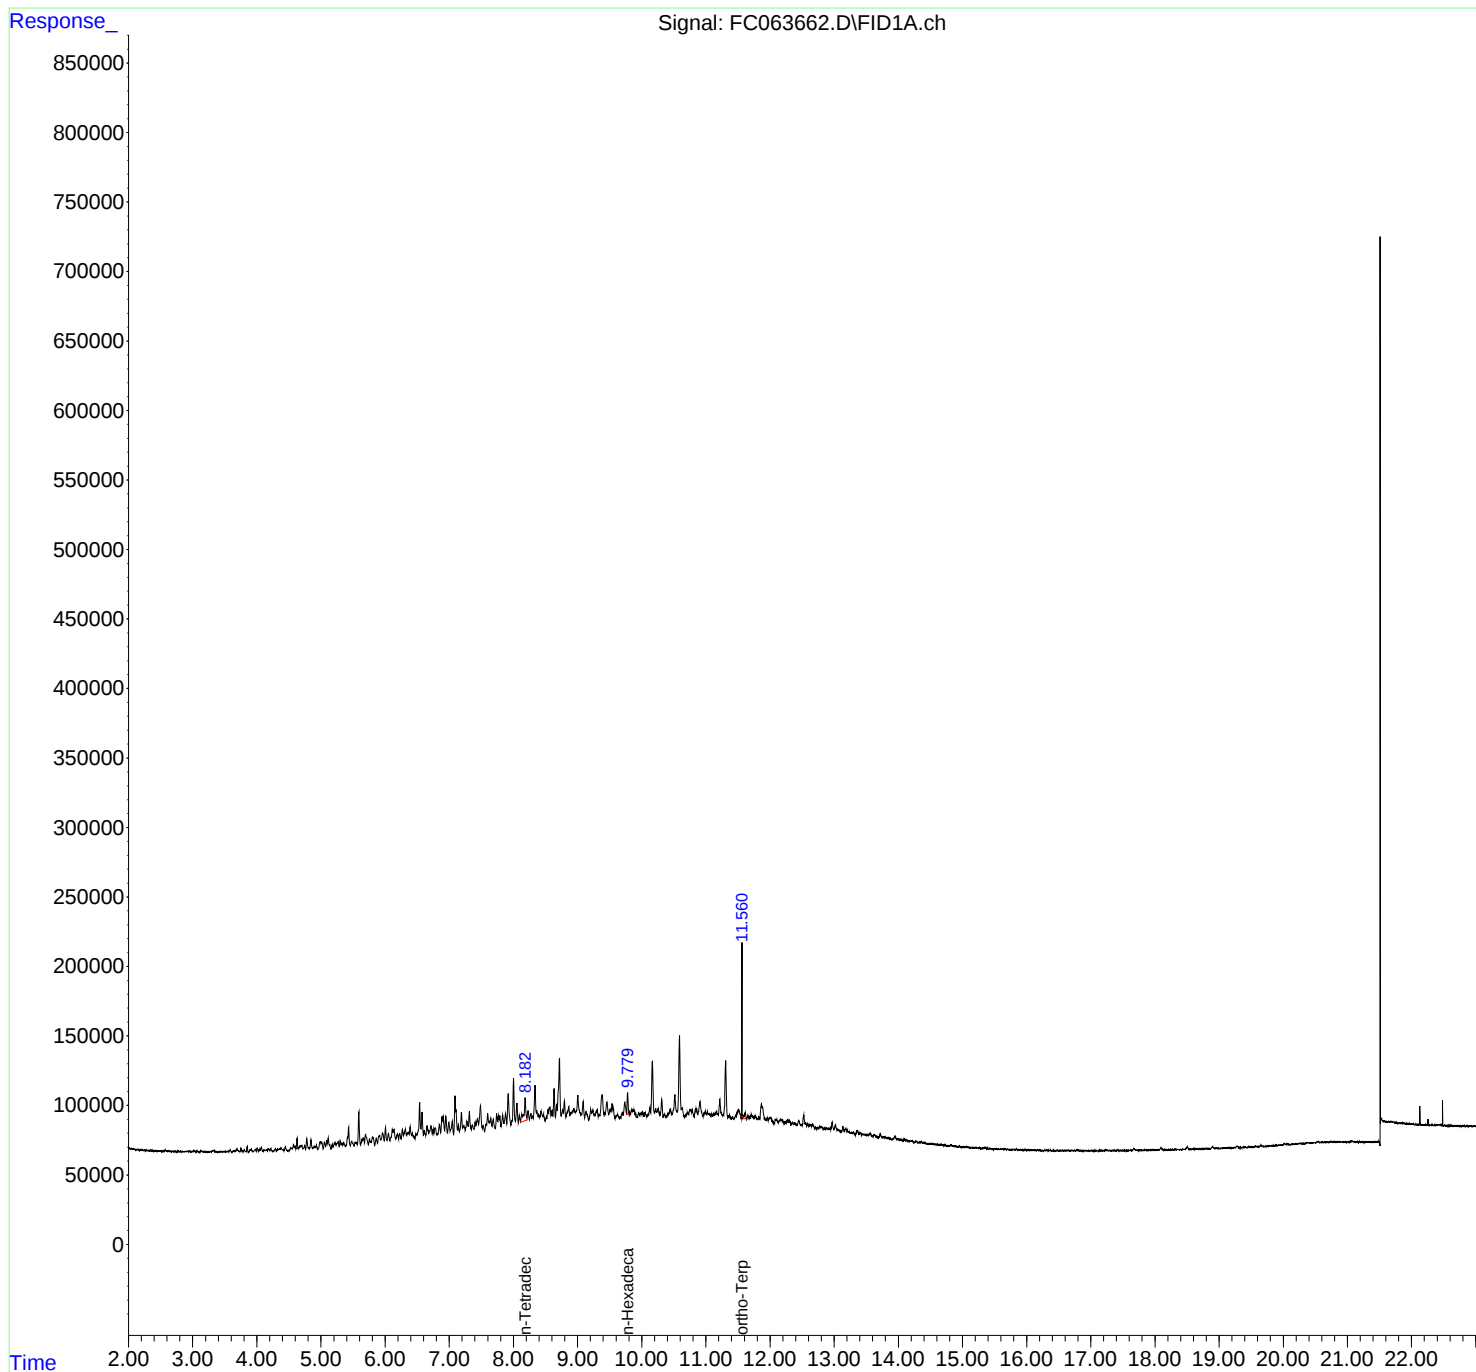


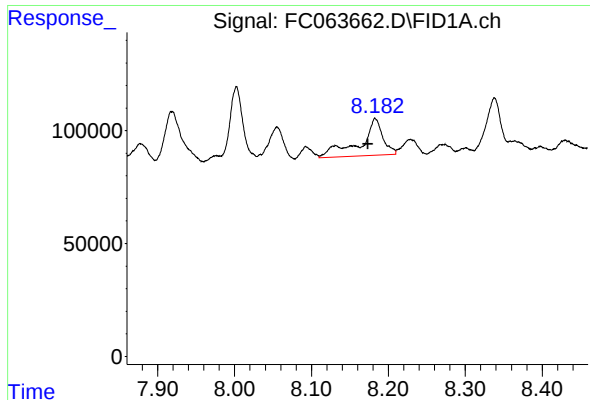

#6 n-Tetradecane (C14)


R.T.: 8.183 min
Delta R.T.: 0.009 min
Response: 338451
Conc: 2.14 ug/ml

Instrument :
FID_C
ClientSampleId :

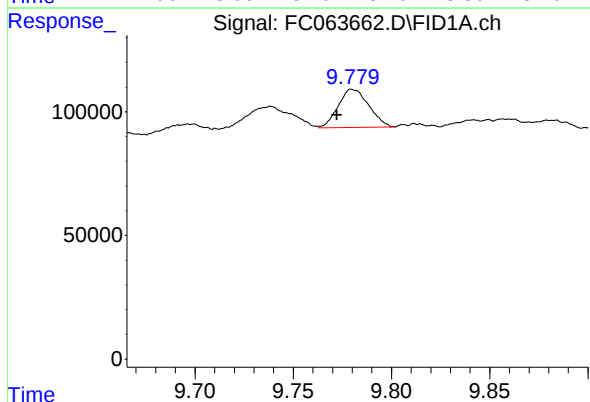


#7 n-Hexadecane (C16)

R.T.: 9.780 min
Delta R.T.: 0.008 min
Response: 166926
Conc: 1.04 ug/ml

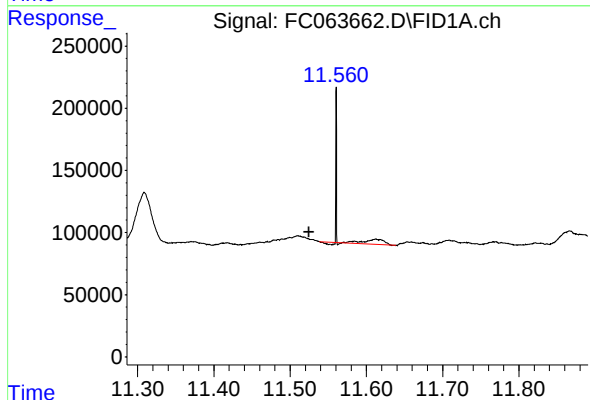

#9 ortho-Terphenyl (SURR)

R.T.: 11.561 min
Delta R.T.: 0.036 min
Response: 129656
Conc: 0.69 ug/ml

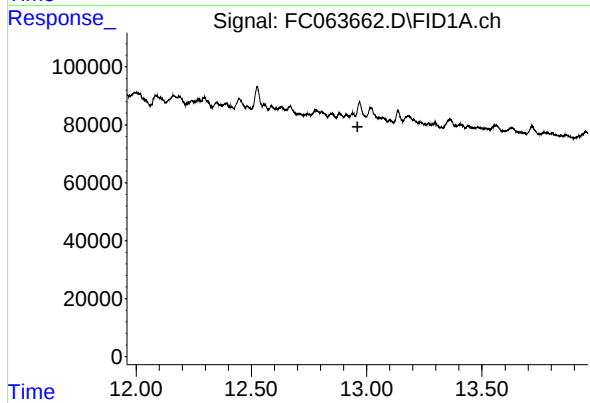

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.960 min
Response: 0
Conc: N.D.