

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC052122AL\
 Data File : FC059873.D
 Signal(s) : FID1A.CH
 Acq On : 21 May 2022 10:23
 Operator : UA/NP
 Sample : N2942-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 RATZER-RD-SP-1-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/23/2022
 Supervised By :Ankita Jodhani 05/23/2022

Integration File: sample.E
 Quant Time: May 23 01:00:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050522.M
 Quant Title : GC Extractables
 QLast Update : Mon May 09 11:12:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.647	5029094	34.247 ug/mlm
Spiked Amount	50.000	Recovery	= 68.49%
12) S 1-chlorooctadecane (S...	12.019	4108088	35.698 ug/ml
Spiked Amount	50.000	Recovery	= 71.40%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC052122AL\
Data File : FC059873.D
Signal(s) : FID1A.CH
Acq On : 21 May 2022 10:23
Operator : UA/NP
Sample : N2942-04
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
RATZER-RD-SP-1-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

Integration File: sample.E
Quant Time: May 23 01:00:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 050522.M
Quant Title : GC Extractables
QLast Update : Mon May 09 11:12:42 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

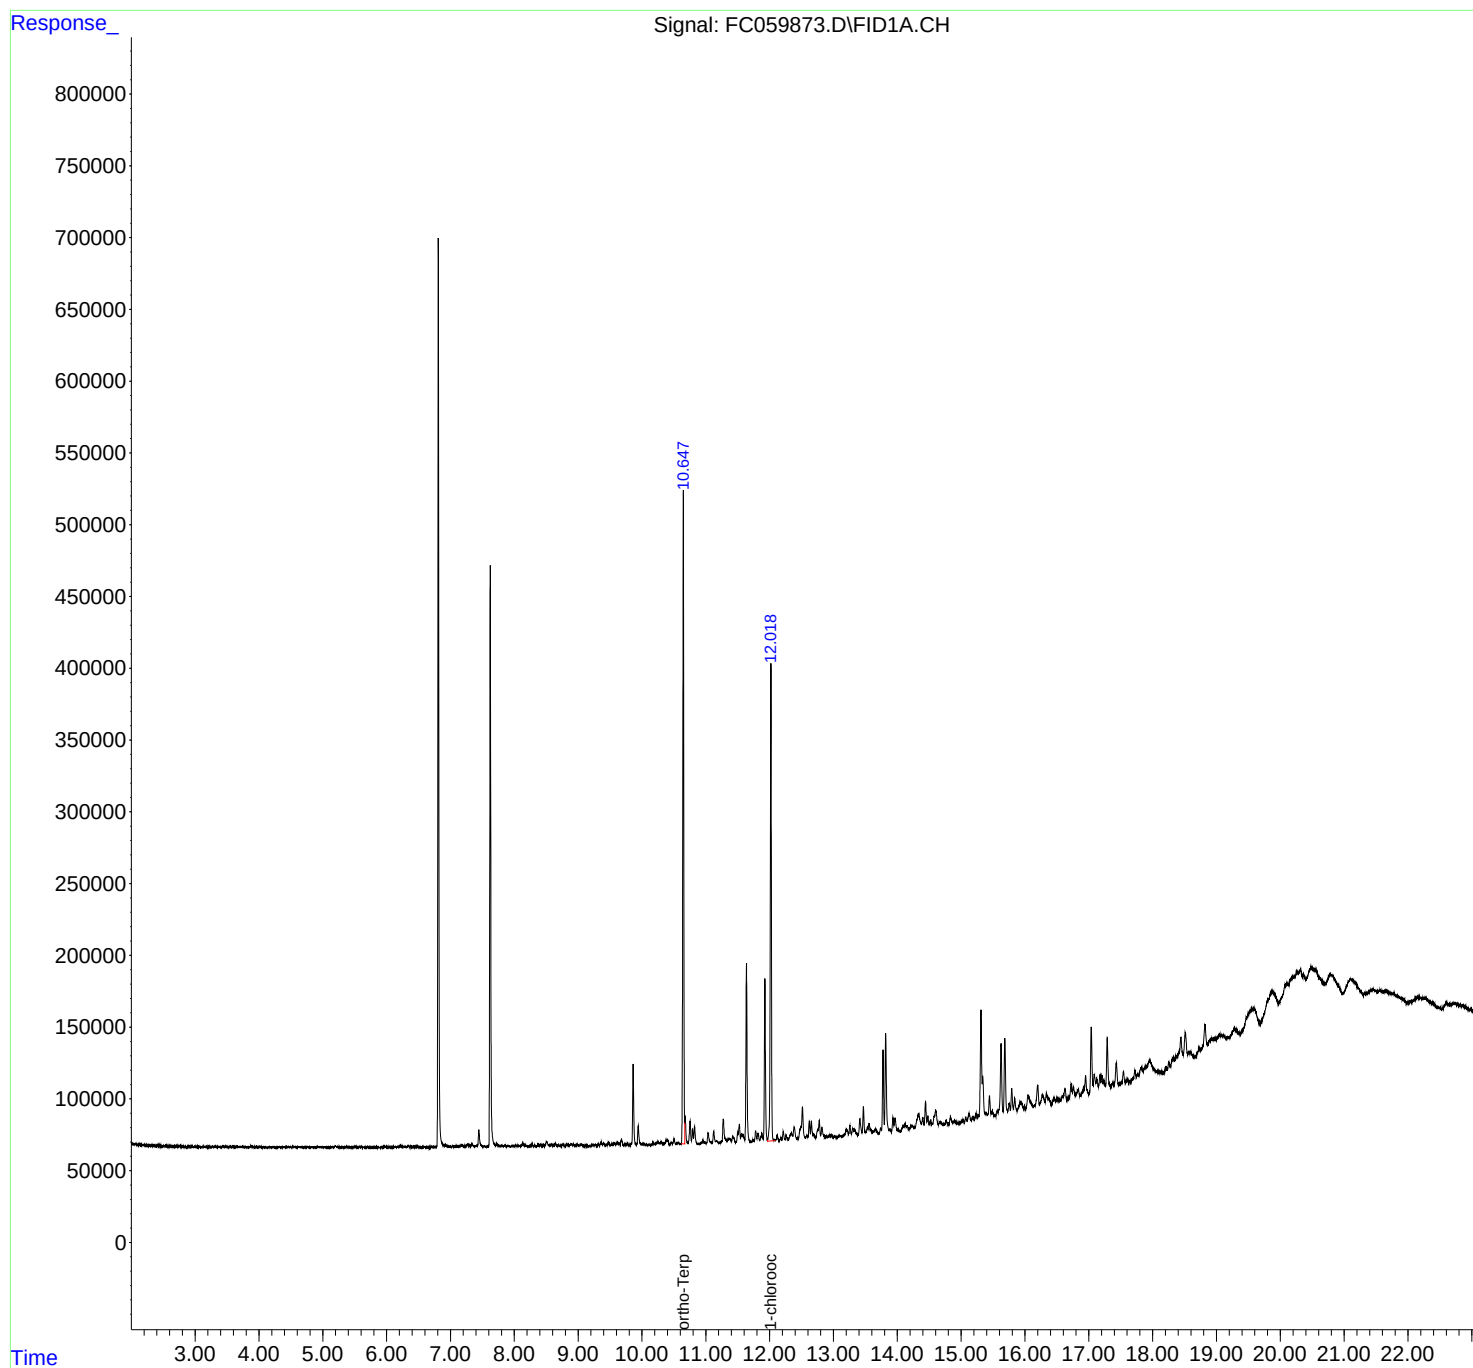

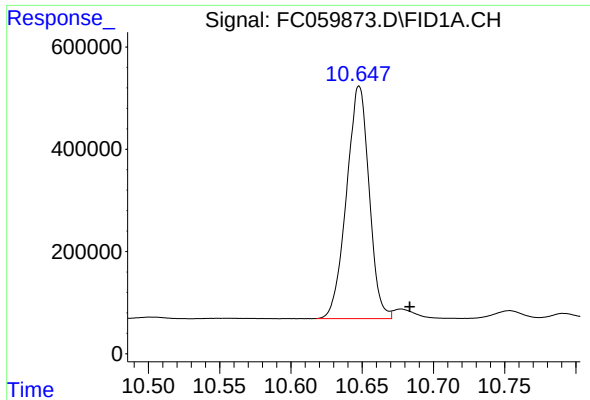


#9 ortho-Terphenyl (SURR)

R.T.: 10.647 min
Delta R.T.: -0.036 min
Response: 5029094
Conc: 34.25 ug/ml

Instrument :
FID_C
ClientSampleId :
RATZER-RD-SP-1-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/23/2022

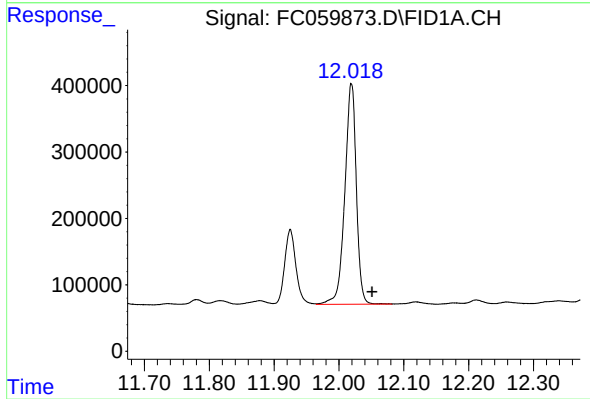

#12 1-chlorooctadecane (SURR)

R.T.: 12.019 min
Delta R.T.: -0.032 min
Response: 4108088
Conc: 35.70 ug/ml