

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC052620AL\
 Data File : FC047578.D
 Signal(s) : FID1A.CH
 Acq On : 26 May 2020 8:42
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: May 27 02:12:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050820.M
 Quant Title : GC Extractables
 QLast Update : Fri May 08 16:49:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
20) T n-Hexatriacontane (C36)	20.193	122183	1.409 ug/ml
22) T n-Tetracontane (C40)	21.876	184441	2.268 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC052620AL\
Data File : FC047578.D
Signal(s) : FID1A.CH
Acq On : 26 May 2020 8:42
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: May 27 02:12:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 050820.M
Quant Title : GC Extractables
QLast Update : Fri May 08 16:49:27 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

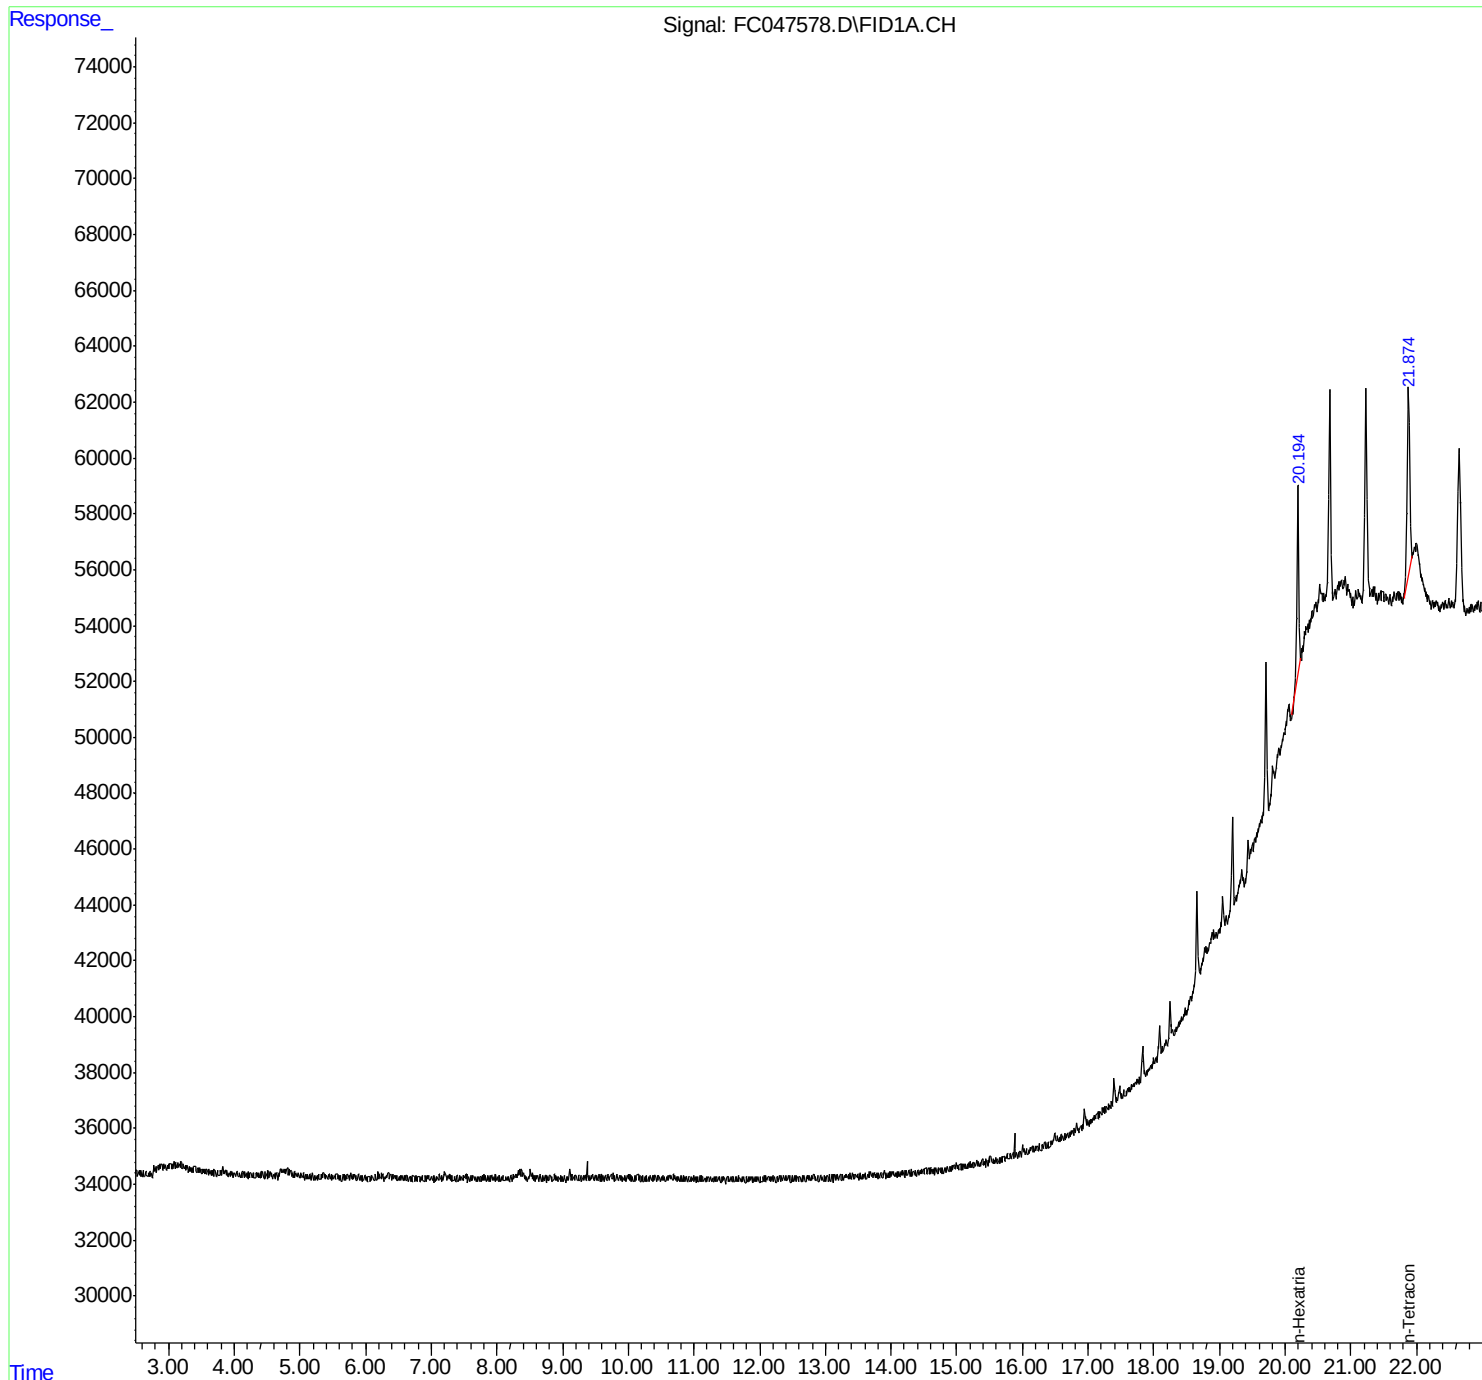


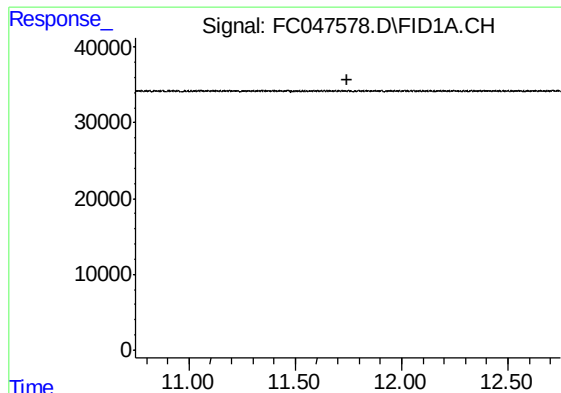

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.748 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
MECL2

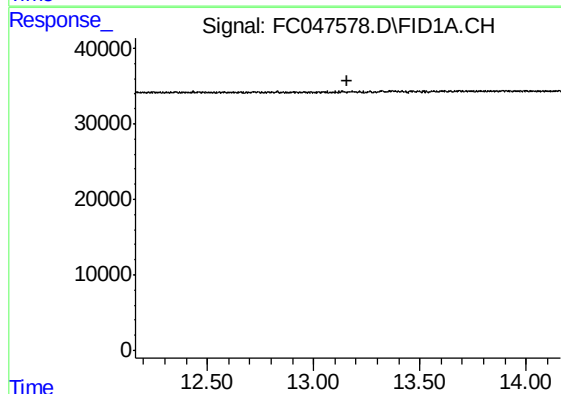


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

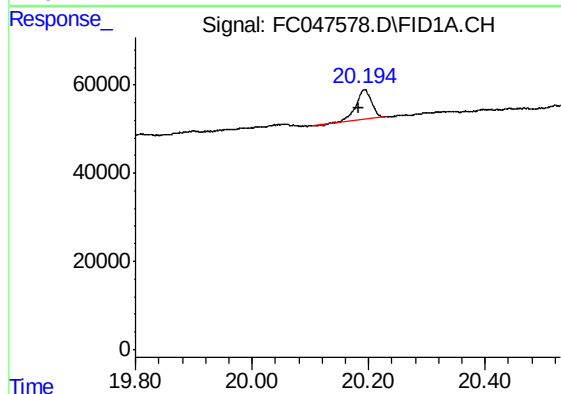

#20 n-Hexatriacontane (C36)

R.T.: 20.193 min
Delta R.T.: 0.009 min
Response: 122183
Conc: 1.41 ug/ml

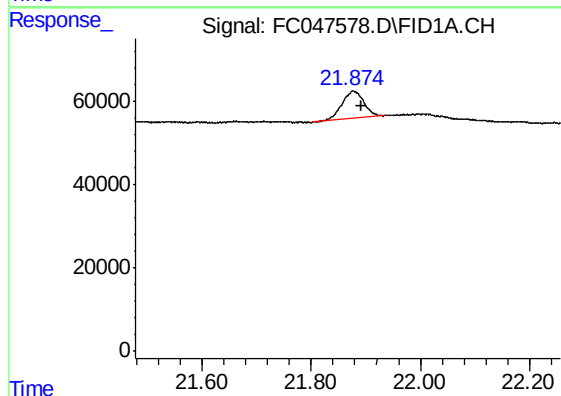

#22 n-Tetracontane (C40)

R.T.: 21.876 min
Delta R.T.: -0.016 min
Response: 184441
Conc: 2.27 ug/ml