

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052620\
 Data File : PS010416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 12:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 13:40:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.921	325.2E6	278.8E6	462.477	519.882
Target Compounds							
1) T	Dalapon	0.000	2.623	0	57634	N.D.	<MDL
5) T	DICAMBA	0.000	7.110	0	494331	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.713	0	194351	N.D.	<MDL
9) T	2,4-D	0.000	7.952	0	849290	N.D.	1.225
12) T	2,4,5-T	0.000	9.194	0	286732	N.D.	<MDL
13) T	2,4-DB	0.000	9.711	0	286655	N.D.	<MDL
15) T	Picloram	0.000	11.019	0	4346727	N.D.	1.030
16) T	DCPA	0.000	10.951	0	543854	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052620\
Data File : PS010416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 12:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 13:40:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

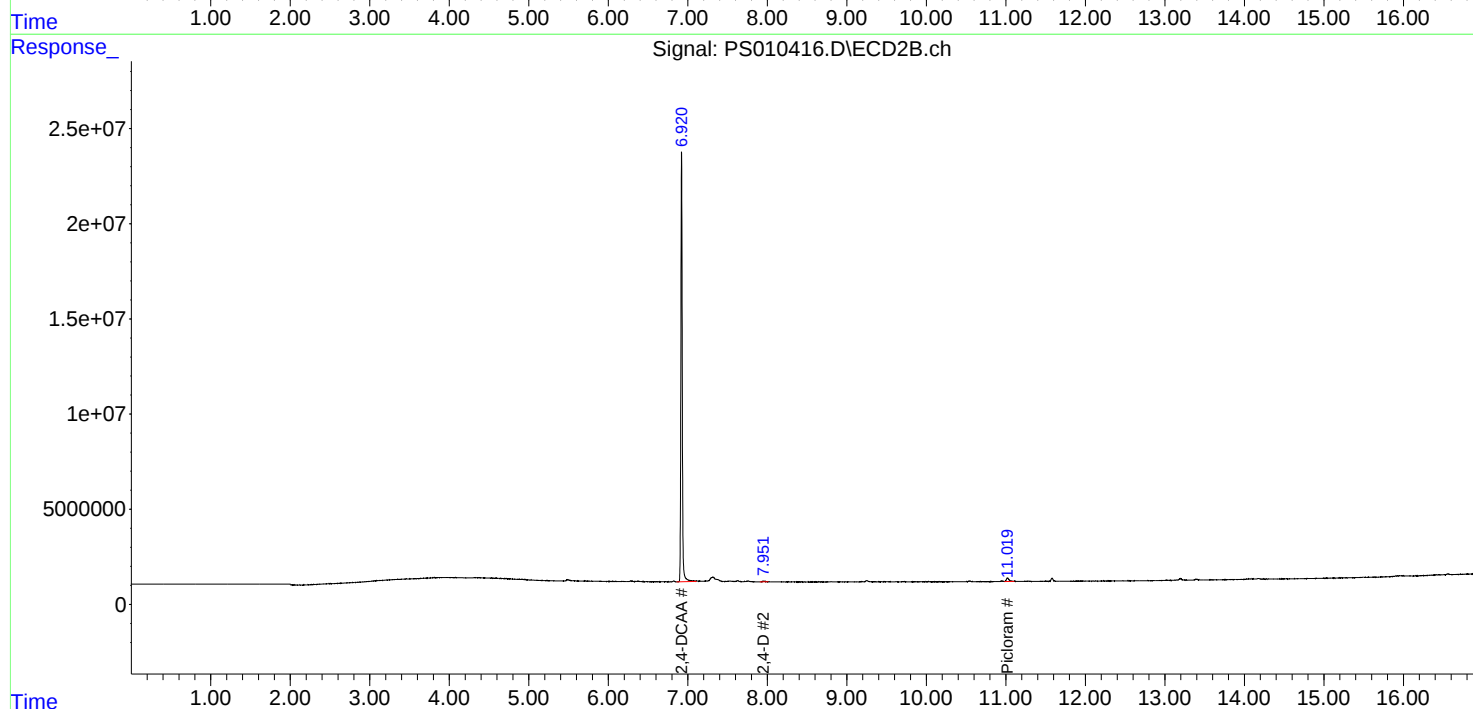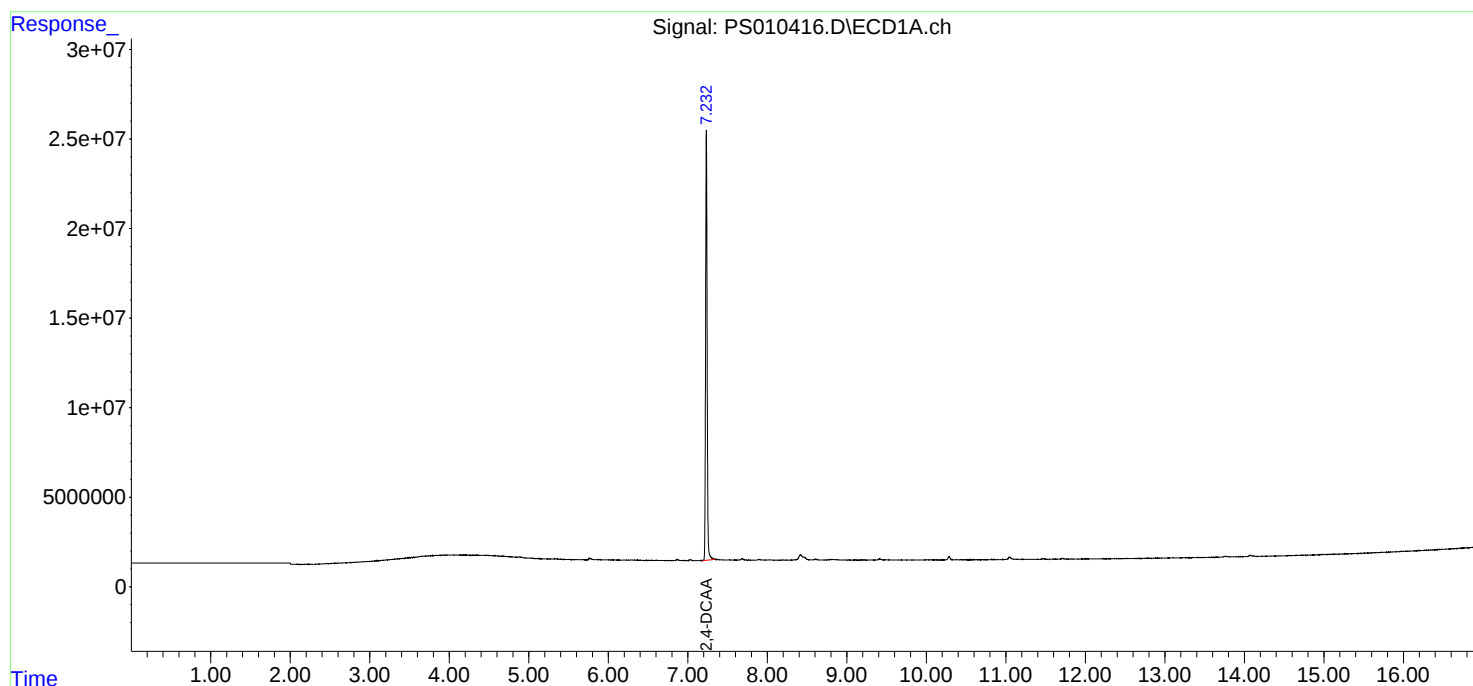


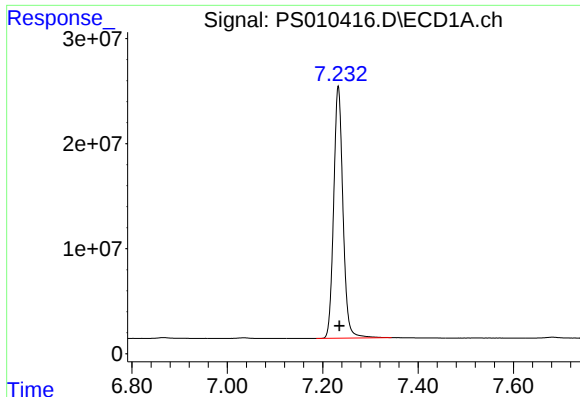

#4 2,4-DCAA


R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 325165147
Conc: 462.48 ng/ml

Instrument :
FID_C
ClientSampleId :

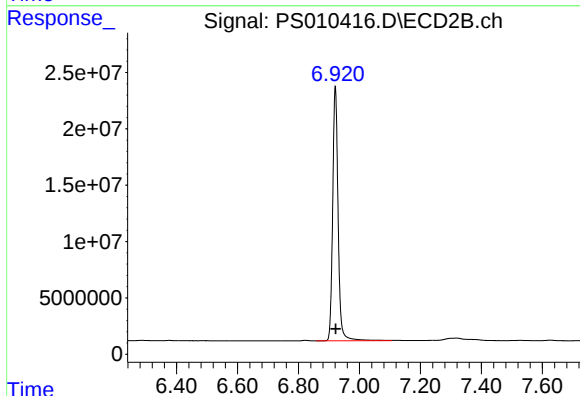


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 278808160
Conc: 519.88 ng/ml

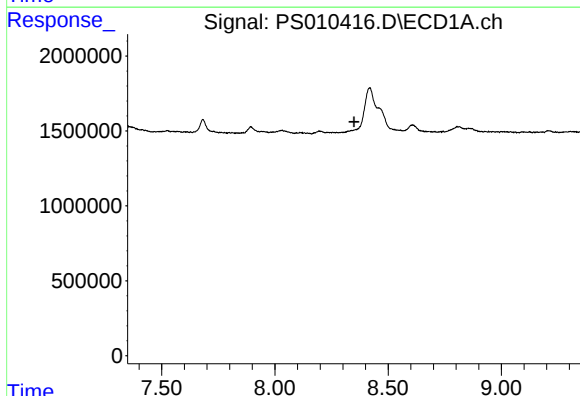


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

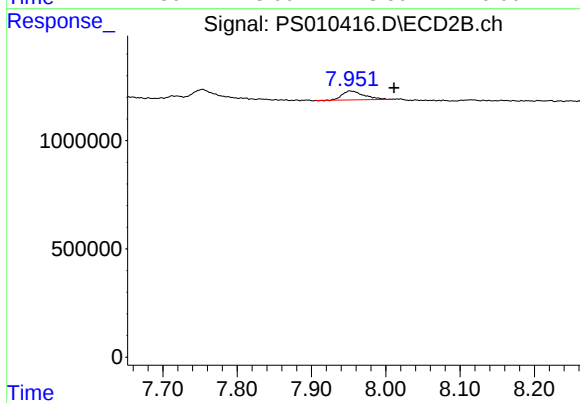

#9 2,4-D


R.T.: 7.952 min
Delta R.T.: -0.060 min
Response: 849290
Conc: 1.22 ng/ml

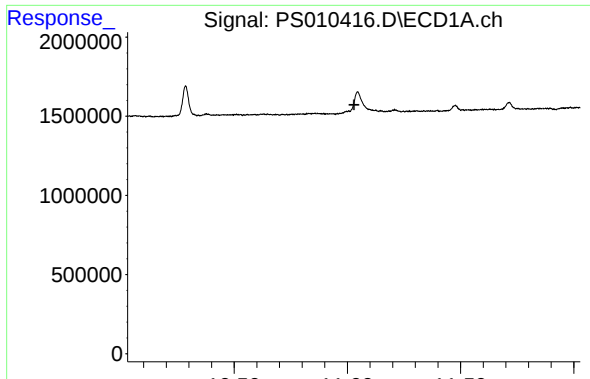

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.029 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

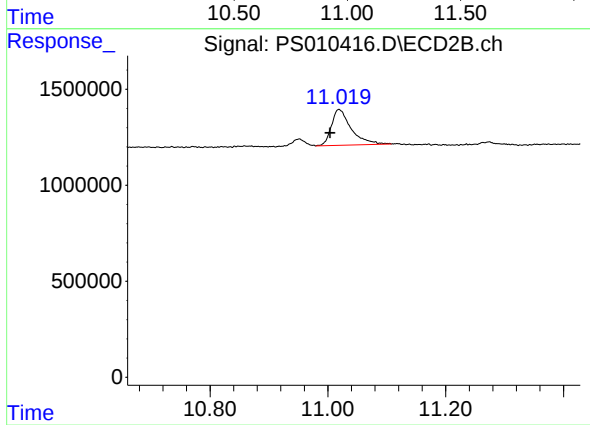

#15 Picloram

R.T.: 11.019 min
Delta R.T.: 0.015 min
Response: 4346727
Conc: 1.03 ng/ml