

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060123AL\
 Data File : FC063721.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jun 2023 20:43
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 03:52:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
 Quant Title : GC Extractables
 QLast Update : Sat May 27 06:12:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	17.619	135351	1.059 ug/ml
18) T	n-Dotriacontane (C32)	18.499	222223	1.786 ug/ml
19) T	n-Tetratriacontane (C34)	19.278	152381	1.236 ug/ml
20) T	n-Hexatriacontane (C36)	20.009	60201	0.502 ug/ml
21) T	n-Octatriacontane (C38)	20.737	210812	1.746 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060123AL\
Data File : FC063721.D
Signal(s) : FID1A.ch
Acq On : 01 Jun 2023 20:43
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 03:52:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

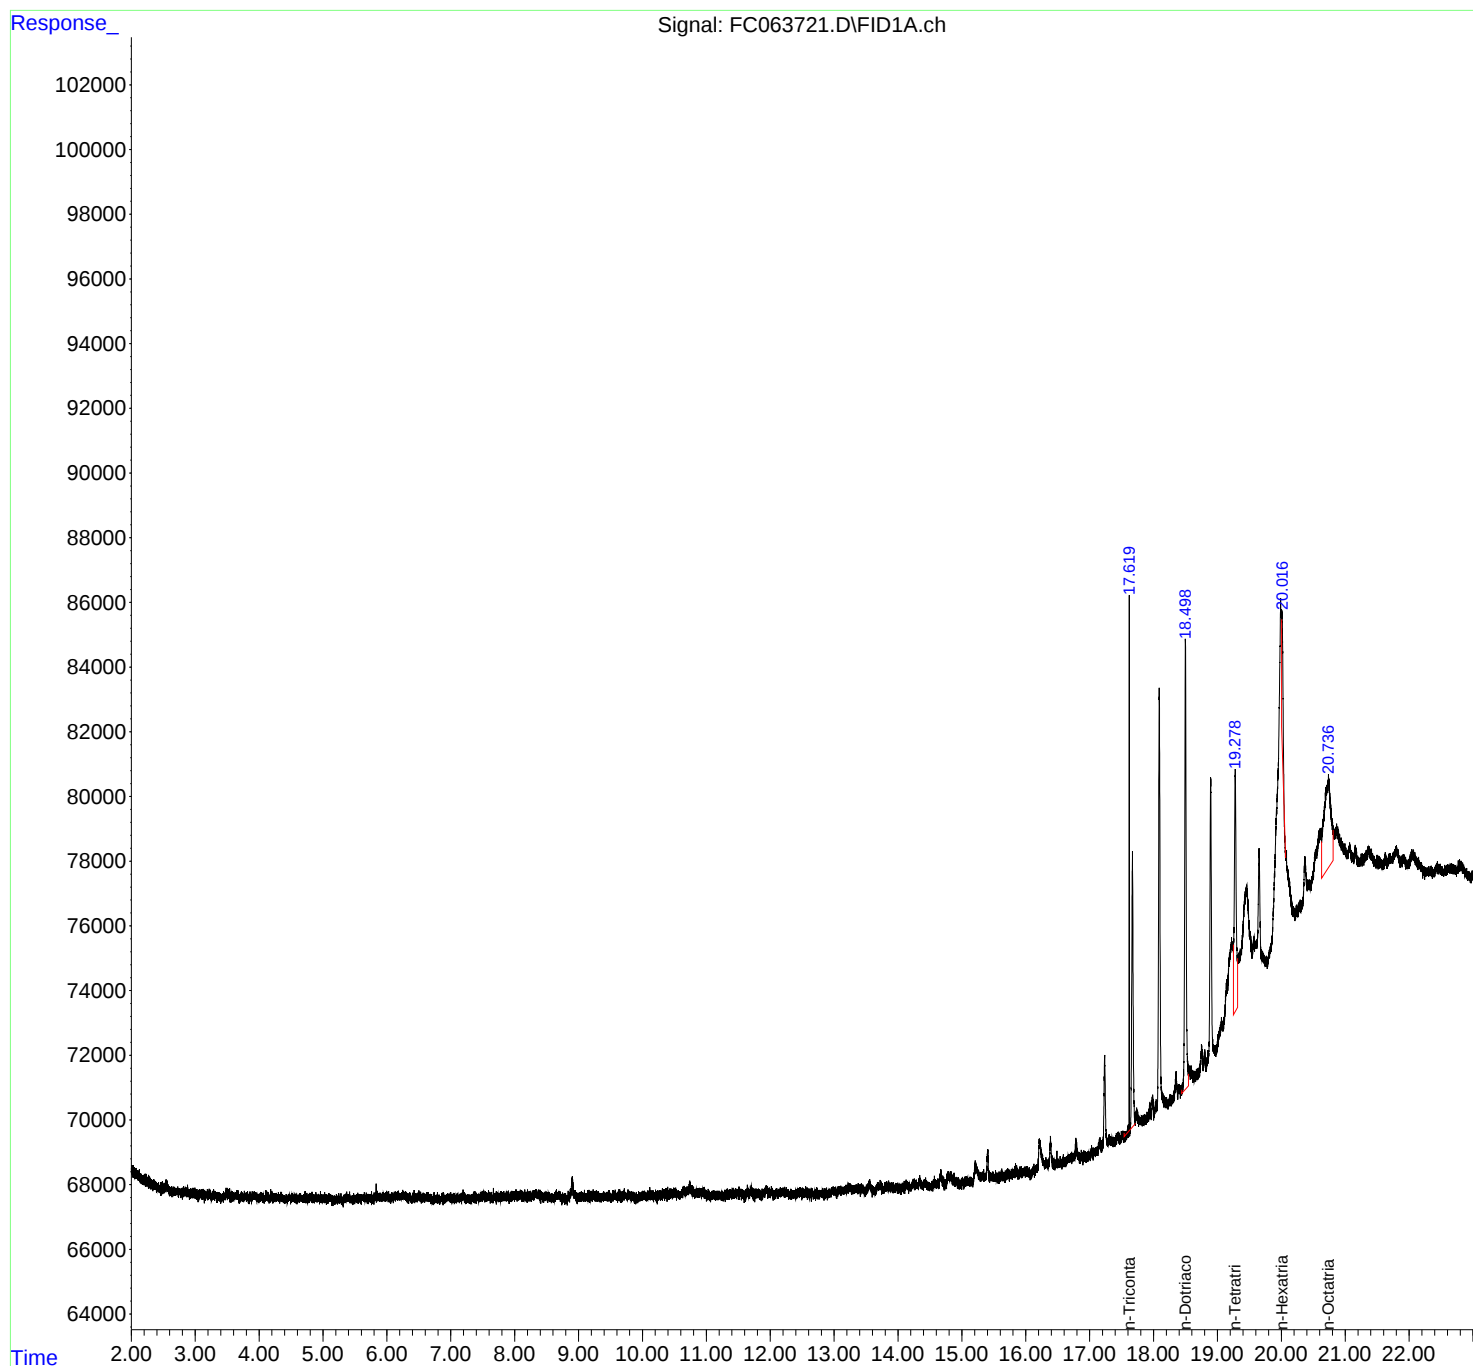


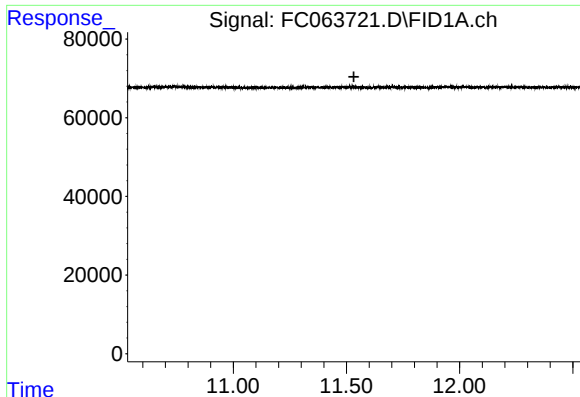

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.533 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

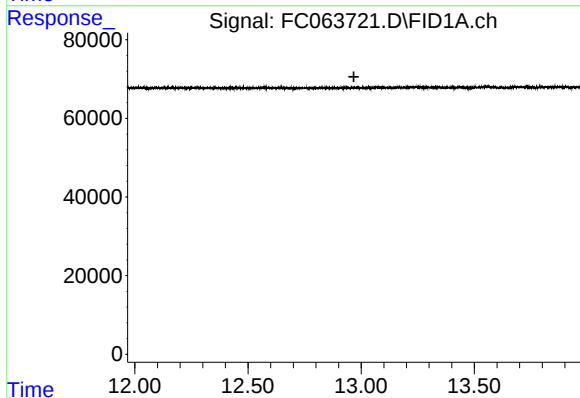


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.968 min
Response: 0
Conc: N.D.

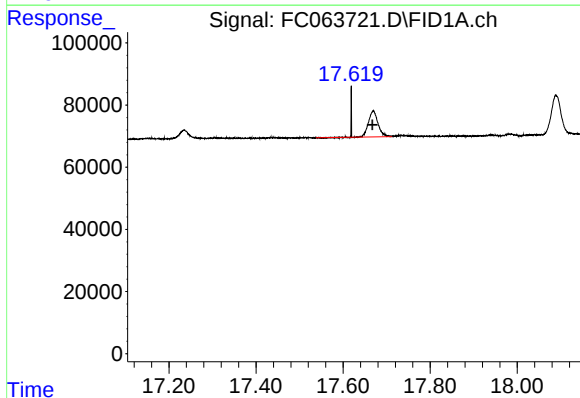


#17 n-Tricontane (C30)

R.T.: 17.619 min
Delta R.T.: -0.048 min
Response: 135351
Conc: 1.06 ug/ml

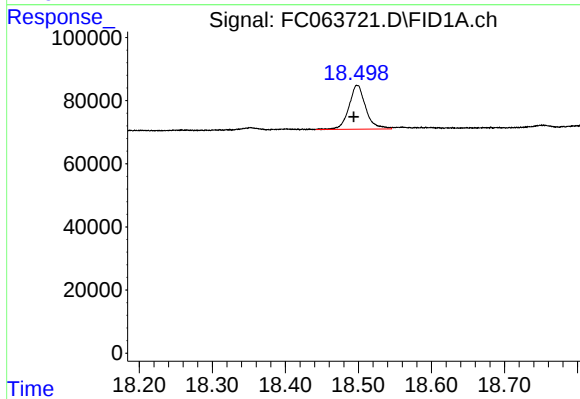

#18 n-Dotriacontane (C32)


R.T.: 18.499 min
Delta R.T.: 0.005 min
Response: 222223
Conc: 1.79 ug/ml

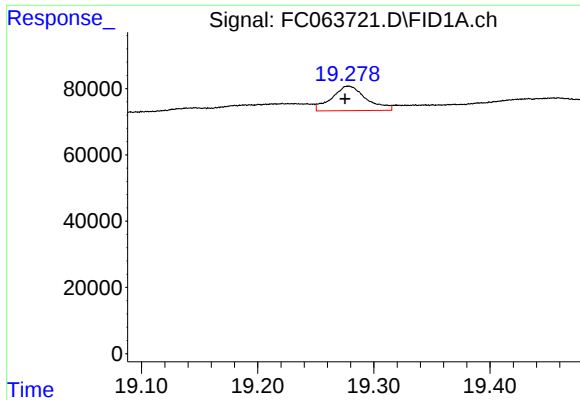

#19 n-Tetratriacontane (C34)


R.T.: 19.278 min
Delta R.T.: 0.003 min
Response: 152381
Conc: 1.24 ug/ml

Instrument :
FID_C
ClientSampleId :

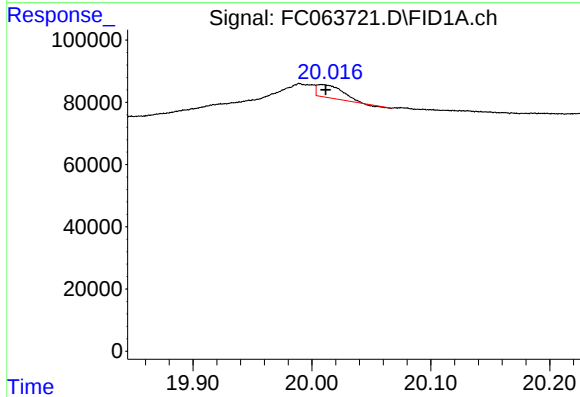

#20 n-Hexatriacontane (C36)

R.T.: 20.009 min
Delta R.T.: -0.003 min
Response: 60201
Conc: 0.50 ug/ml

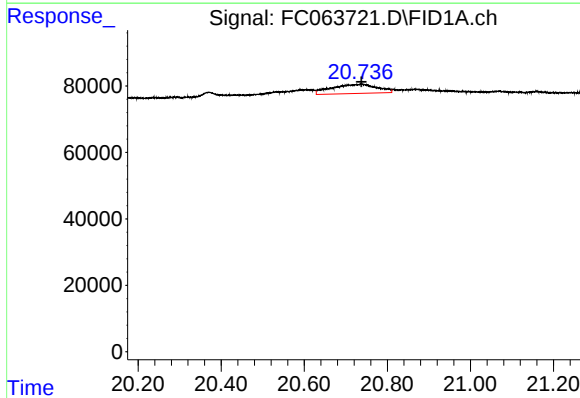

#21 n-Octatriacontane (C38)

R.T.: 20.737 min
Delta R.T.: 0.000 min
Response: 210812
Conc: 1.75 ug/ml