

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
 Data File : PS019604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jun 2022 09:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 15:28:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.783	1101.6E6	450.1E6	459.160	580.883 #
Target Compounds							
1) T	Dalapon	2.973f	0.000	673157	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.376	0.000	171944	0	<MDL	N.D. #
3) T	4-Nitroph...	6.991f	0.000	1586152	0	1.616	N.D. #
5) T	DICAMBA	0.000	7.010f	0	3559745	N.D.	1.041
6) T	MCP	0.000	7.010	0	3559745	N.D.	1.315
7) T	MCPA	7.720	7.183f	909756	3824601	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.637f	0	1917255	N.D.	2.170
9) T	2,4-D	0.000	7.925f	0	340493	N.D.	<MDL
10) T	Pentachlo...	8.621	8.289	433678	711813	<MDL	<MDL #
11) T	2,4,5-TP ...	9.128	8.648	1012495	343353	<MDL	<MDL #
12) T	2,4,5-T	9.452	9.059	9241479	327859	<MDL	<MDL #
13) T	2,4-DB	10.015	9.474f	5039319	549534	1.246	<MDL #
14) T	DINOSEB	0.000	9.858	0	206470	N.D.	<MDL
15) T	Picloram	10.964	10.889f	280.1E6	5433800	9.437	<MDL #
16) T	DCPA	11.430	10.781	2932681	1188108	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060422\
Data File : PS019604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jun 2022 09:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 15:28:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

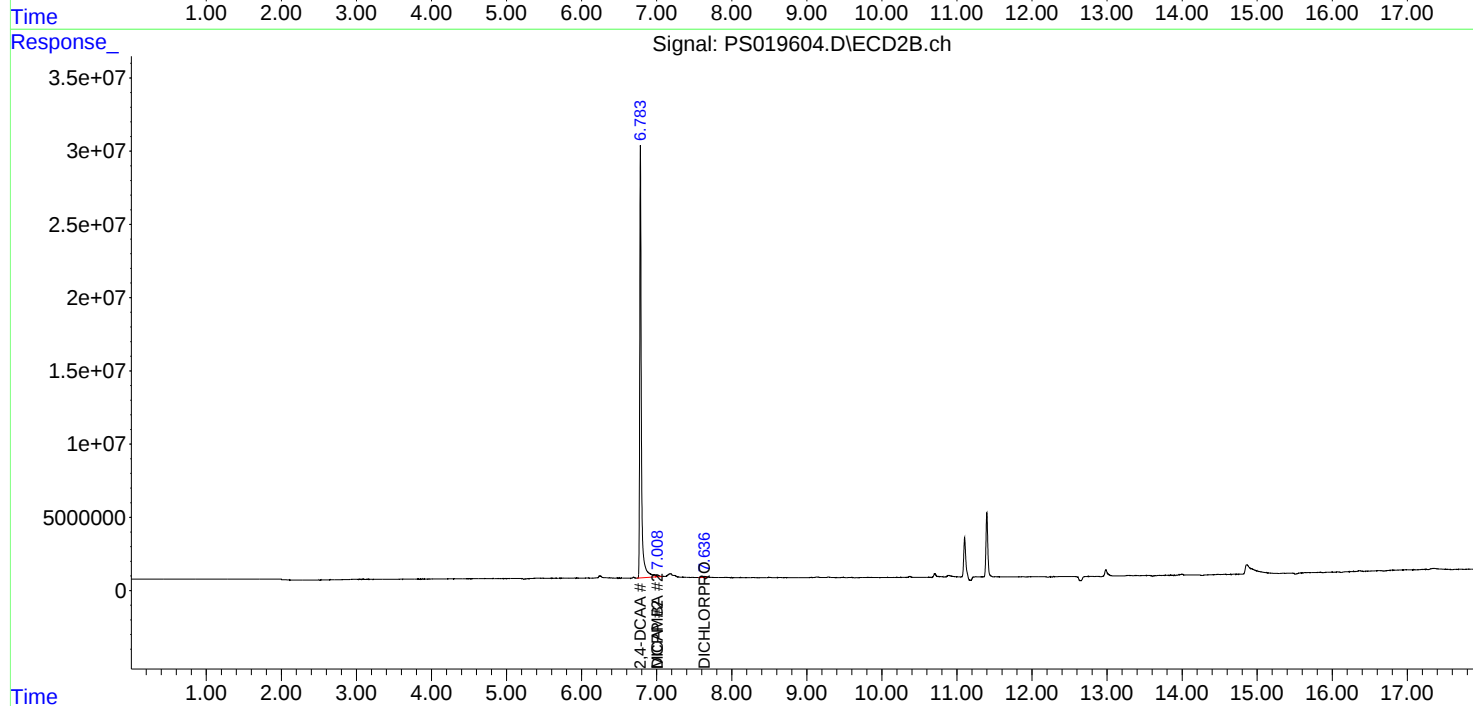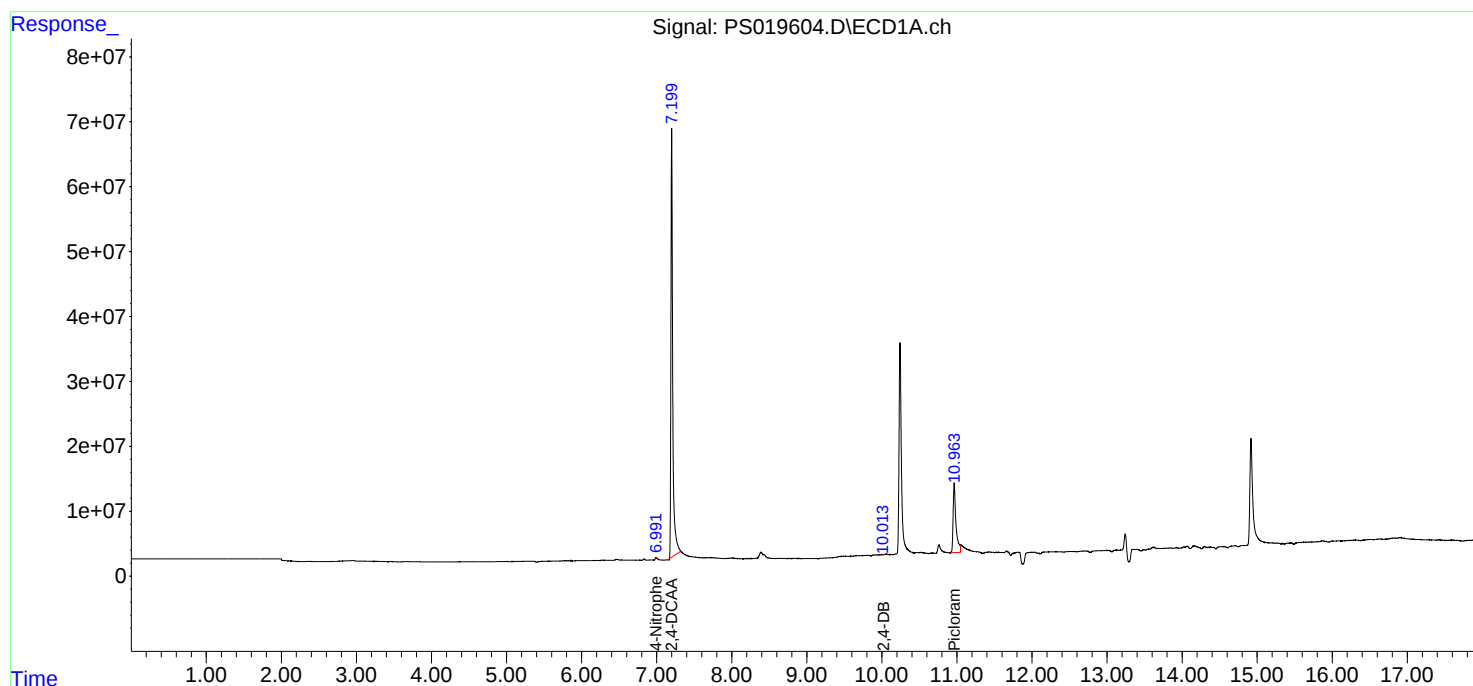


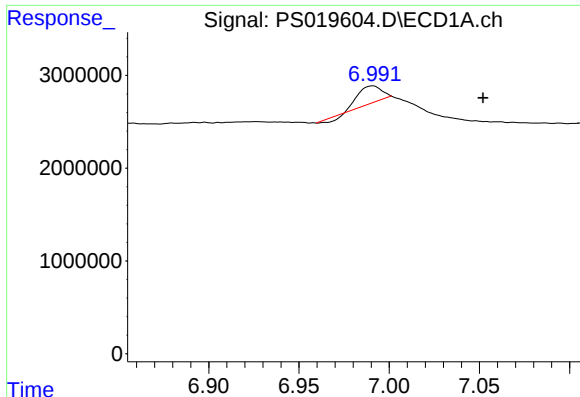

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: -0.061 min
Response: 1586152
Conc: 1.62 ng/ml

Instrument :
FID_C
ClientSampleId :

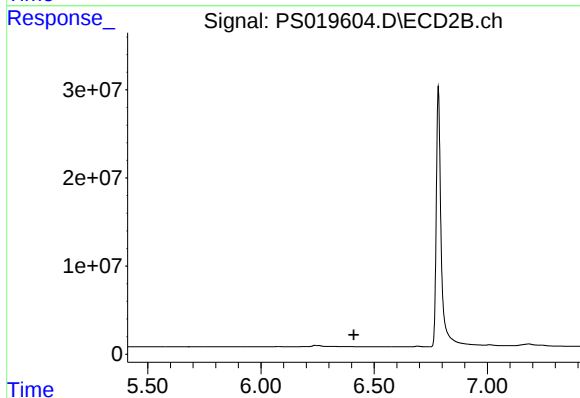


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

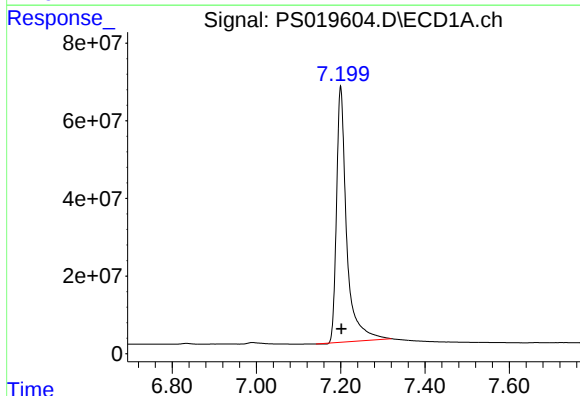


#4 2,4-DCAA

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1101602142
Conc: 459.16 ng/ml

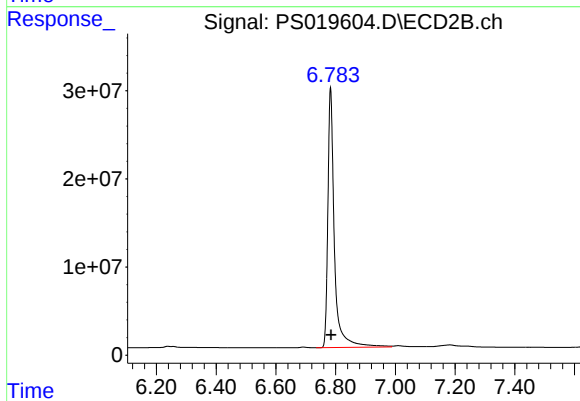

#4 2,4-DCAA


R.T.: 6.783 min
Delta R.T.: -0.002 min
Response: 450108747
Conc: 580.88 ng/ml

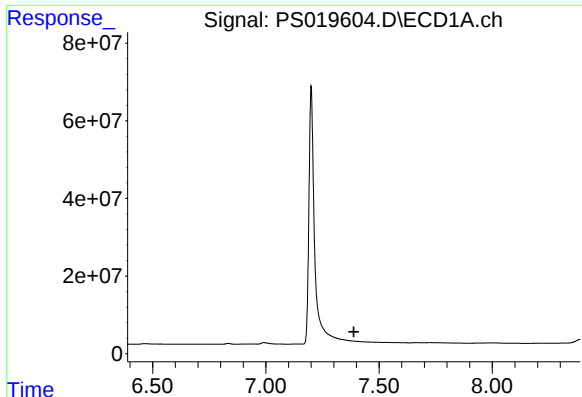

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.388 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

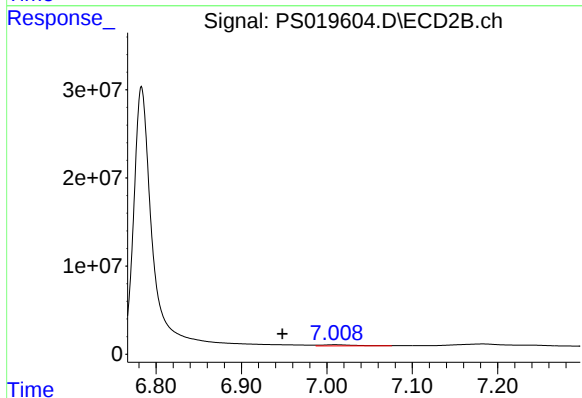


#5 DICAMBA

R.T.: 7.010 min
Delta R.T.: 0.062 min
Response: 3559745
Conc: 1.04 ng/ml

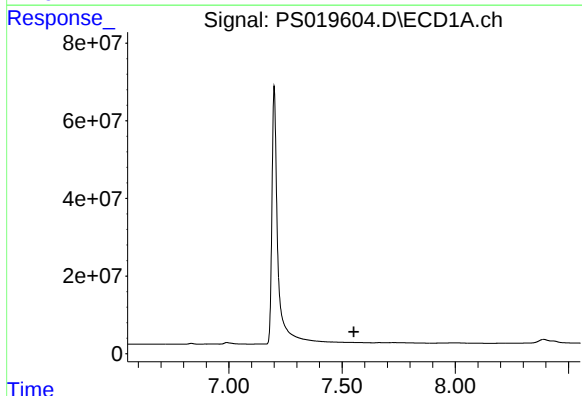


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

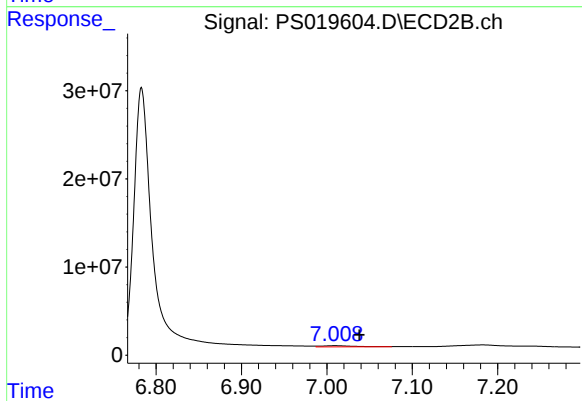

#6 MCPP


R.T.: 7.010 min
Delta R.T.: -0.028 min
Response: 3559745
Conc: 1.32 ug/ml

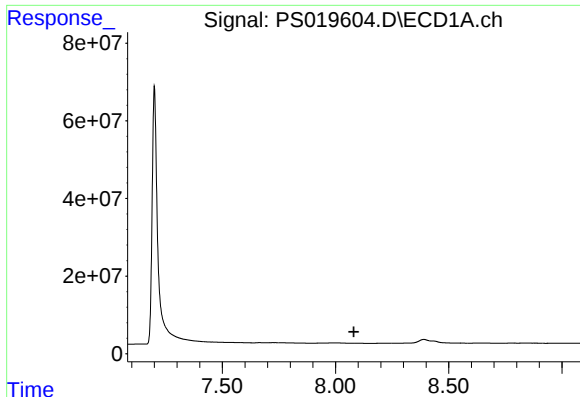

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

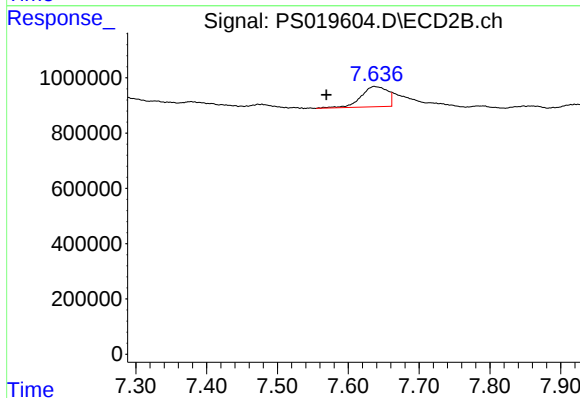


#8 DICHLORPROP

R.T.: 7.637 min
Delta R.T.: 0.067 min
Response: 1917255
Conc: 2.17 ng/ml

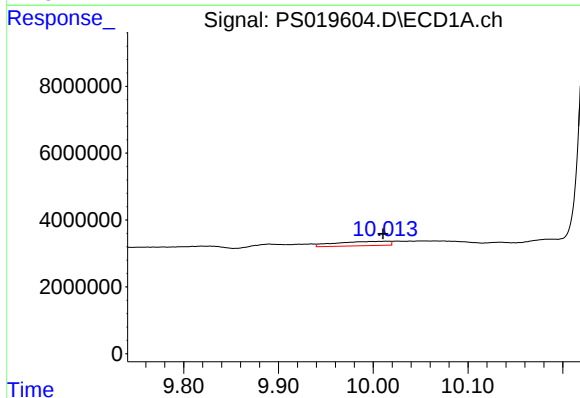


#13 2,4-DB

R.T.: 10.015 min
Delta R.T.: 0.004 min
Response: 5039319
Conc: 1.25 ng/ml

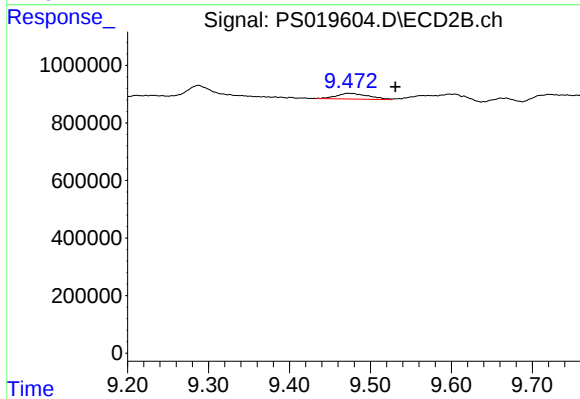

#13 2,4-DB


R.T.: 9.474 min
Delta R.T.: -0.057 min
Response: 549534
Conc: N.D.

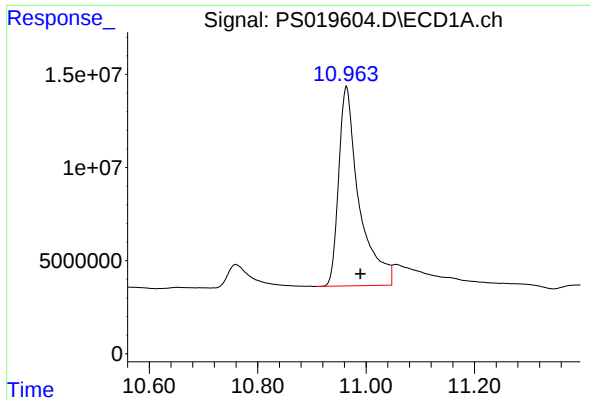

#15 Picloram

R.T.: 10.964 min
Delta R.T.: -0.026 min
Response: 280069913
Conc: 9.44 ng/ml

Instrument :
FID_C
ClientSampleId :

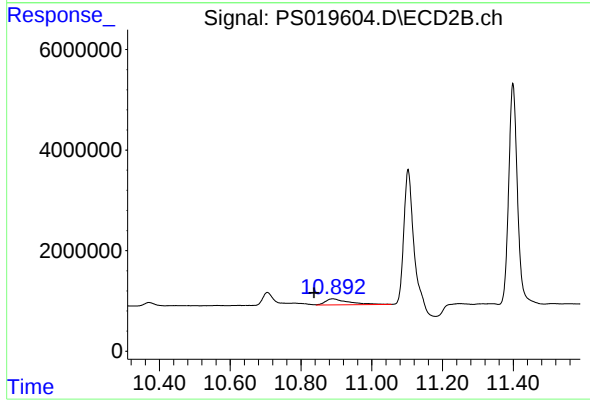

#15 Picloram

R.T.: 10.889 min
Delta R.T.: 0.052 min
Response: 5433800
Conc: N.D.