

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060523AL\
 Data File : FC063724.D
 Signal(s) : FID1A.ch
 Acq On : 05 Jun 2023 08:34
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 06 02:32:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
 Quant Title : GC Extractables
 QLast Update : Sat May 27 06:12:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	17.672	40486	0.317 ug/ml
18) T n-Dotriacontane (C32)	18.507	28327	0.228 ug/ml
19) T n-Tetratriacontane (C34)	19.283	37069	0.301 ug/ml
20) T n-Hexatriacontane (C36)	20.068f	49256	0.410 ug/ml
21) T n-Octatriacontane (C38)	20.755	31414	0.260 ug/ml
22) T n-Tetracontane (C40)	21.632	208865	1.724 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060523AL\
Data File : FC063724.D
Signal(s) : FID1A.ch
Acq On : 05 Jun 2023 08:34
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 06 02:32:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

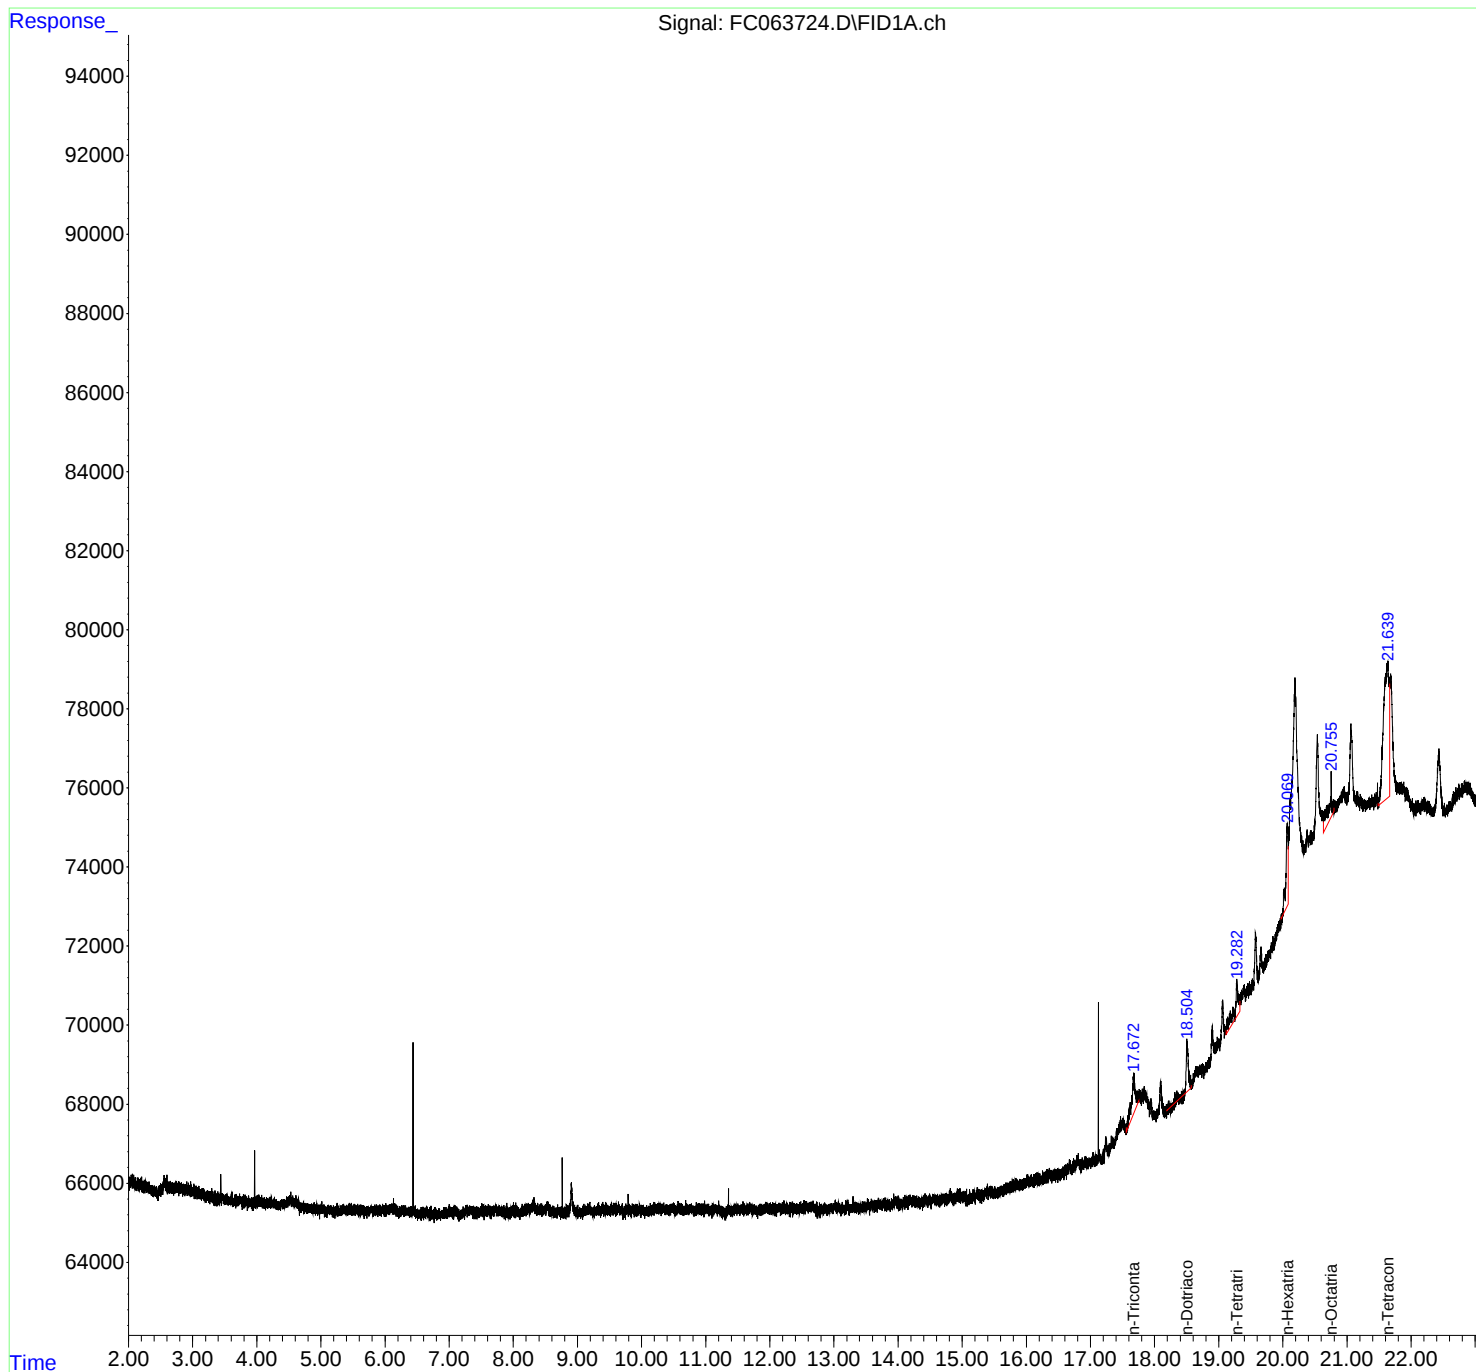


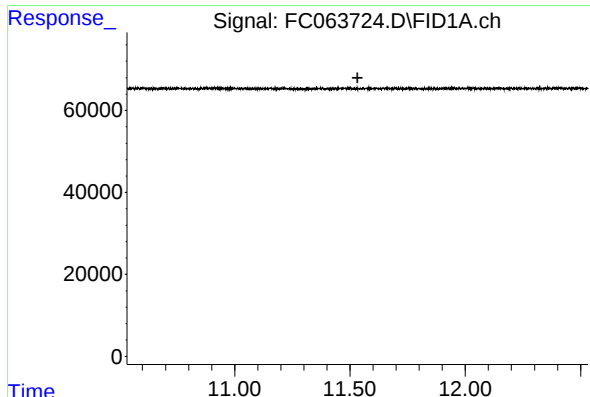

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.533 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

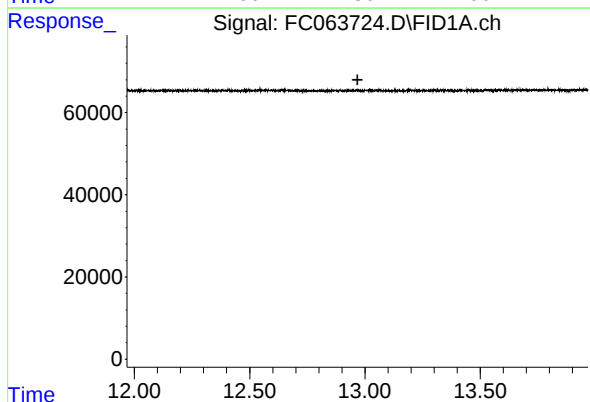


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.968 min
Response: 0
Conc: N.D.

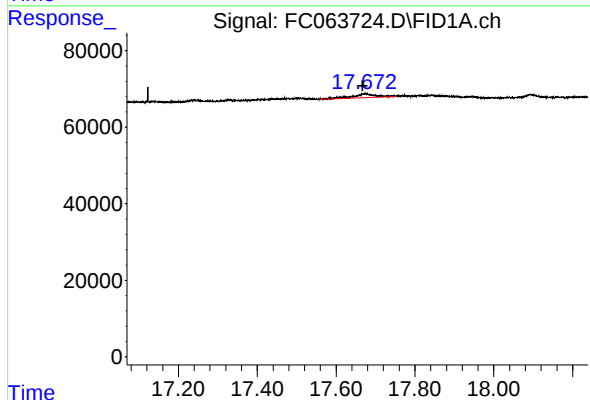


#17 n-Tricontane (C30)

R.T.: 17.672 min
Delta R.T.: 0.005 min
Response: 40486
Conc: 0.32 ug/ml

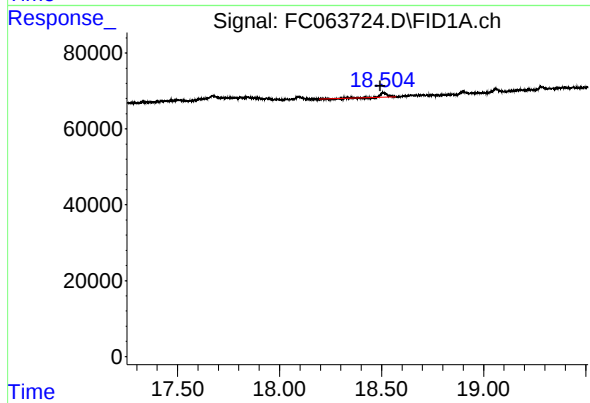

#18 n-Dotriacontane (C32)


R.T.: 18.507 min
Delta R.T.: 0.013 min
Response: 28327
Conc: 0.23 ug/ml

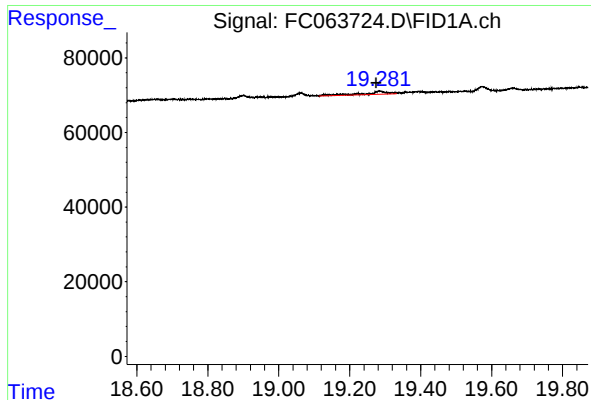

#19 n-Tetratriacontane (C34)


R.T.: 19.283 min
Delta R.T.: 0.008 min
Response: 37069
Conc: 0.30 ug/ml

Instrument :
FID_C
ClientSampleId :

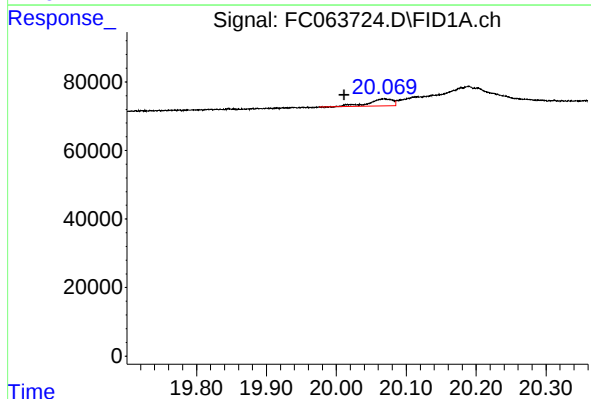


#20 n-Hexatriacontane (C36)

R.T.: 20.068 min
Delta R.T.: 0.057 min
Response: 49256
Conc: 0.41 ug/ml

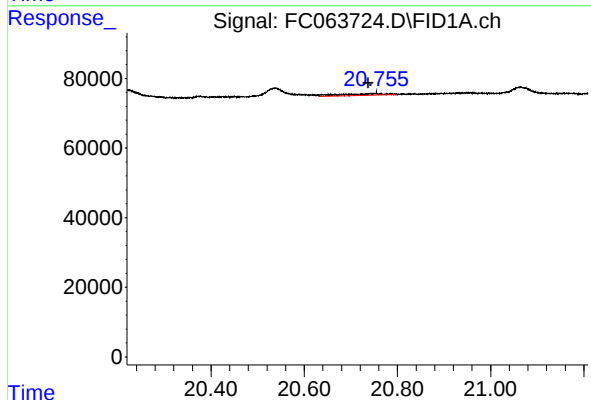

#21 n-Octatriacontane (C38)

R.T.: 20.755 min
Delta R.T.: 0.017 min
Response: 31414
Conc: 0.26 ug/ml

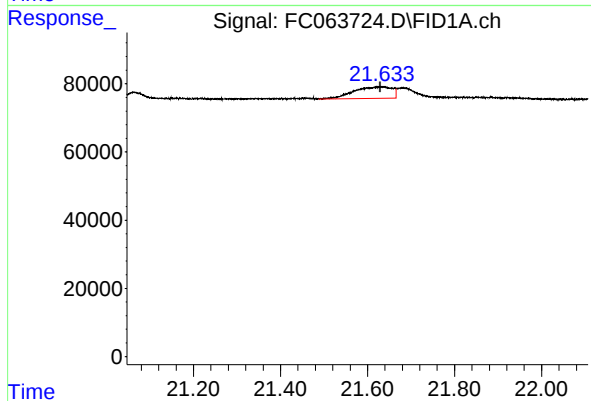

#22 n-Tetracontane (C40)

R.T.: 21.632 min
Delta R.T.: 0.002 min
Response: 208865
Conc: 1.72 ug/ml