

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060722AL\
 Data File : FC060125.D
 Signal(s) : FID1A.CH
 Acq On : 07 Jun 2022 12:52
 Operator : UA/NP
 Sample : N3197-03DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 02:27:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 08:22:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.647	719024	4.620 ug/ml
Spiked Amount 50.000		Recovery =	9.24%
12) S 1-chlorooctadecane (S...	12.013	767969	6.194 ug/ml
Spiked Amount 50.000		Recovery =	12.39%
Target Compounds			
10) T n-Eicosane (C20)	11.643f	931495	6.529 ug/ml
13) T n-Docosane (C22)	12.802	107218	0.752 ug/ml
16) T n-Octacosane (C28)	15.823f	228458	1.754 ug/ml
18) T n-Dotriacontane (C32)	17.480	286640	2.571 ug/ml
20) T n-Hexatriacontane (C36)	18.878f	112243	1.185 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC060722AL\
Data File : FC060125.D
Signal(s) : FID1A.CH
Acq On : 07 Jun 2022 12:52
Operator : UA/NP
Sample : N3197-03DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 02:27:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

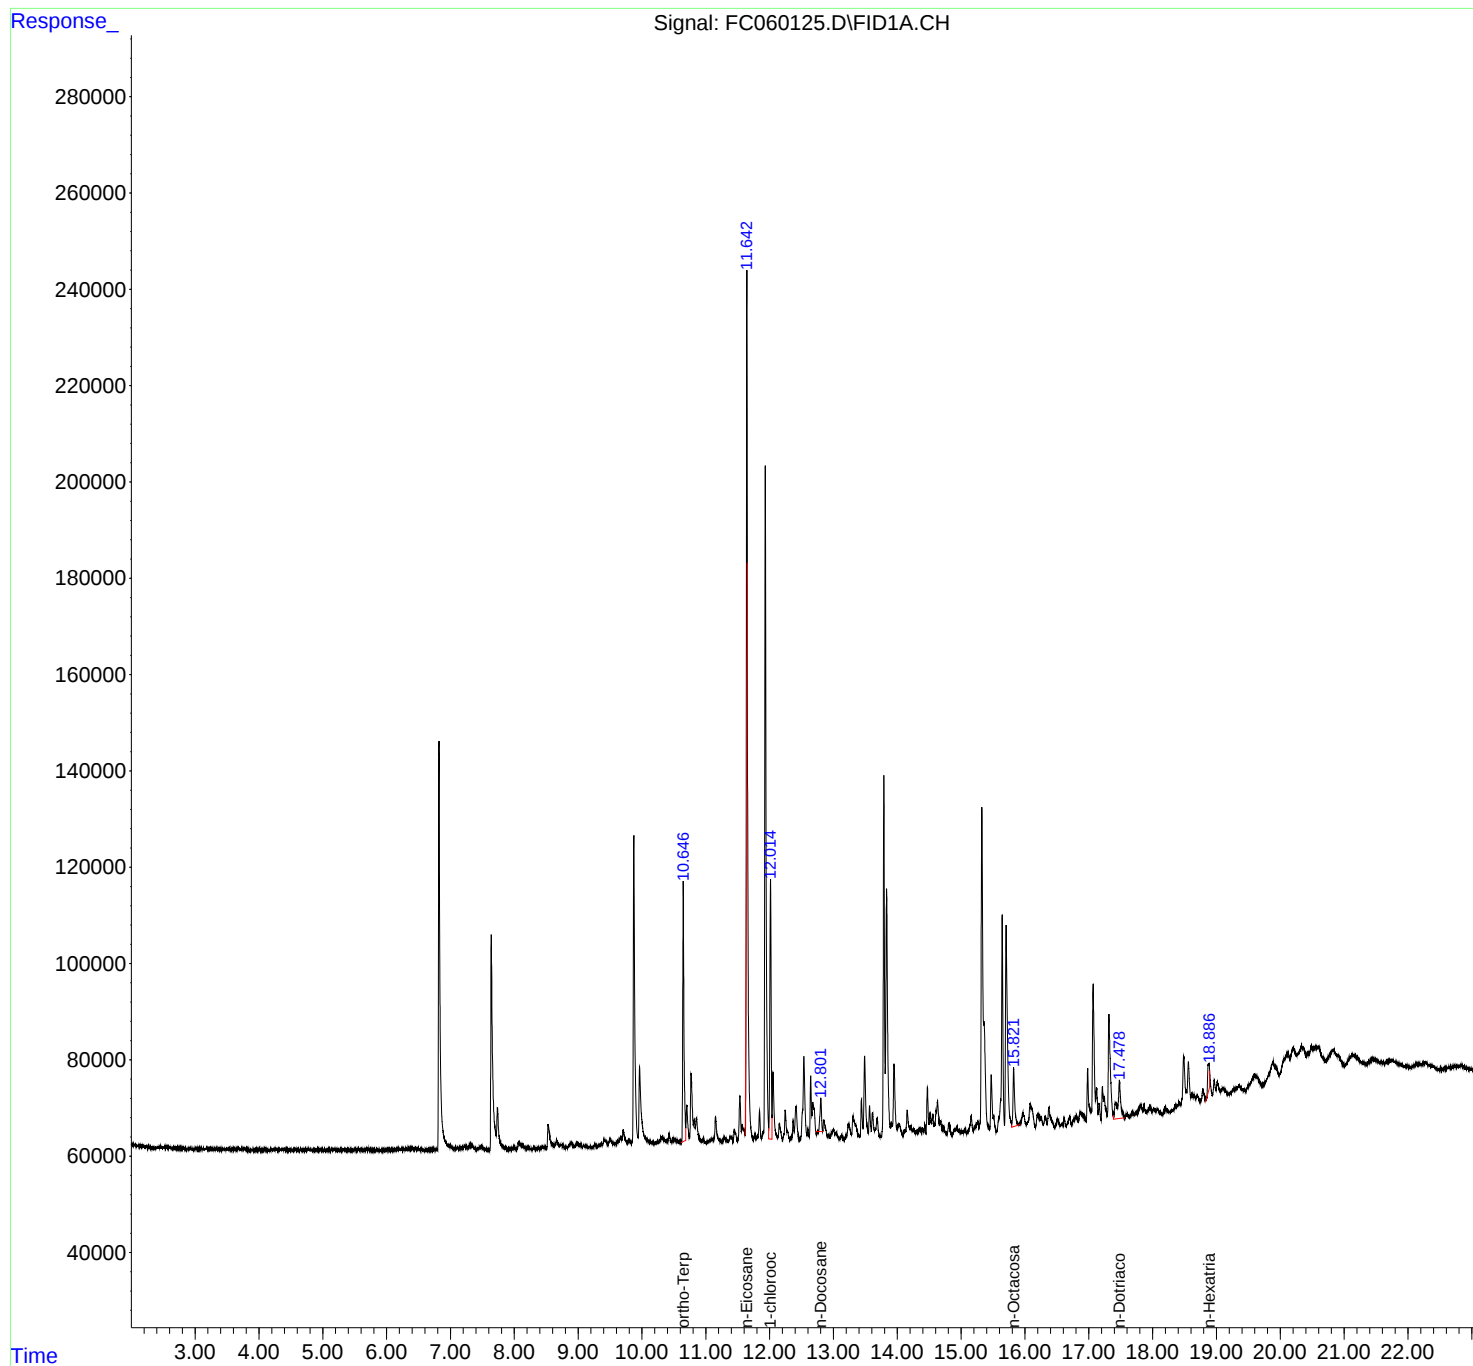


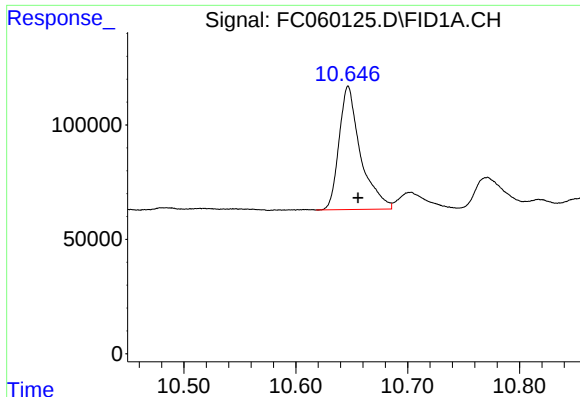

#9 ortho-Terphenyl (SURR)


R.T.: 10.647 min
Delta R.T.: -0.009 min
Response: 719024
Conc: 4.62 ug/ml

Instrument :
FID_C
ClientSampleId :

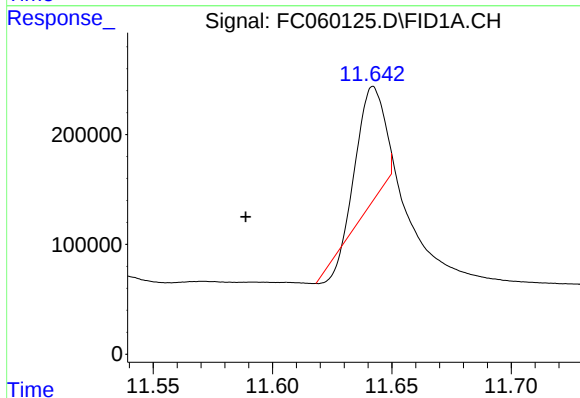


#10 n-Eicosane (C20)

R.T.: 11.643 min
Delta R.T.: 0.054 min
Response: 931495
Conc: 6.53 ug/ml

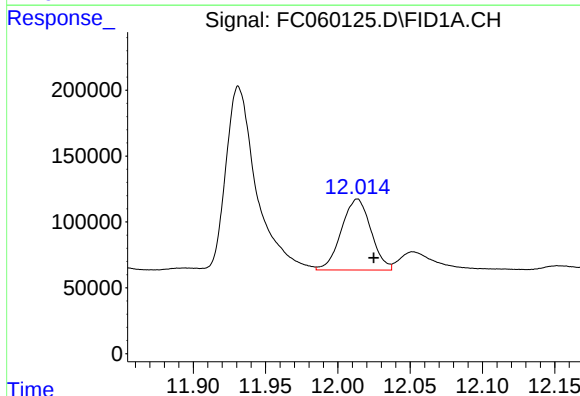


#12 1-chlorooctadecane (SURR)

R.T.: 12.013 min
Delta R.T.: -0.012 min
Response: 767969
Conc: 6.19 ug/ml

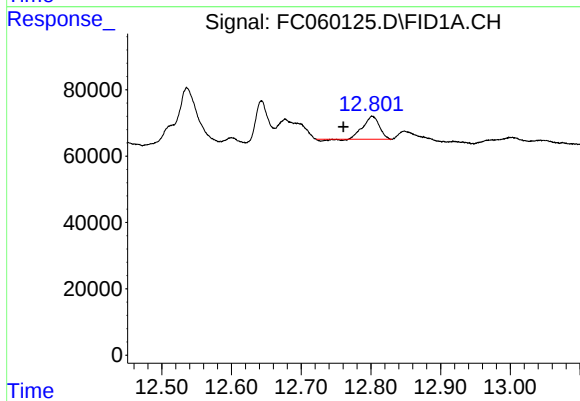

#13 n-Docosane (C22)


R.T.: 12.802 min
Delta R.T.: 0.042 min
Response: 107218
Conc: 0.75 ug/ml

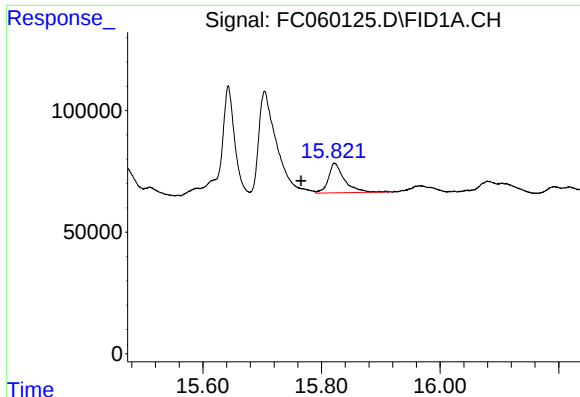

#16 n-Octacosane (C28)


R.T.: 15.823 min
Delta R.T.: 0.057 min
Response: 228458
Conc: 1.75 ug/ml

Instrument :
FID_C
ClientSampleId :

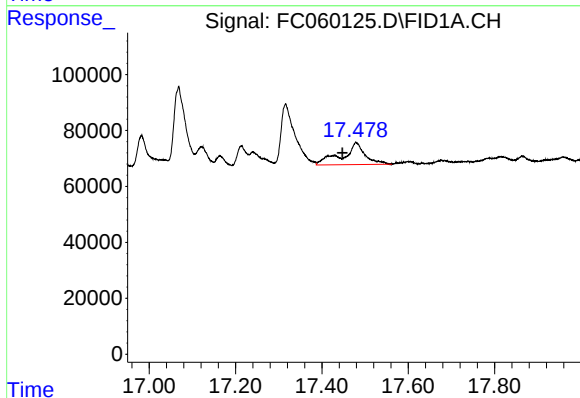

#18 n-Dotriacontane (C32)

R.T.: 17.480 min
Delta R.T.: 0.033 min
Response: 286640
Conc: 2.57 ug/ml

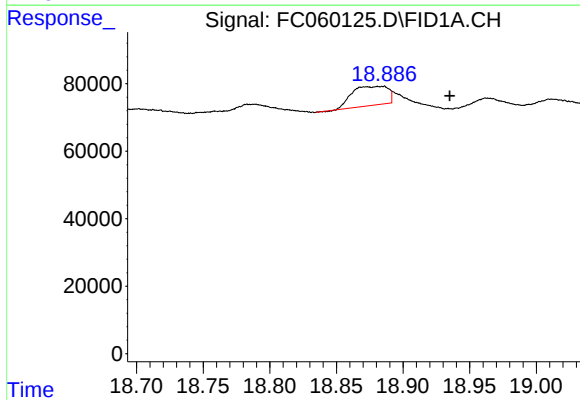

#20 n-Hexatriacontane (C36)

R.T.: 18.878 min
Delta R.T.: -0.057 min
Response: 112243
Conc: 1.19 ug/ml