

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC060923AL\  
 Data File : FC063802.D  
 Signal(s) : FID1A.ch  
 Acq On : 09 Jun 2023 09:02  
 Operator : YP/AJ  
 Sample : 03067-03DL 10X  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 DT-03DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/12/2023  
 Supervised By :Ankita Jodhani 06/12/2023

Integration File: autoint1.e  
 Quant Time: Jun 10 01:07:16 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 052723.M  
 Quant Title : GC Extractables  
 QLast Update : Sat May 27 06:12:33 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.533 | 714419     | 3.915 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 7.83%        |
| 12) S 1-chlorooctadecane (S... | 12.967 | 397748     | 3.113 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 6.23%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC060923AL\  
Data File : FC063802.D  
Signal(s) : FID1A.ch  
Acq On : 09 Jun 2023 09:02  
Operator : YP/AJ  
Sample : 03067-03DL 10X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
DT-03DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/12/2023  
Supervised By :Ankita Jodhani 06/12/2023

Integration File: autoint1.e  
Quant Time: Jun 10 01:07:16 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 052723.M  
Quant Title : GC Extractables  
QLast Update : Sat May 27 06:12:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

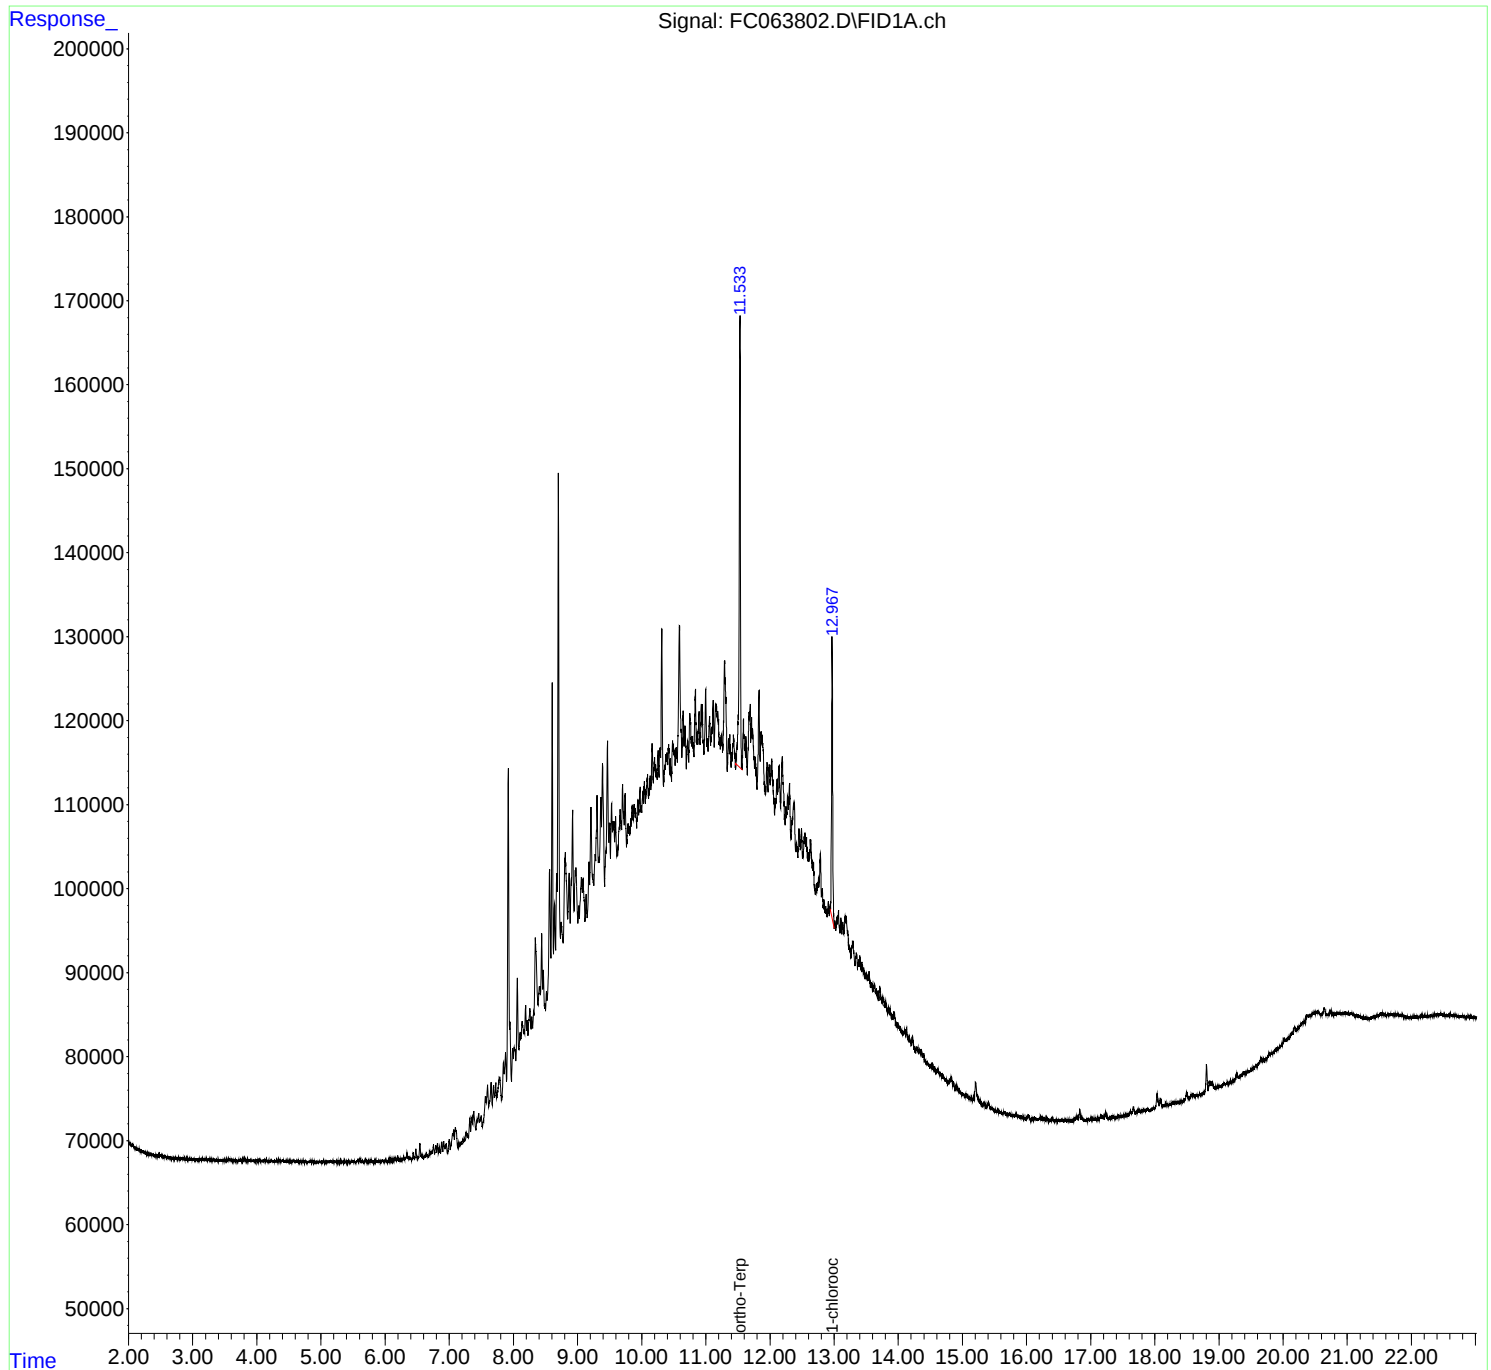

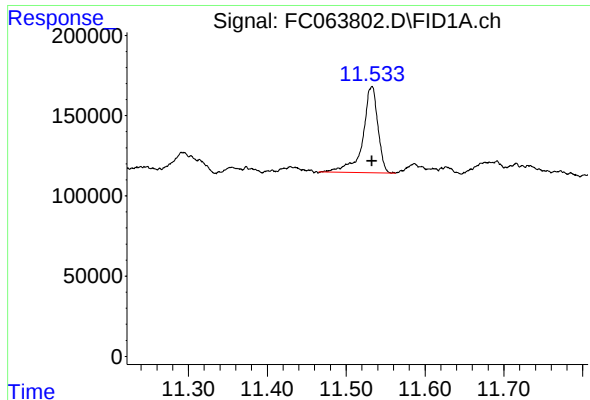


#9 ortho-Terphenyl (SURR)

R.T.: 11.533 min  
Delta R.T.: 0.000 min  
Response: 714419  
Conc: 3.91 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
DT-03DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/12/2023  
Supervised By :Ankita Jodhani 06/12/2023

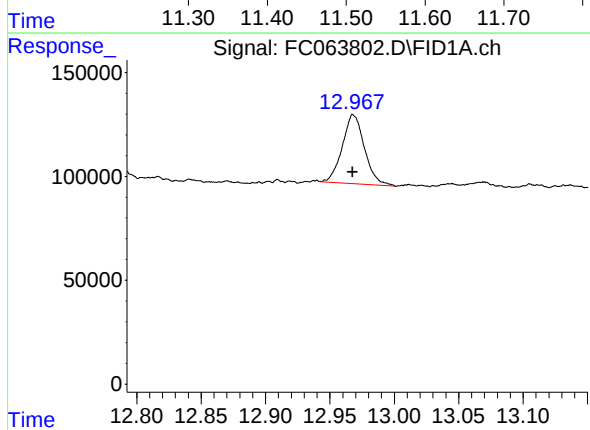

#12 1-chlorooctadecane (SURR)

R.T.: 12.967 min  
Delta R.T.: 0.000 min  
Response: 397748  
Conc: 3.11 ug/ml m