

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061021AL\
 Data File : FC054183.D
 Signal(s) : FID1A.CH
 Acq On : 11 Jun 2021 7:23
 Operator : DD\AJ
 Sample : M2646-01DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 11 08:51:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 04:43:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.350	1002968	6.605 ug/ml
Spiked Amount 50.000		Recovery =	13.21%
12) S 1-chlorooctadecane (S...	12.796	774967	6.579 ug/ml
Spiked Amount 50.000		Recovery =	13.16%
Target Compounds			
19) T n-Tetratriacontane (C34)	19.123	130798	1.118 ug/ml
20) T n-Hexatriacontane (C36)	19.860	113140	1.025 ug/ml
21) T n-Octatriacontane (C38)	20.567	136393	1.334 ug/ml
22) T n-Tetracontane (C40)	21.430	660629	6.174 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061021AL\
Data File : FC054183.D
Signal(s) : FID1A.CH
Acq On : 11 Jun 2021 7:23
Operator : DD\AJ
Sample : M2646-01DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 11 08:51:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 04:43:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

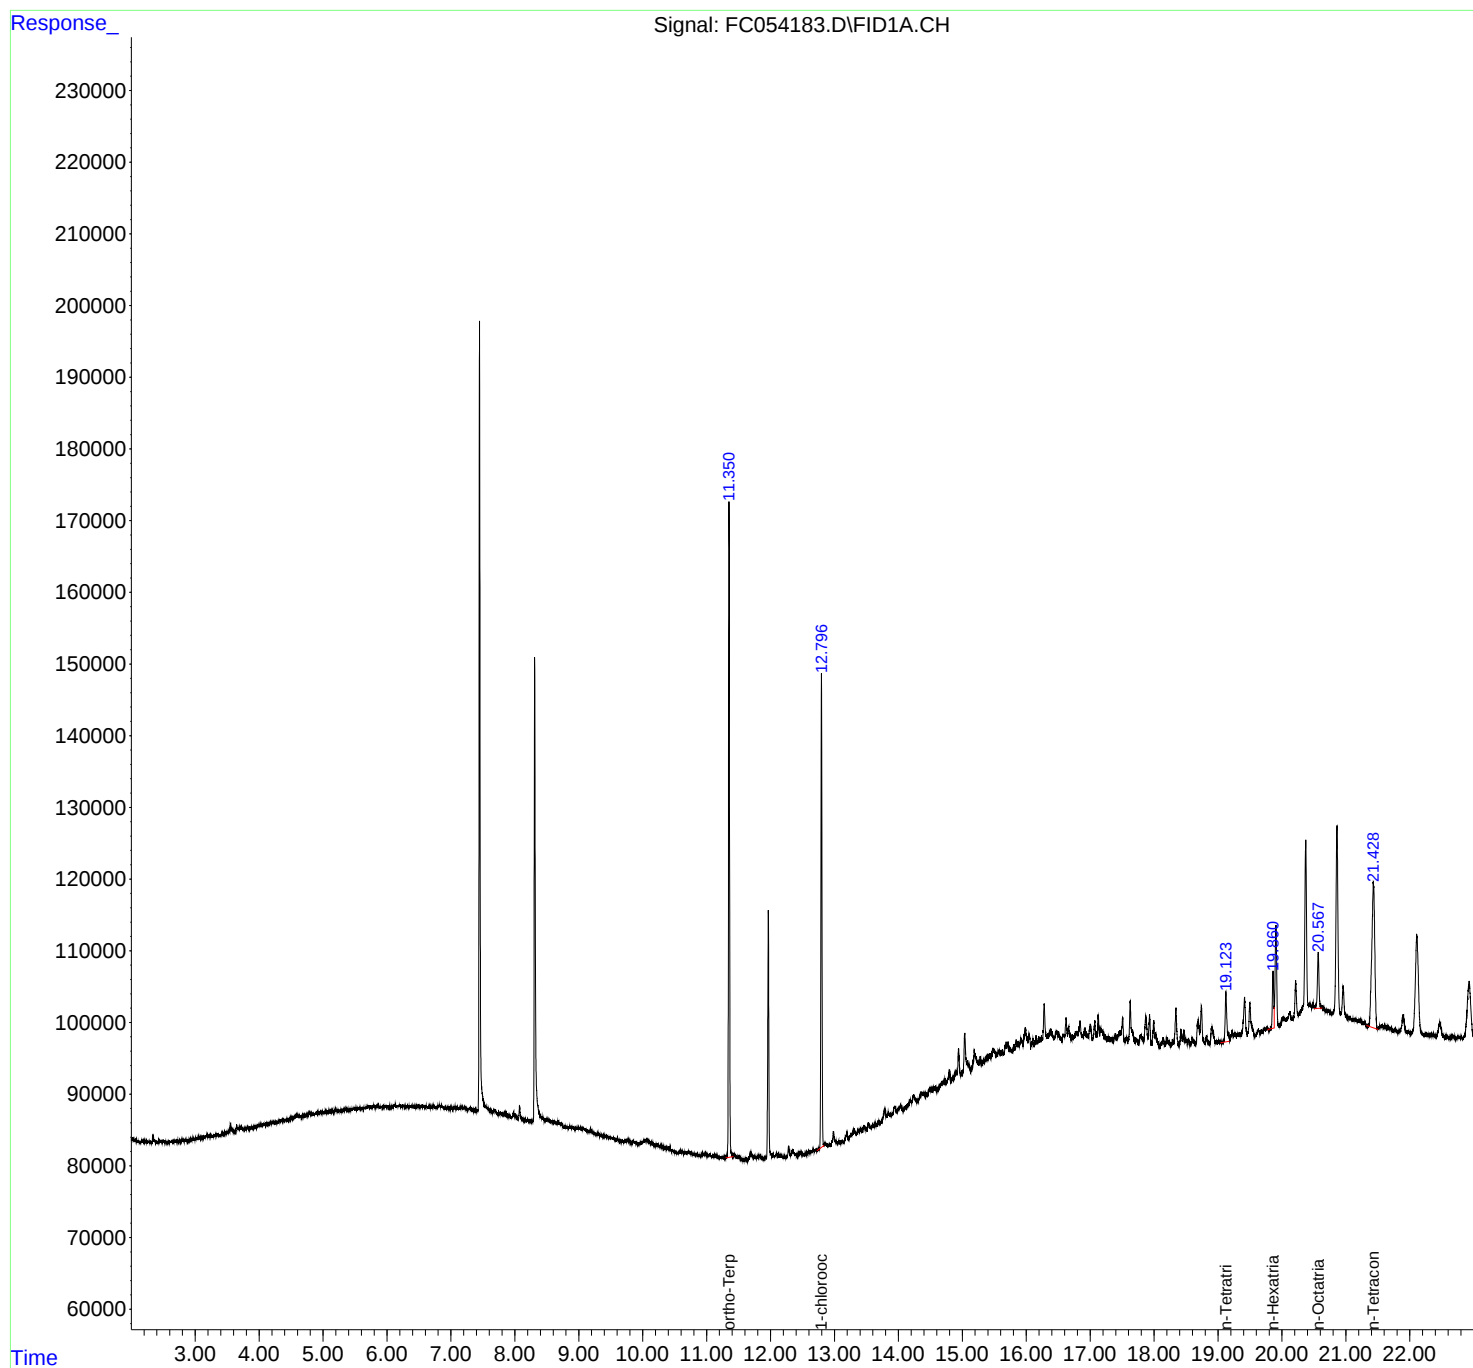


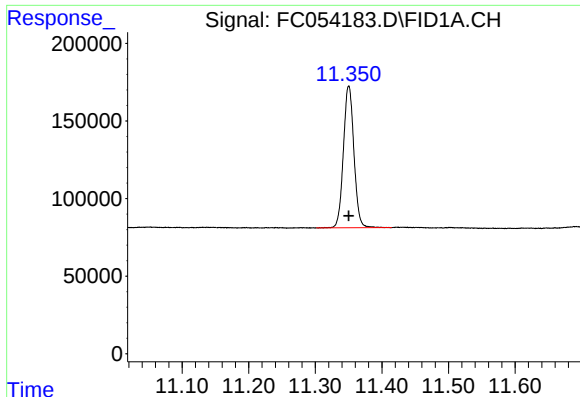

#9 ortho-Terphenyl (SURR)


R.T.: 11.350 min
Delta R.T.: 0.000 min
Response: 1002968
Conc: 6.60 ug/ml

Instrument :
FID_C
ClientSampleId :

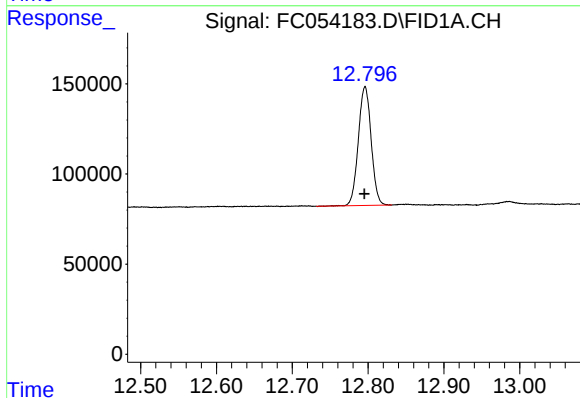


#12 1-chlorooctadecane (SURR)

R.T.: 12.796 min
Delta R.T.: 0.001 min
Response: 774967
Conc: 6.58 ug/ml

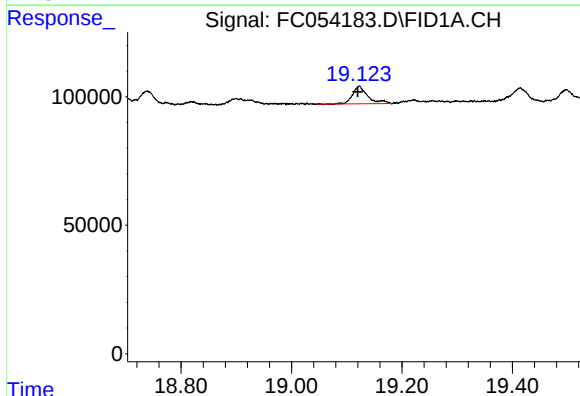


#19 n-Tetratriacontane (C34)

R.T.: 19.123 min
Delta R.T.: 0.003 min
Response: 130798
Conc: 1.12 ug/ml

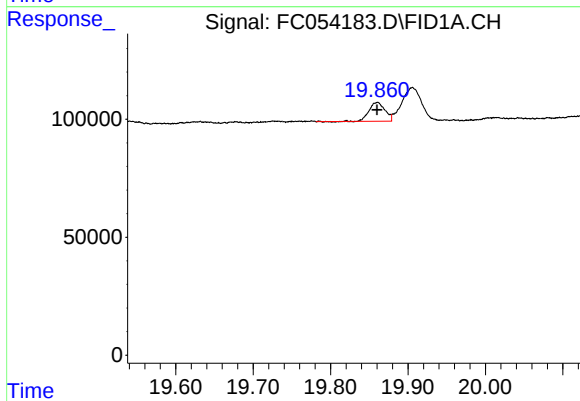

#20 n-Hexatriacontane (C36)


R.T.: 19.860 min
Delta R.T.: 0.000 min
Response: 113140
Conc: 1.03 ug/ml

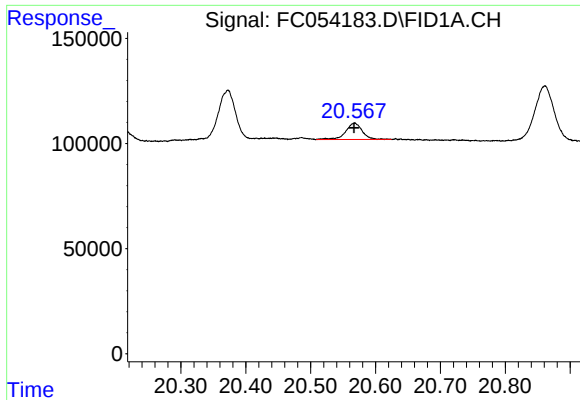

#21 n-Octatriacontane (C38)

R.T.: 20.567 min
Delta R.T.: 0.000 min
Response: 136393
Conc: 1.33 ug/ml

Instrument :
FID_C
ClientSampleId :

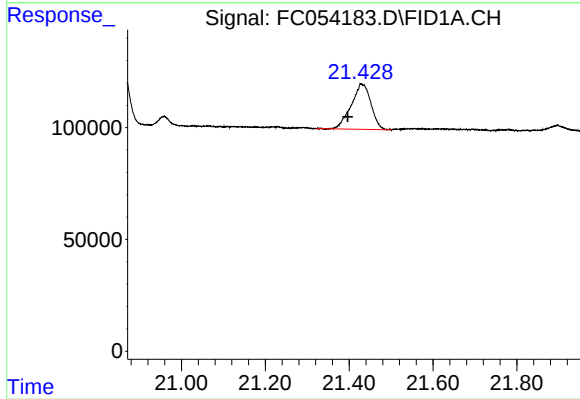

#22 n-Tetracontane (C40)

R.T.: 21.430 min
Delta R.T.: 0.034 min
Response: 660629
Conc: 6.17 ug/ml