

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC061022AL\  
 Data File : FC060202.D  
 Signal(s) : FID1A.CH  
 Acq On : 10 Jun 2022 22:40  
 Operator : UA/NP  
 Sample : N3269-03  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 14A-TP-8-(7.5-8.0)

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/13/2022  
 Supervised By :Ankita Jodhani 06/13/2022

Integration File: autoint1.e  
 Quant Time: Jun 10 23:07:58 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 052722.M  
 Quant Title : GC Extractables  
 QLast Update : Sat May 28 08:22:04 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units    |
|--------------------------------|--------|----------|---------------|
| -----                          |        |          |               |
| System Monitoring Compounds    |        |          |               |
| 9) S ortho-Terphenyl (SURR)    | 10.679 | 7653236  | 49.178 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 98.36%      |
| 12) S 1-chlorooctadecane (S... | 12.004 | 6772040  | 54.618 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 109.24%     |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC061022AL\  
Data File : FC060202.D  
Signal(s) : FID1A.CH  
Acq On : 10 Jun 2022 22:40  
Operator : UA/NP  
Sample : N3269-03  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
14A-TP-8-(7.5-8.0)


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/13/2022  
Supervised By :Ankita Jodhani 06/13/2022

Integration File: autoint1.e  
Quant Time: Jun 10 23:07:58 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 052722.M  
Quant Title : GC Extractables  
QLast Update : Sat May 28 08:22:04 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

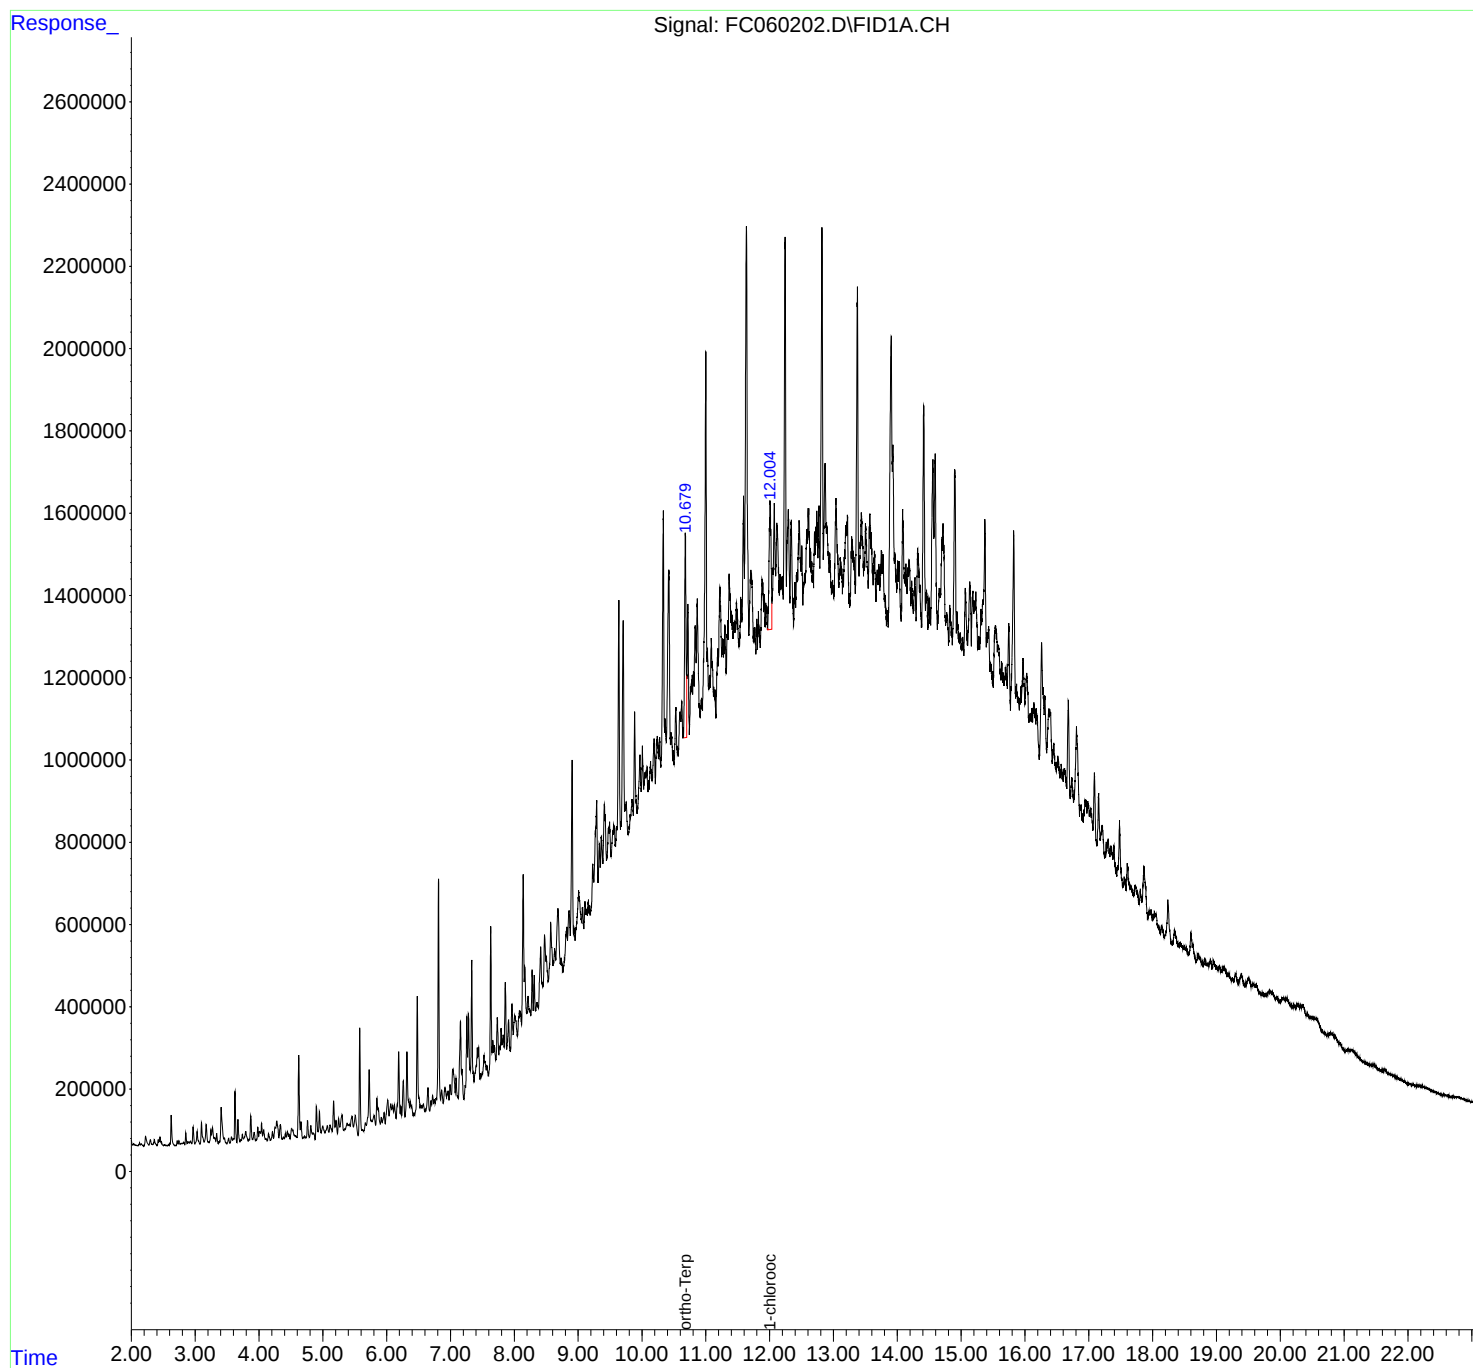

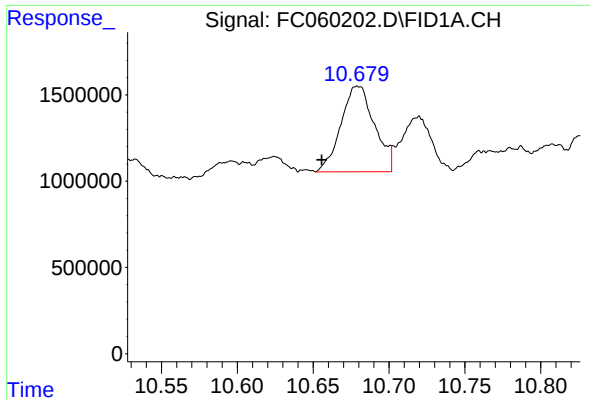


#9 ortho-Terphenyl (SURR)

R.T.: 10.679 min  
Delta R.T.: 0.023 min  
Response: 7653236  
Conc: 49.18 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
14A-TP-8-(7.5-8.0)

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/13/2022  
Supervised By :Ankita Jodhani 06/13/2022

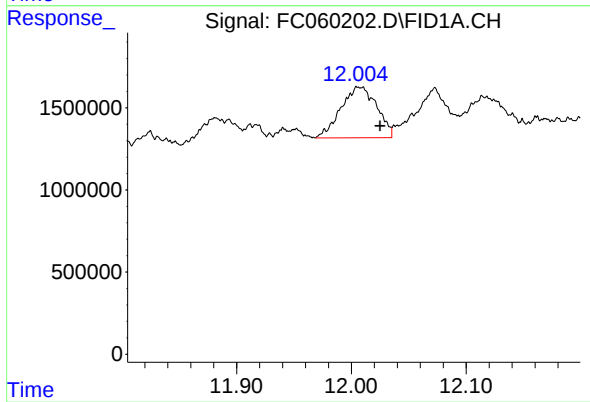

#12 1-chlorooctadecane (SURR)

R.T.: 12.004 min  
Delta R.T.: -0.021 min  
Response: 6772040  
Conc: 54.62 ug/ml m