

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061224AL\
Data File : FC066586.D
Signal(s) : FID1A.ch
Acq On : 12 Jun 2024 17:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 13 03:54:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052824.M
Quant Title : GC Extractables
QLast Update : Tue May 28 12:26:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.544	29202	0.237 ug/ml
19) T	n-Tetratriacontane (C34)	19.337	113194	0.944 ug/ml
20) T	n-Hexatriacontane (C36)	20.072	390461	3.223 ug/ml
21) T	n-Octatriacontane (C38)	20.782	75983	0.657 ug/ml
22) T	n-Tetracontane (C40)	21.729	376807	3.076 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061224AL\
Data File : FC066586.D
Signal(s) : FID1A.ch
Acq On : 12 Jun 2024 17:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 13 03:54:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052824.M
Quant Title : GC Extractables
QLast Update : Tue May 28 12:26:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

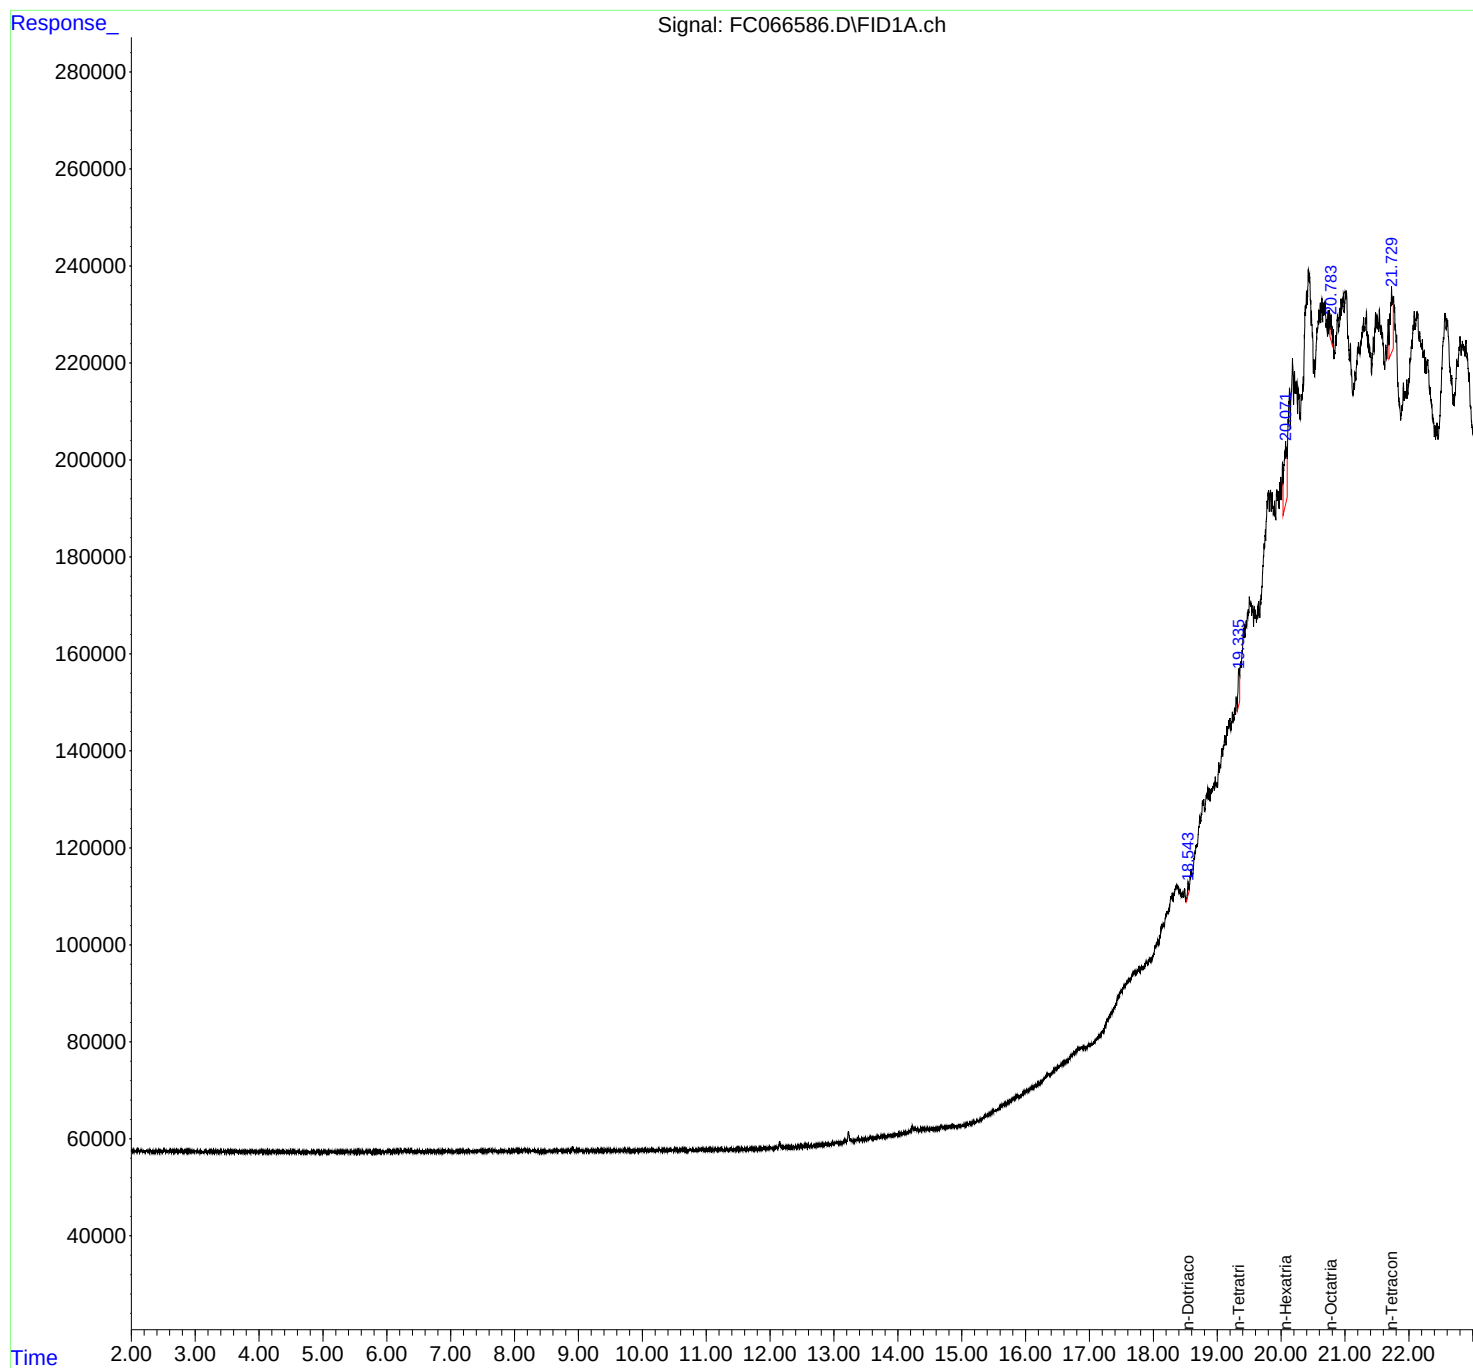


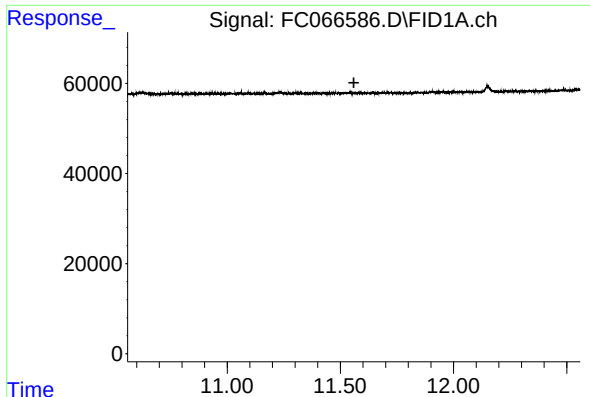

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.560 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

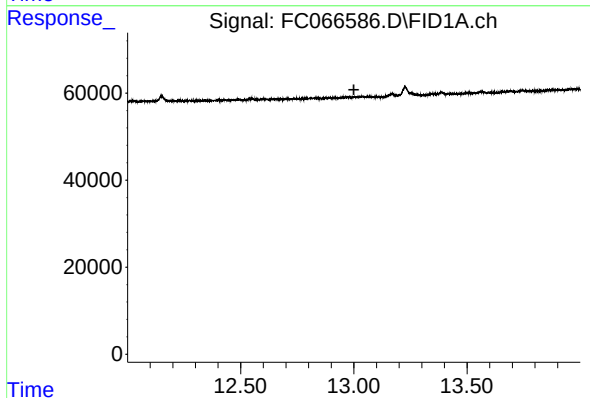


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.000 min
Response: 0
Conc: N.D.

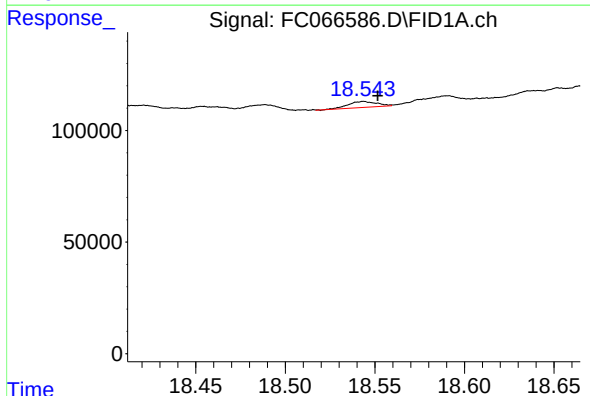


#18 n-Dotriacontane (C32)

R.T.: 18.544 min
Delta R.T.: -0.008 min
Response: 29202
Conc: 0.24 ug/ml

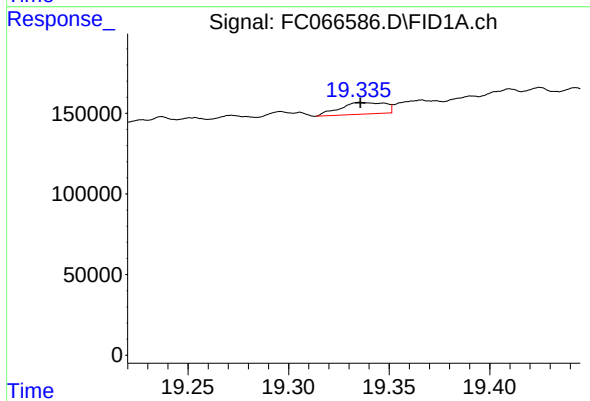

#19 n-Tetratriacontane (C34)


R.T.: 19.337 min
Delta R.T.: 0.001 min
Response: 113194
Conc: 0.94 ug/ml

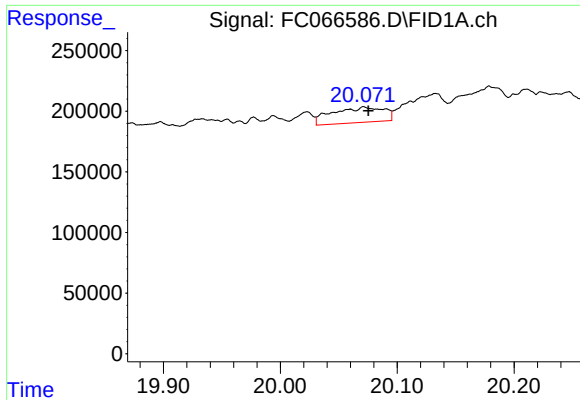

#20 n-Hexatriacontane (C36)


R.T.: 20.072 min
Delta R.T.: -0.003 min
Response: 390461
Conc: 3.22 ug/ml

Instrument :
FID_C
ClientSampleId :

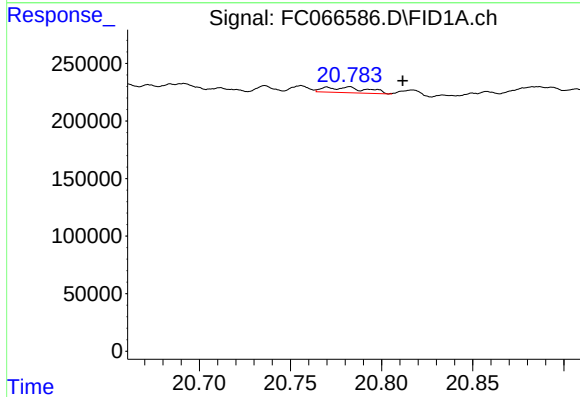

#21 n-Octatriacontane (C38)

R.T.: 20.782 min
Delta R.T.: -0.030 min
Response: 75983
Conc: 0.66 ug/ml

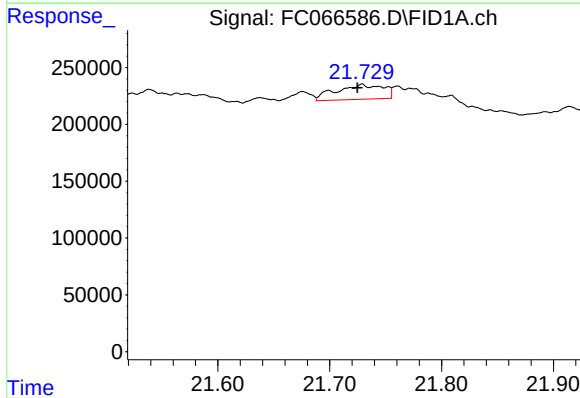

#22 n-Tetracontane (C40)

R.T.: 21.729 min
Delta R.T.: 0.004 min
Response: 376807
Conc: 3.08 ug/ml