

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061322AL\
 Data File : FC060217.D
 Signal(s) : FID1A.CH
 Acq On : 13 Jun 2022 13:30
 Operator : UA/NP
 Sample : N3269-04DL 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 14A-TP-8(14.5-15.0)DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/14/2022
 Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
 Quant Time: Jun 13 14:00:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 08:22:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.646	690867	4.439 ug/mlm
Spiked Amount 50.000		Recovery =	8.88%
12) S 1-chlorooctadecane (S...	12.015	594971	4.799 ug/mlm
Spiked Amount 50.000		Recovery =	9.60%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061322AL\
Data File : FC060217.D
Signal(s) : FID1A.CH
Acq On : 13 Jun 2022 13:30
Operator : UA/NP
Sample : N3269-04DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
14A-TP-8(14.5-15.0)DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
Quant Time: Jun 13 14:00:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

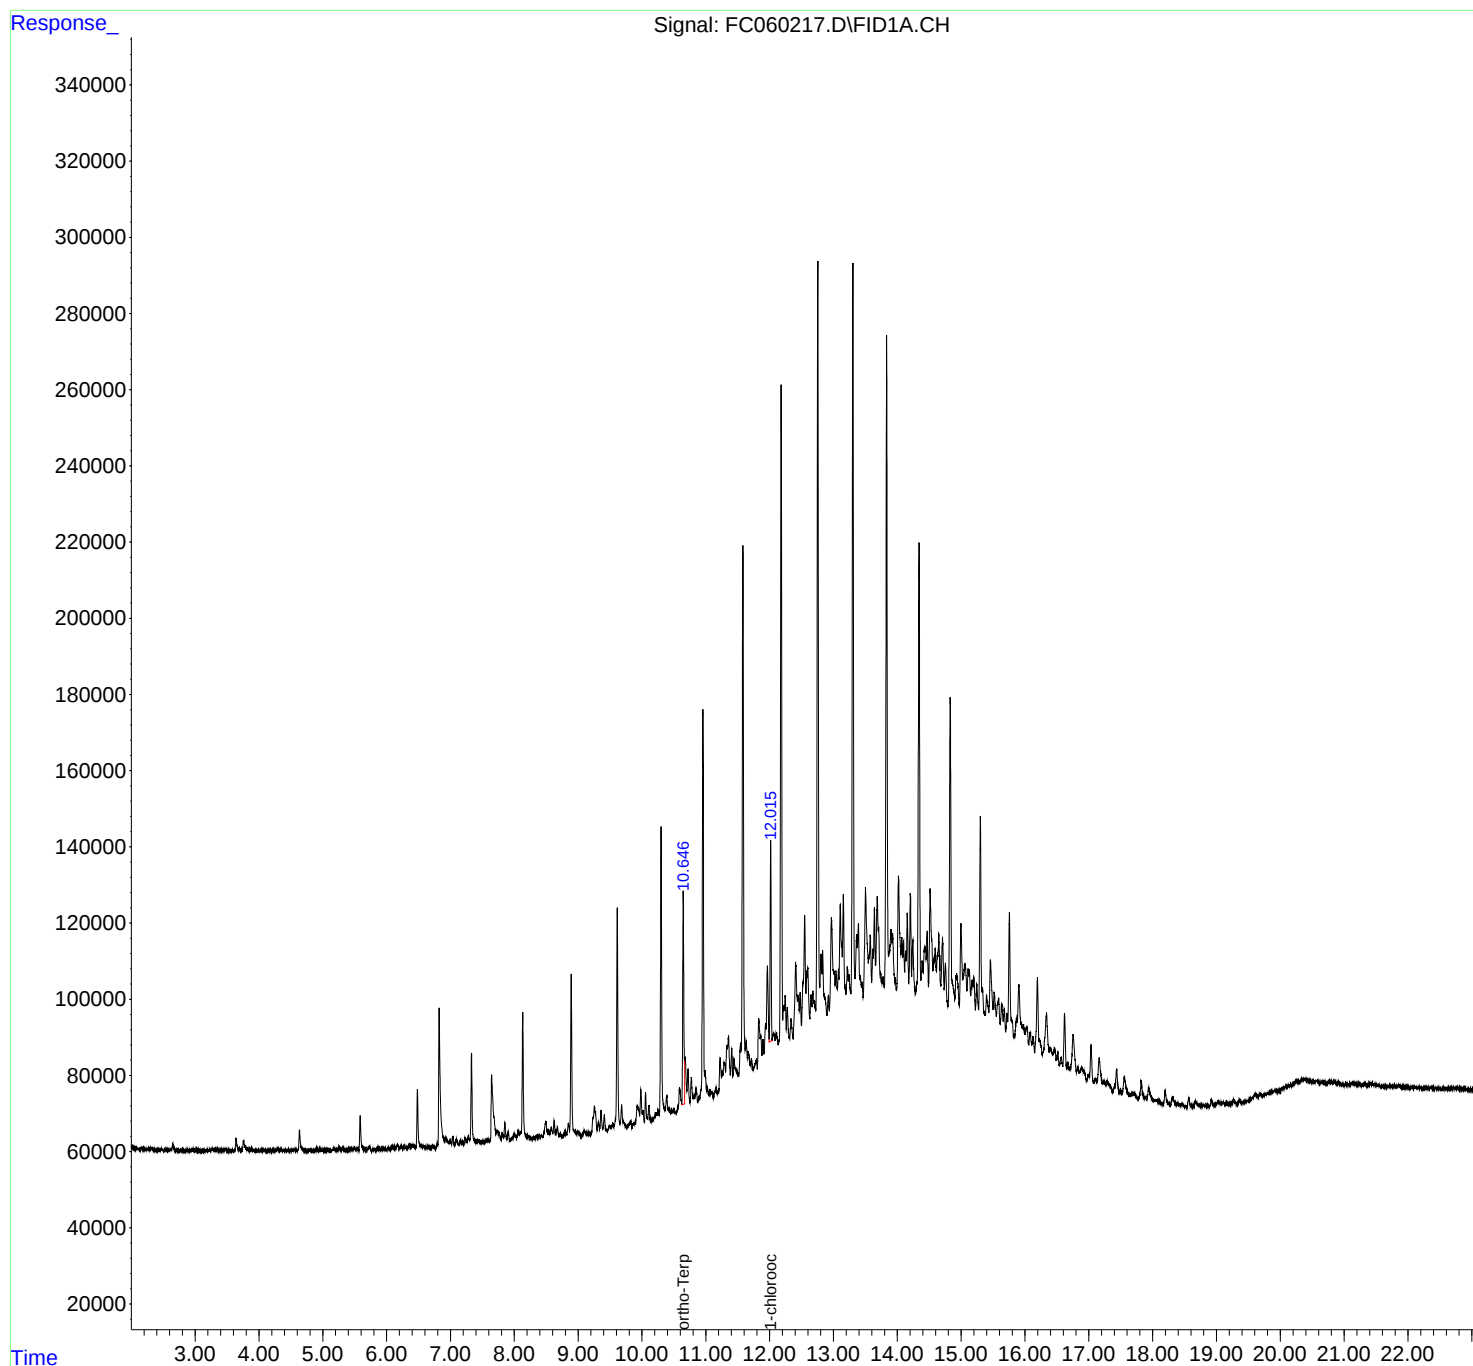

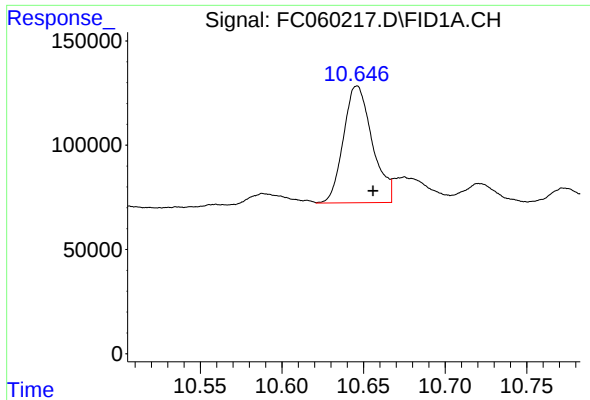


#9 ortho-Terphenyl (SURR)

R.T.: 10.646 min
Delta R.T.: -0.010 min
Response: 690867
Conc: 4.44 ug/ml

Instrument :
FID_C
ClientSampleId :
14A-TP-8(14.5-15.0)DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

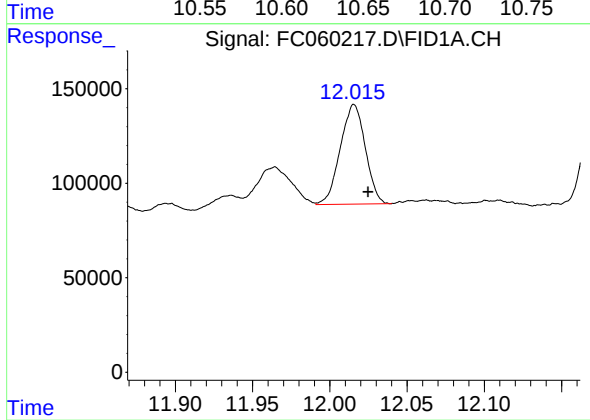

#12 1-chlorooctadecane (SURR)

R.T.: 12.015 min
Delta R.T.: -0.010 min
Response: 594971
Conc: 4.80 ug/ml m