

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061322AL\
 Data File : FC060219.D
 Signal(s) : FID1A.CH
 Acq On : 13 Jun 2022 15:04
 Operator : UA/NP
 Sample : N3296-03DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 Field Sampling Hourly RateDL

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 06/14/2022
 Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
 Quant Time: Jun 14 01:50:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 08:22:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.644	1460208	9.383 ug/ml
Spiked Amount 50.000		Recovery =	18.77%
12) S 1-chlorooctadecane (S...	12.013	1068403	8.617 ug/mlm
Spiked Amount 50.000		Recovery =	17.23%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061322AL\
Data File : FC060219.D
Signal(s) : FID1A.CH
Acq On : 13 Jun 2022 15:04
Operator : UA/NP
Sample : N3296-03DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
Field Sampling Hourly RateDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

Integration File: autoint1.e
Quant Time: Jun 14 01:50:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

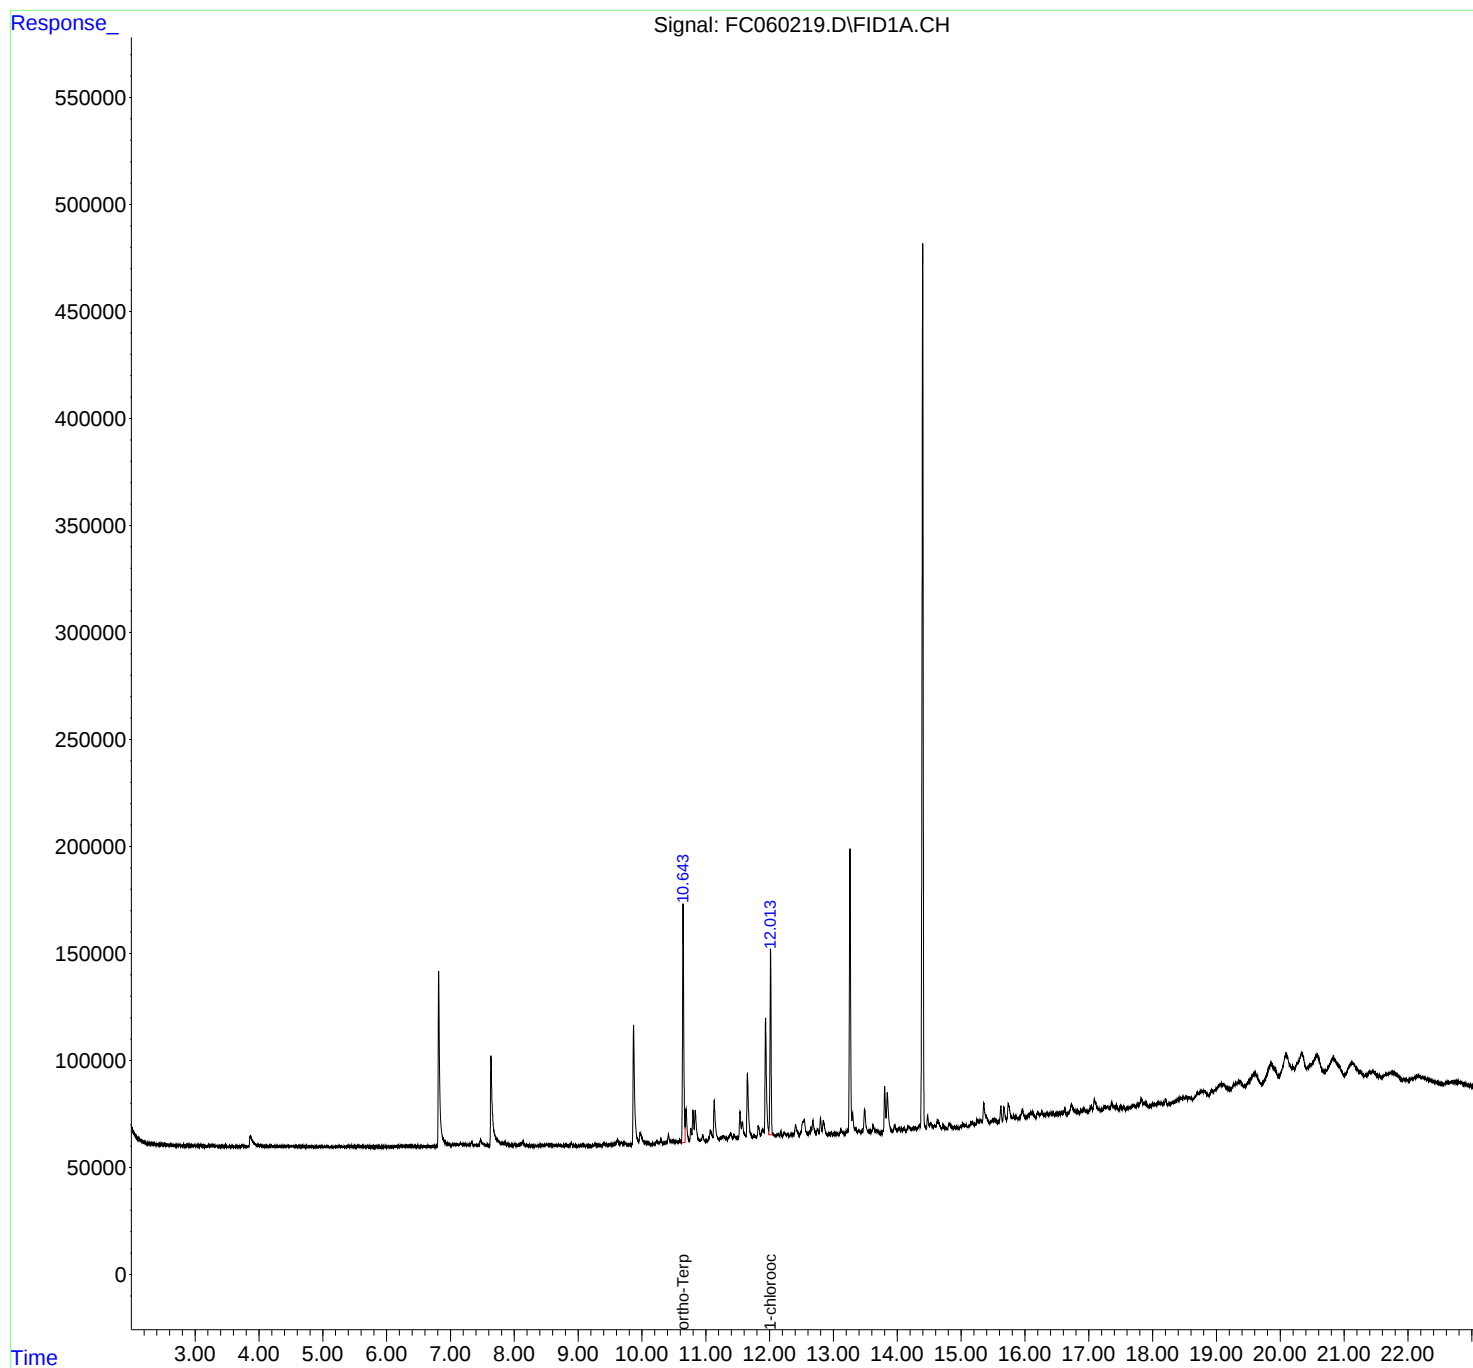

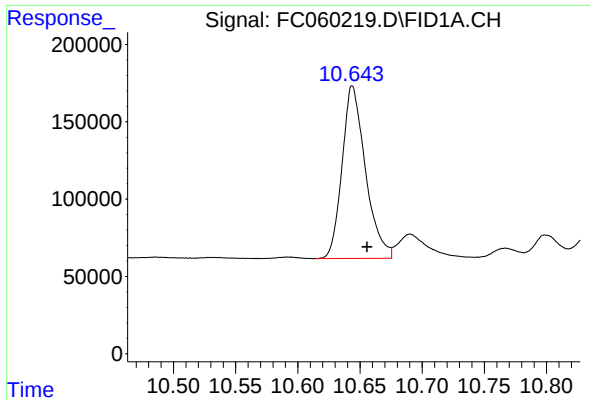


#9 ortho-Terphenyl (SURR)

R.T.: 10.644 min
Delta R.T.: -0.011 min
Response: 1460208
Conc: 9.38 ug/ml

Instrument :
FID_C
ClientSampleId :
Field Sampling Hourly RateDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2022
Supervised By :Ankita Jodhani 06/14/2022

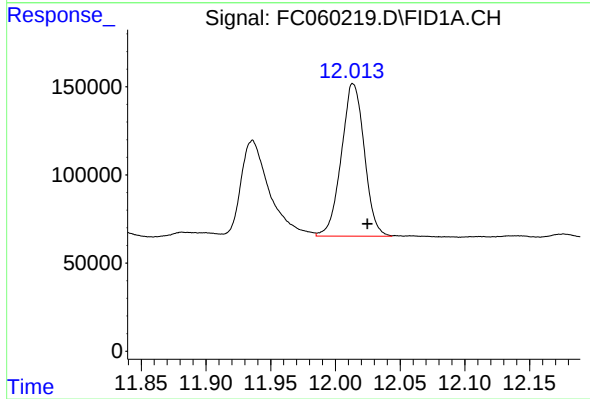

#12 1-chlorooctadecane (SURR)

R.T.: 12.013 min
Delta R.T.: -0.012 min
Response: 1068403
Conc: 8.62 ug/ml m