

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061324AL\
Data File : FC066604.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2024 09:47
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 03:13:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052824.M
Quant Title : GC Extractables
QLast Update : Tue May 28 12:26:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.534	22617	0.184 ug/ml
19) T	n-Tetratriacontane (C34)	19.318	33136	0.276 ug/ml
22) T	n-Tetracontane (C40)	21.755	136174	1.112 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061324AL\
Data File : FC066604.D
Signal(s) : FID1A.ch
Acq On : 13 Jun 2024 09:47
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 03:13:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052824.M
Quant Title : GC Extractables
QLast Update : Tue May 28 12:26:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

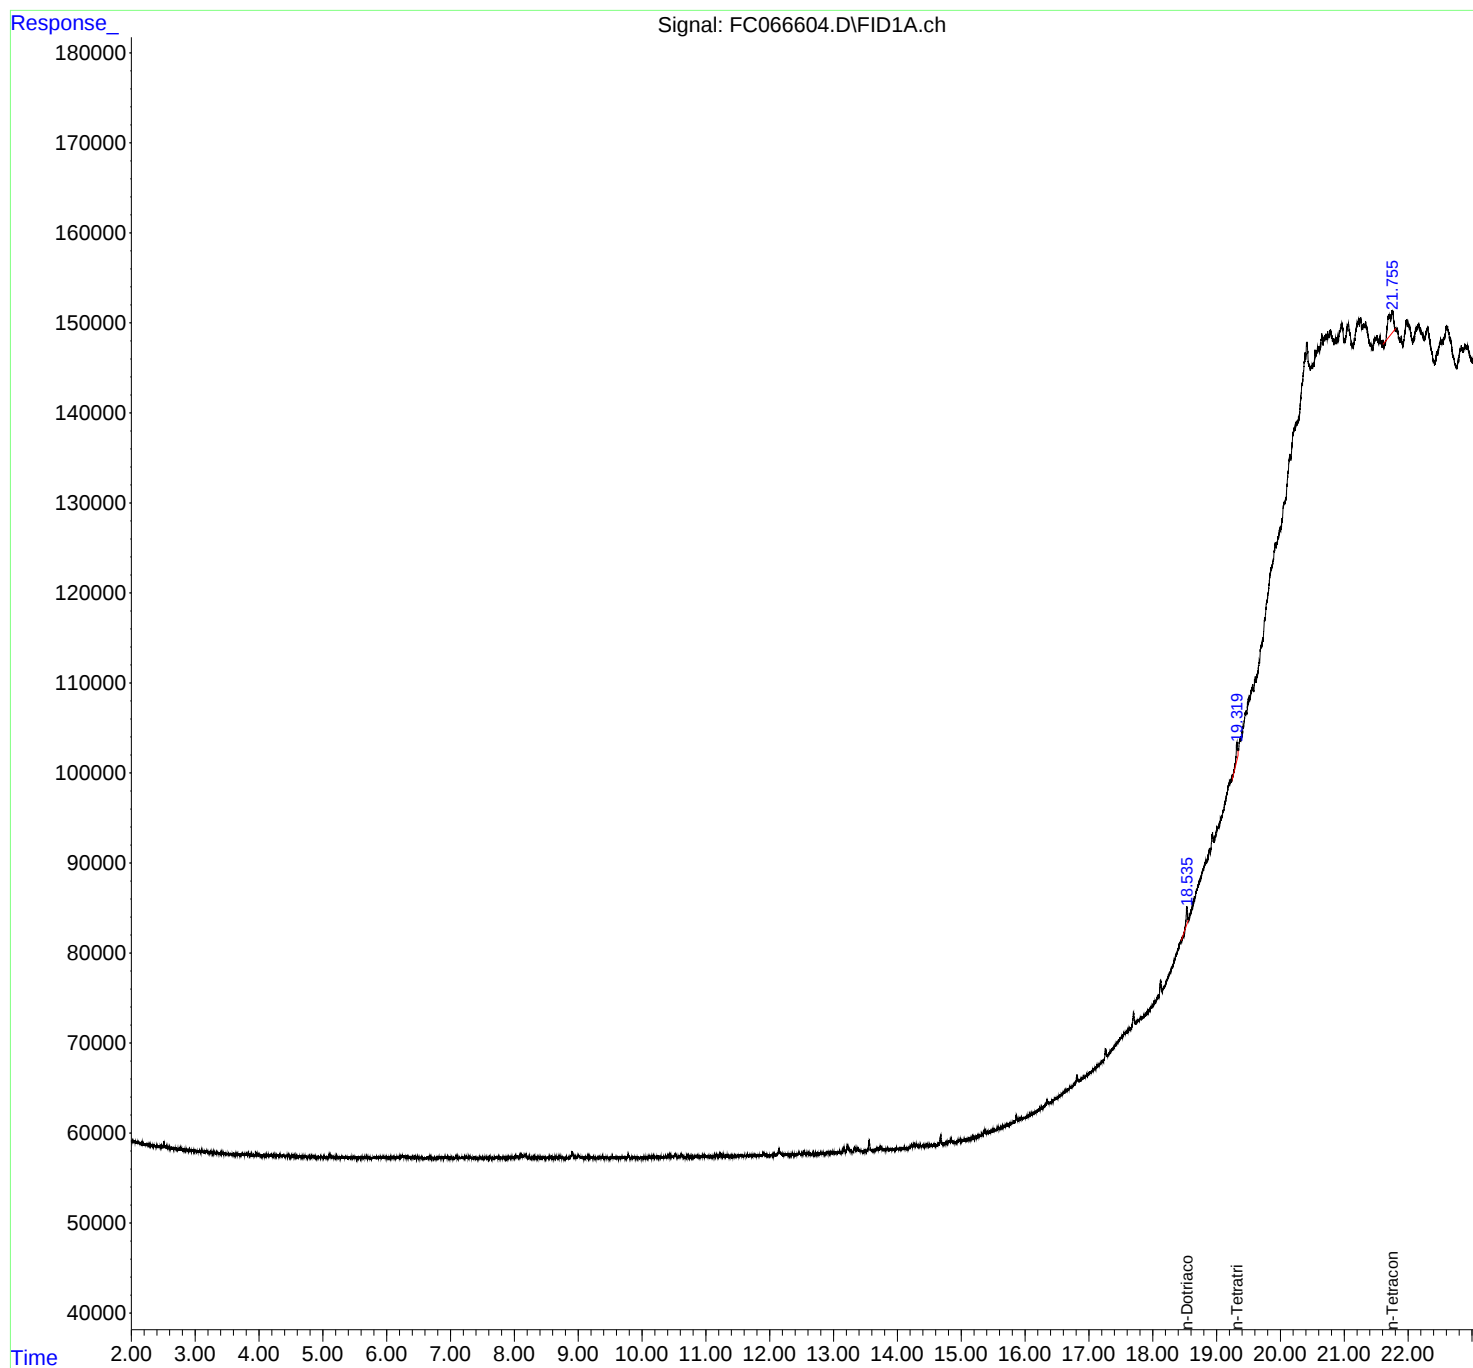


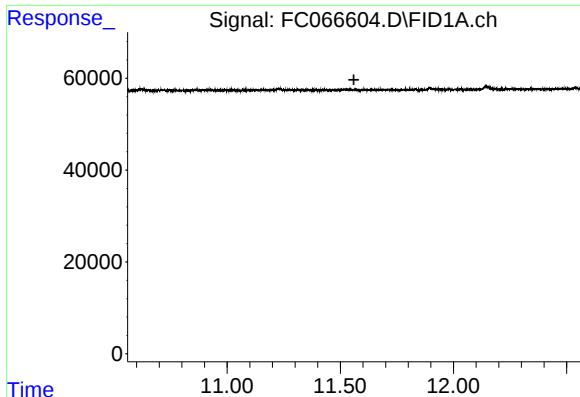

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.560 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

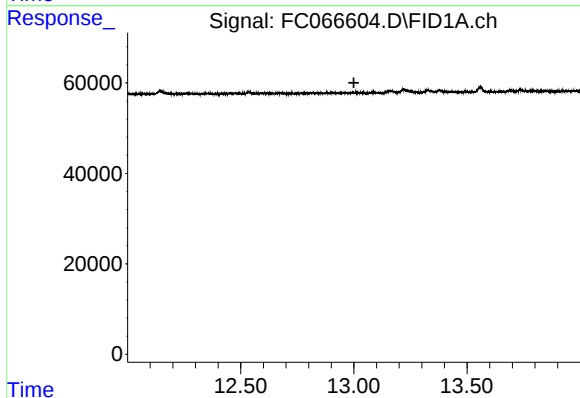


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.000 min
Response: 0
Conc: N.D.

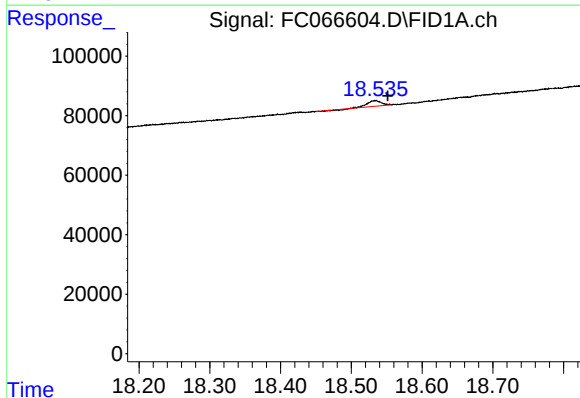


#18 n-Dotriacontane (C32)

R.T.: 18.534 min
Delta R.T.: -0.018 min
Response: 22617
Conc: 0.18 ug/ml

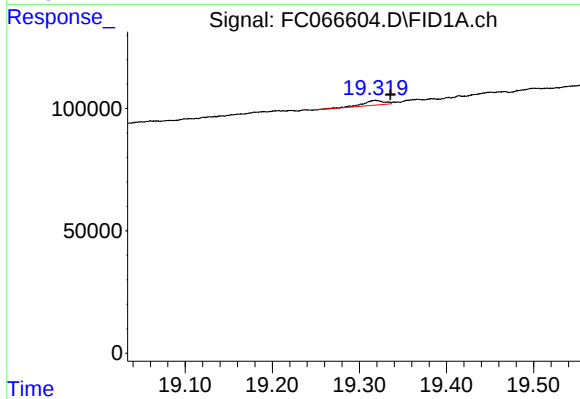

#19 n-Tetratriacontane (C34)

R.T.: 19.318 min
Delta R.T.: -0.017 min
Response: 33136
Conc: 0.28 ug/ml

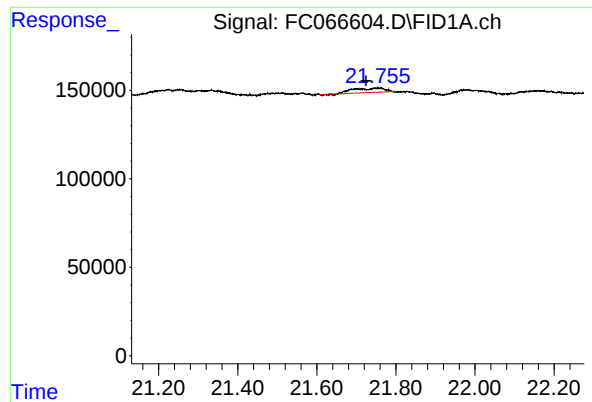

#22 n-Tetracontane (C40)

R.T.: 21.755 min
Delta R.T.: 0.030 min
Response: 136174
Conc: 1.11 ug/ml

Instrument :

FID_C

ClientSampleId :