

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
Data File : FC063856.D
Signal(s) : FID1A.ch
Acq On : 16 Jun 2023 09:21
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 00:11:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.785	91265	0.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
Data File : FC063856.D
Signal(s) : FID1A.ch
Acq On : 16 Jun 2023 09:21
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 00:11:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

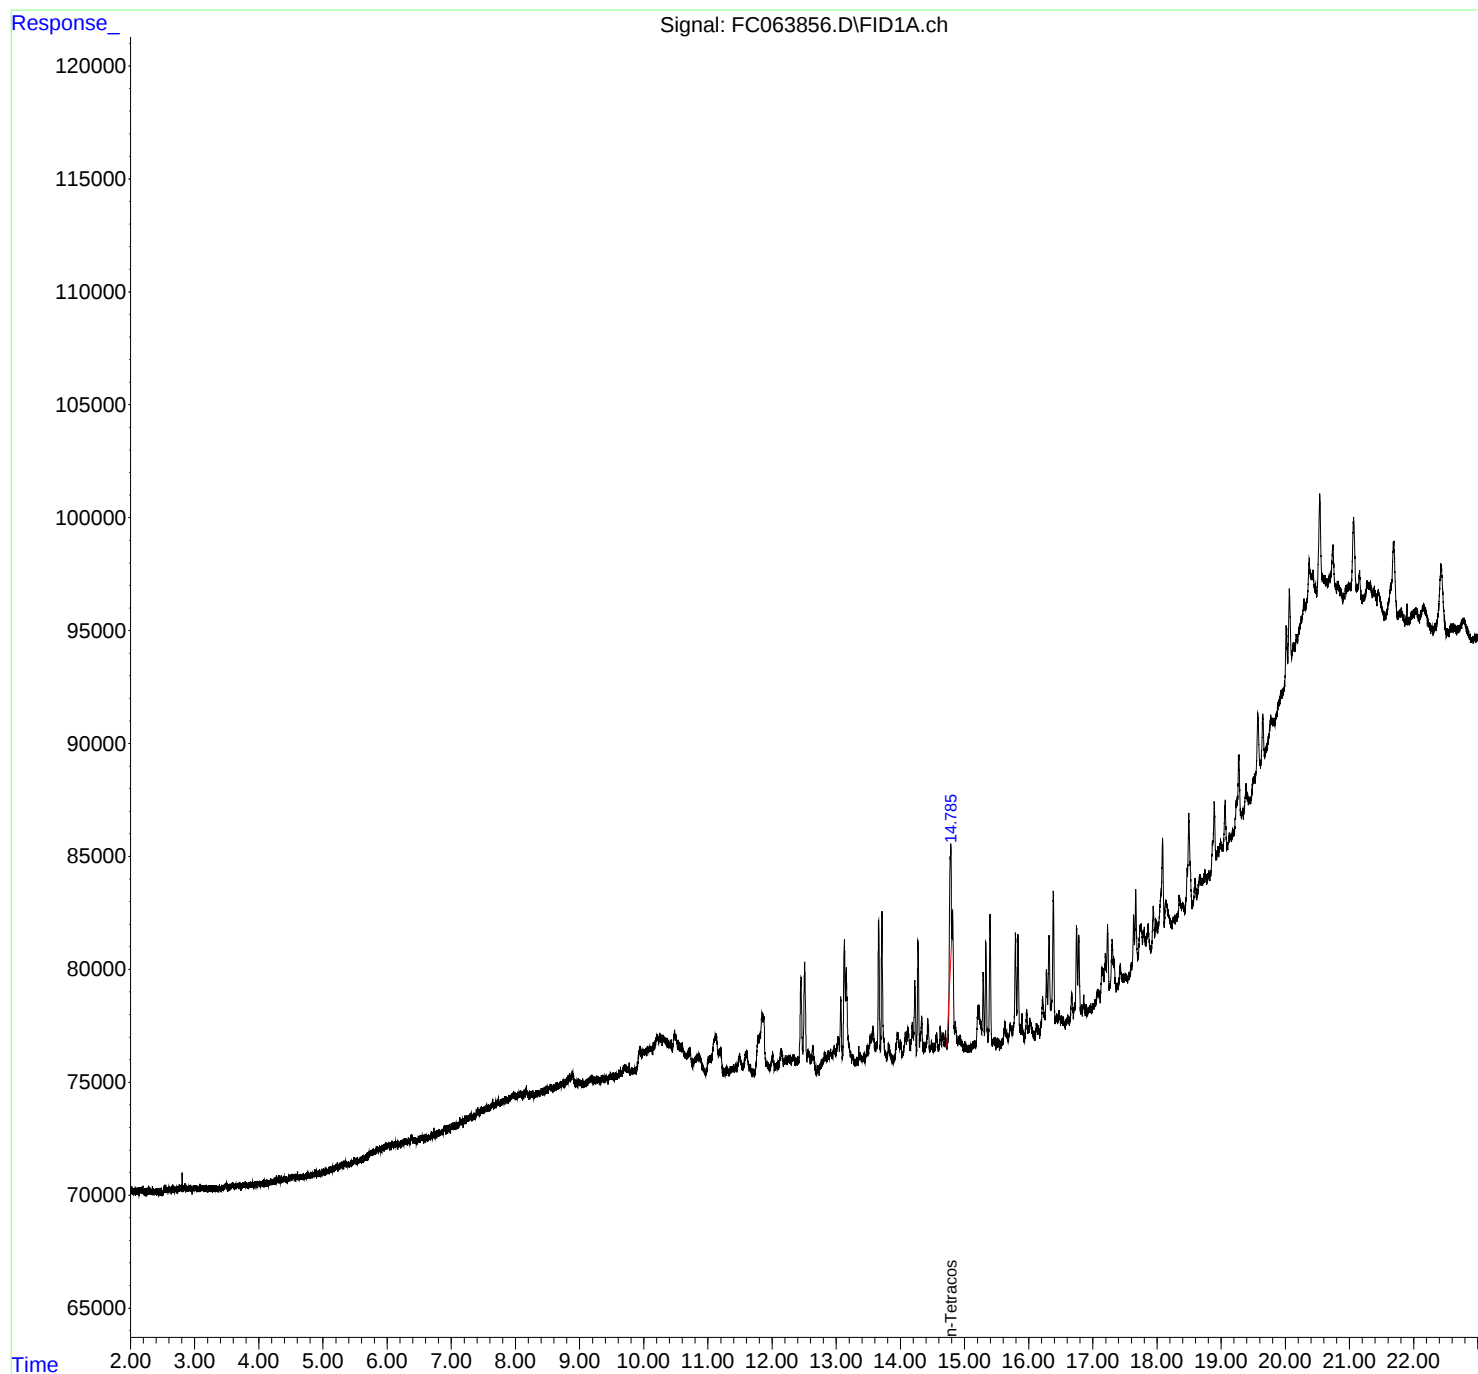


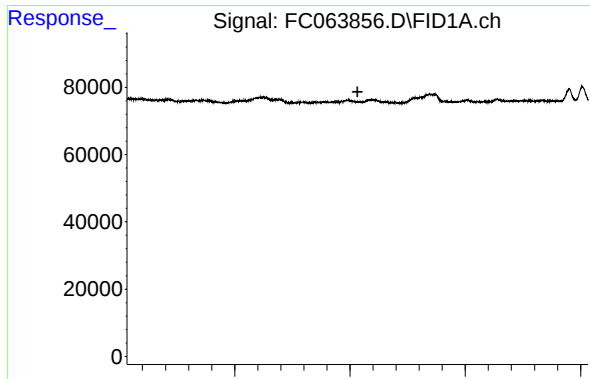

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.533 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

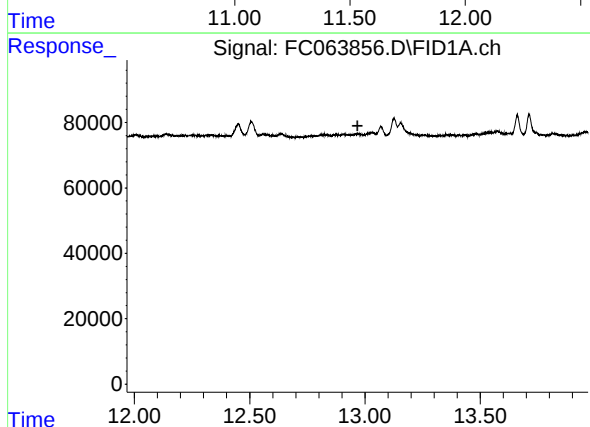

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.968 min
Response: 0
Conc: N.D.

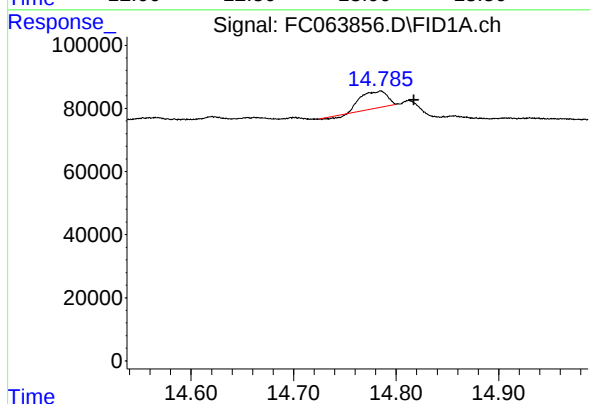

#14 n-Tetracosane (C24)

R.T.: 14.785 min
Delta R.T.: -0.033 min
Response: 91265
Conc: 0.67 ug/ml