

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
 Data File : FC063866.D
 Signal(s) : FID1A.ch
 Acq On : 16 Jun 2023 21:52
 Operator : YP/AJ
 Sample : 03223-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 00:12:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
 Quant Title : GC Extractables
 QLast Update : Sat May 27 06:12:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.967	6904595	54.038 ug/ml
Spiked Amount 50.000		Recovery =	108.08%
Target Compounds			
15) T n-Hexacosane (C26)	15.837	76460	0.577 ug/ml
16) T n-Octacosane (C28)	16.782	281703	2.219 ug/ml
17) T n-Tricontane (C30)	17.664	518704	4.060 ug/ml
18) T n-Dotriacontane (C32)	18.495	850408	6.834 ug/ml
19) T n-Tetratriacontane (C34)	19.278	1401957	11.370 ug/ml
20) T n-Hexatriacontane (C36)	20.013	1618966	13.489 ug/ml
21) T n-Octatriacontane (C38)	20.739	1933778	16.017 ug/ml
22) T n-Tetracontane (C40)	21.632	1639278	13.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
Data File : FC063866.D
Signal(s) : FID1A.ch
Acq On : 16 Jun 2023 21:52
Operator : YP/AJ
Sample : 03223-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 00:12:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

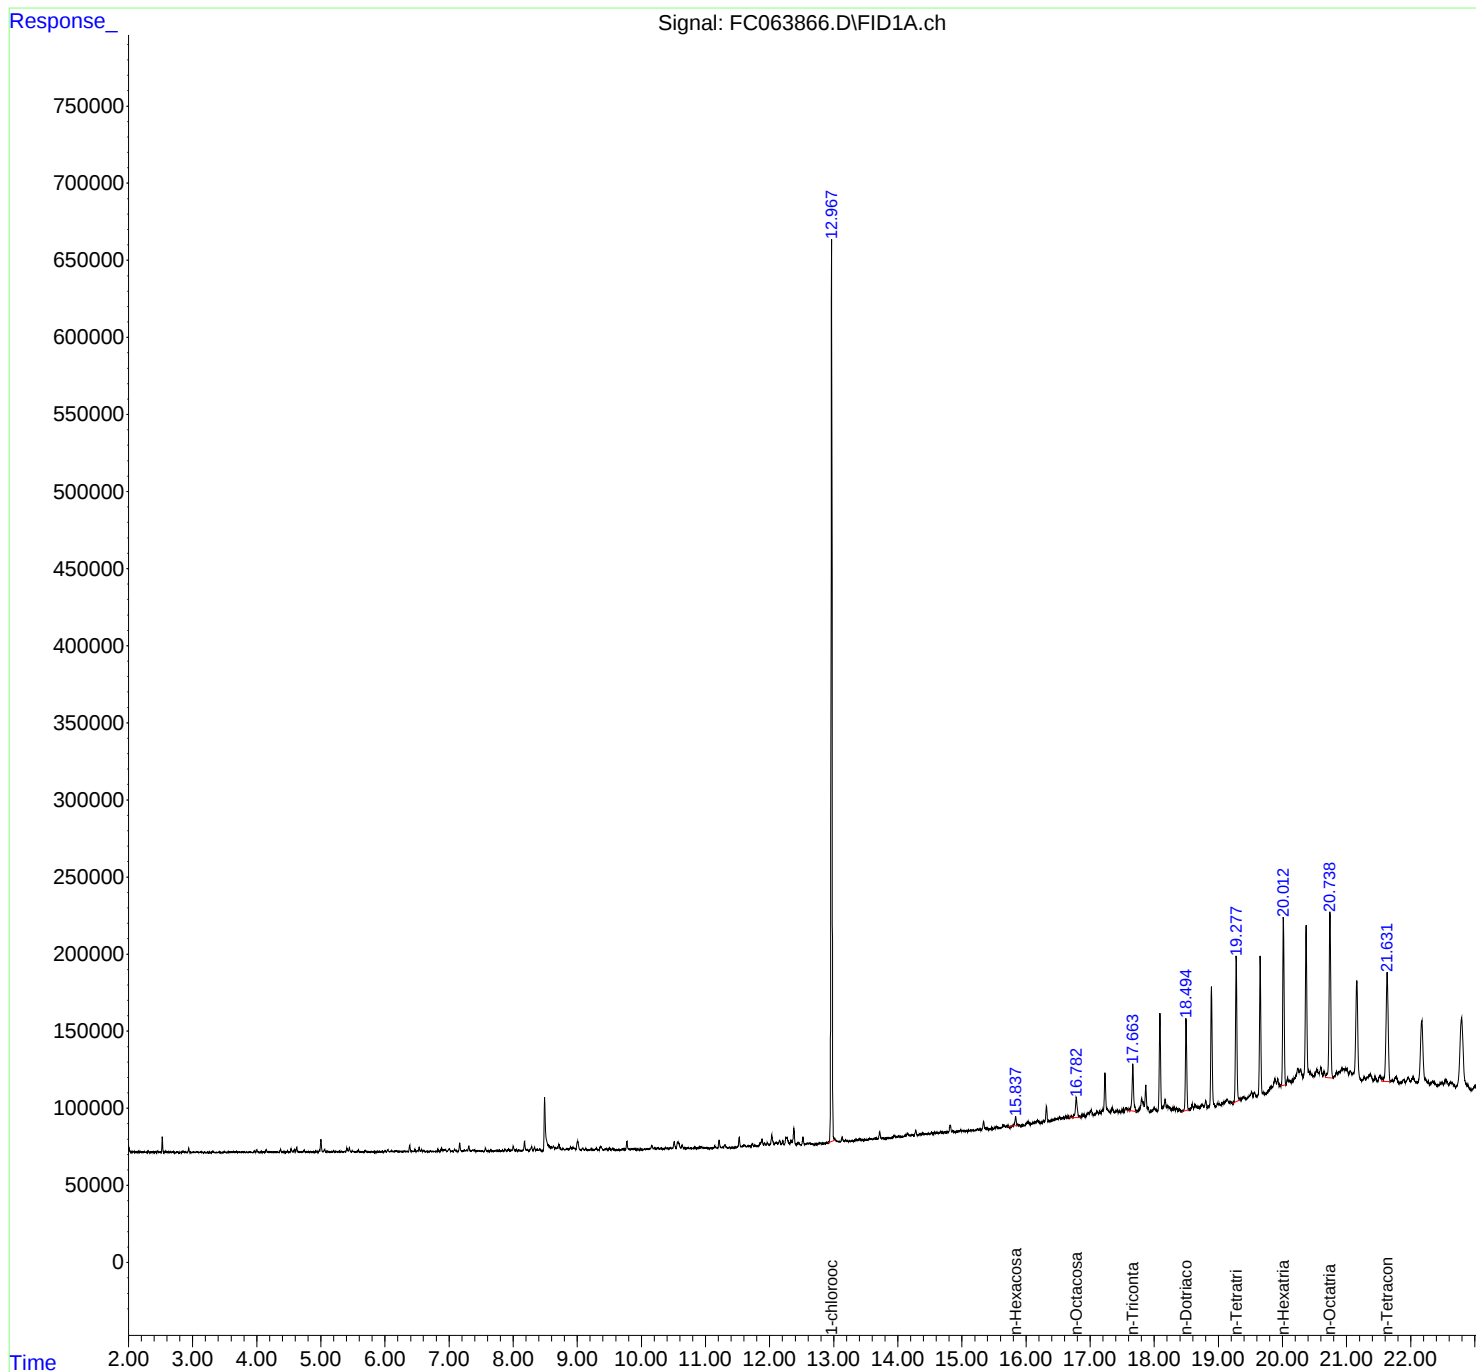


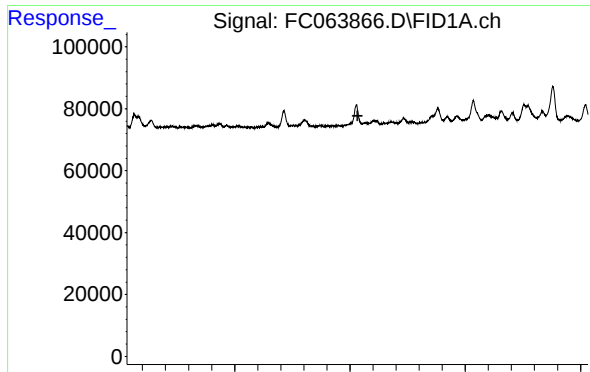

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.533 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

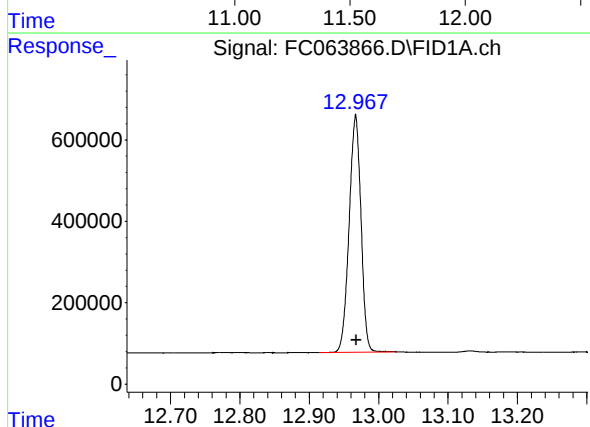


#12 1-chlorooctadecane (SURR)

R.T.: 12.967 min
Delta R.T.: 0.000 min
Response: 6904595
Conc: 54.04 ug/ml

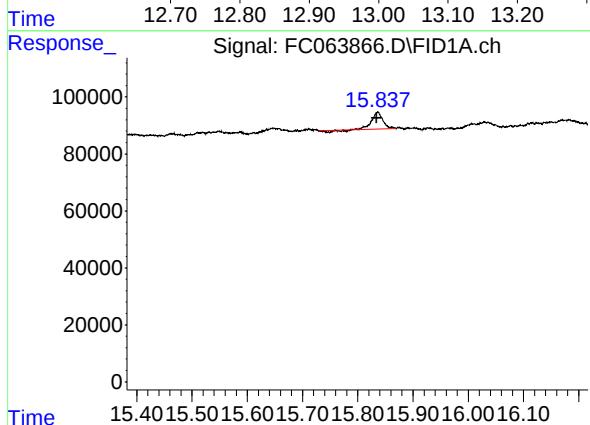


#15 n-Hexacosane (C26)

R.T.: 15.837 min
Delta R.T.: 0.003 min
Response: 76460
Conc: 0.58 ug/ml

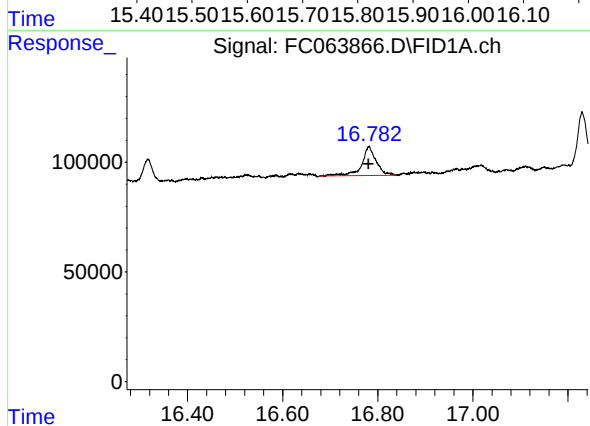

#16 n-Octacosane (C28)


R.T.: 16.782 min
Delta R.T.: 0.000 min
Response: 281703
Conc: 2.22 ug/ml

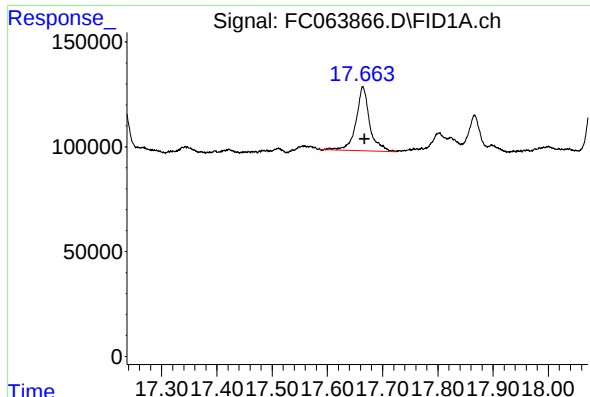

#17 n-Tricontane (C30)


R.T.: 17.664 min
Delta R.T.: -0.003 min
Response: 518704
Conc: 4.06 ug/ml

Instrument :
FID_C
ClientSampleId :

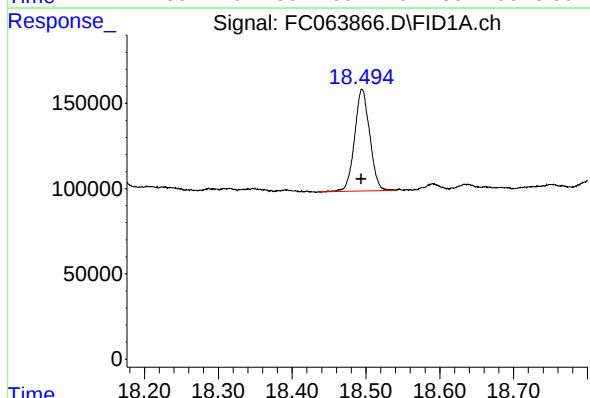


#18 n-Dotriacontane (C32)

R.T.: 18.495 min
Delta R.T.: 0.000 min
Response: 850408
Conc: 6.83 ug/ml

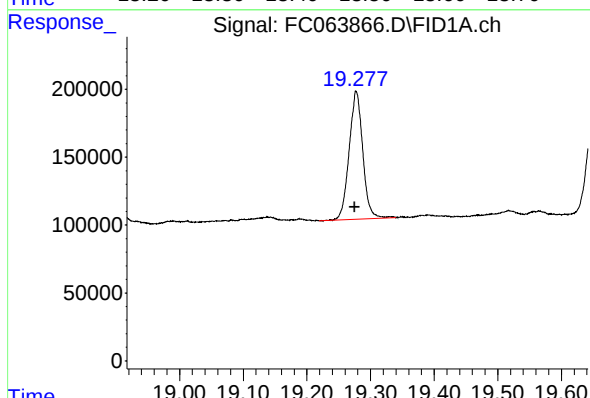


#19 n-Tetratriacontane (C34)

R.T.: 19.278 min
Delta R.T.: 0.002 min
Response: 1401957
Conc: 11.37 ug/ml

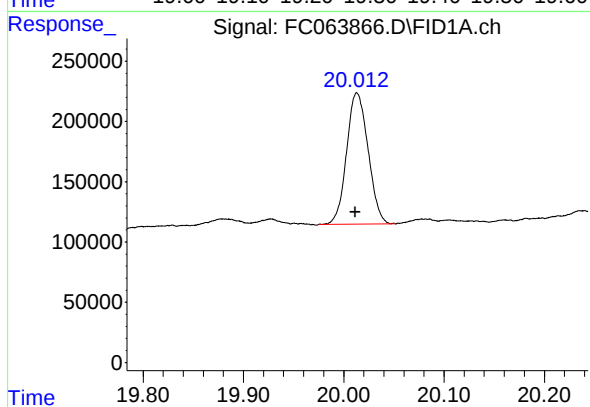

#20 n-Hexatriacontane (C36)


R.T.: 20.013 min
Delta R.T.: 0.002 min
Response: 1618966
Conc: 13.49 ug/ml

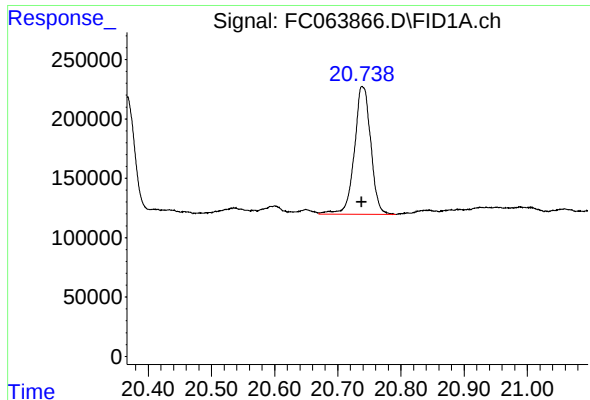

#21 n-Octatriacontane (C38)

R.T.: 20.739 min
Delta R.T.: 0.001 min
Response: 1933778
Conc: 16.02 ug/ml

Instrument :
FID_C
ClientSampleId :

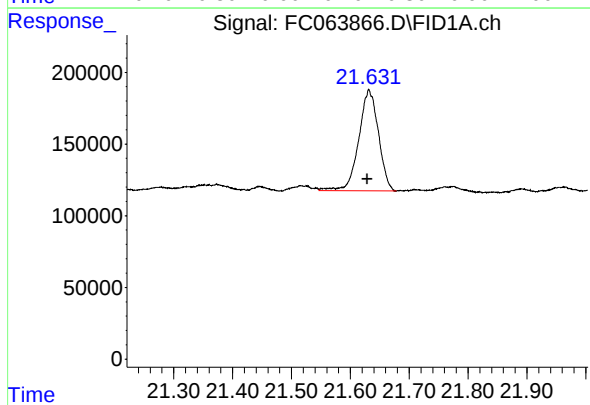

#22 n-Tetracontane (C40)

R.T.: 21.632 min
Delta R.T.: 0.003 min
Response: 1639278
Conc: 13.53 ug/ml