

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
 Data File : FC063870.D
 Signal(s) : FID1A.ch
 Acq On : 17 Jun 2023 00:40
 Operator : YP/AJ
 Sample : 03282-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 04:03:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
 Quant Title : GC Extractables
 QLast Update : Sat May 27 06:12:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.966	2962605	23.187 ug/ml
Spiked Amount 50.000		Recovery =	46.37%
Target Compounds			
4) T n-Dodecane (C12)	6.386	88831	0.543 ug/ml
14) T n-Tetracosane (C24)	14.815	87397	0.637 ug/ml
15) T n-Hexacosane (C26)	15.834	92185	0.695 ug/ml
16) T n-Octacosane (C28)	16.781	118791	0.936 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061623AL\
Data File : FC063870.D
Signal(s) : FID1A.ch
Acq On : 17 Jun 2023 00:40
Operator : YP/AJ
Sample : 03282-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 04:03:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

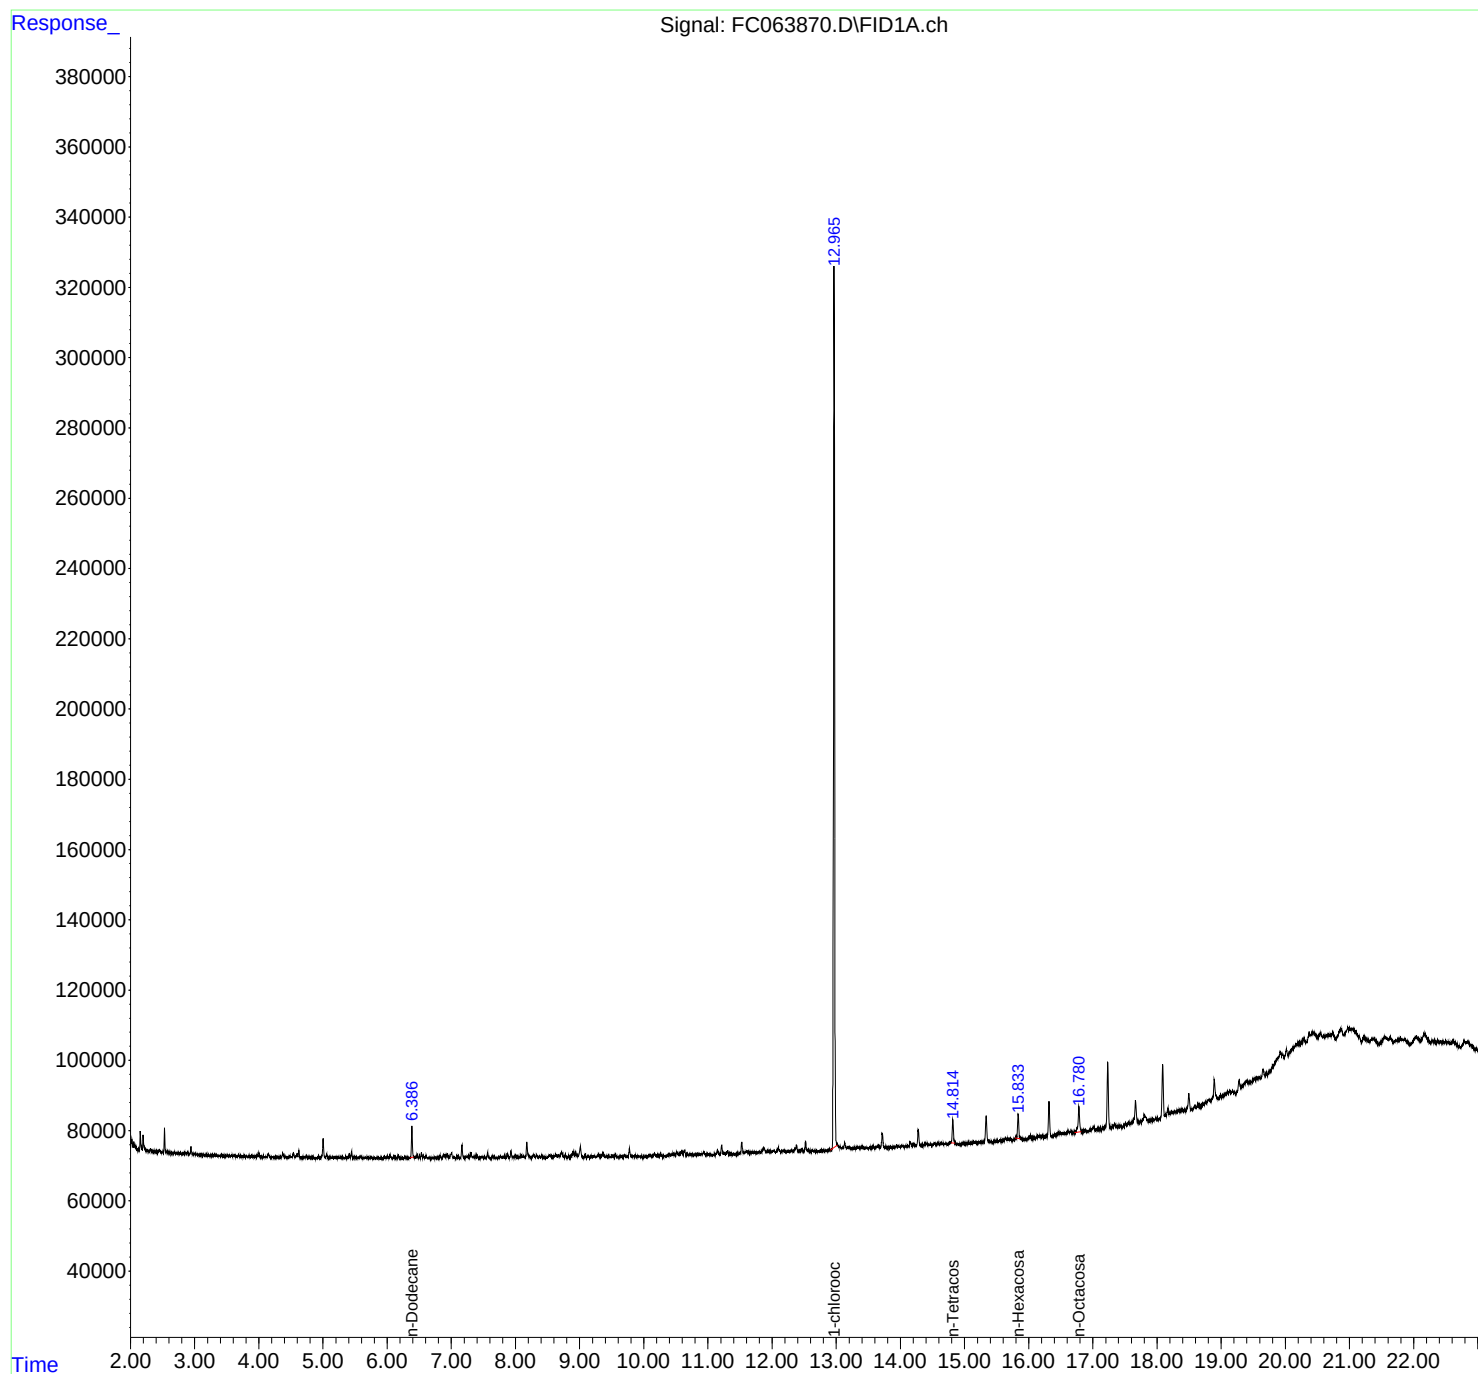


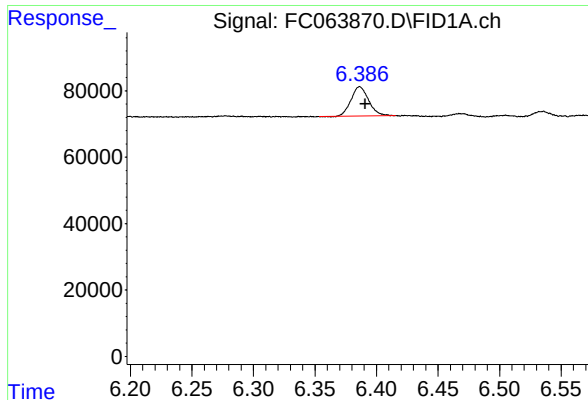

#4 n-Dodecane (C12)


R.T.: 6.386 min
Delta R.T.: -0.005 min
Response: 88831
Conc: 0.54 ug/ml

Instrument :
FID_C
ClientSampleId :

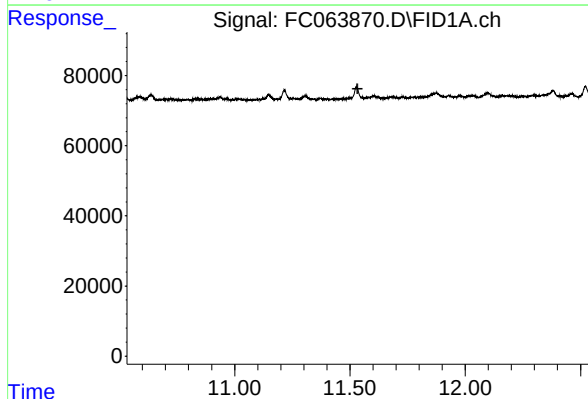


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.533 min
Response: 0
Conc: N.D.

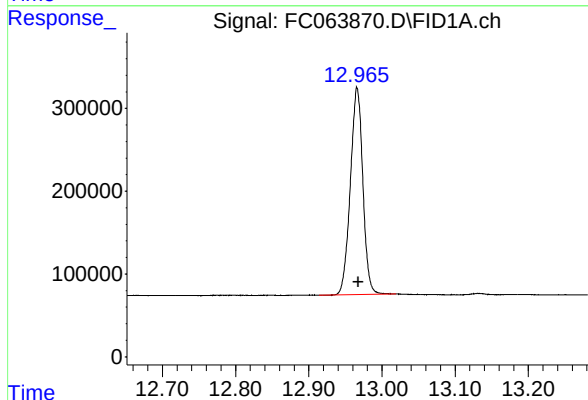


#12 1-chlorooctadecane (SURR)

R.T.: 12.966 min
Delta R.T.: -0.002 min
Response: 2962605
Conc: 23.19 ug/ml

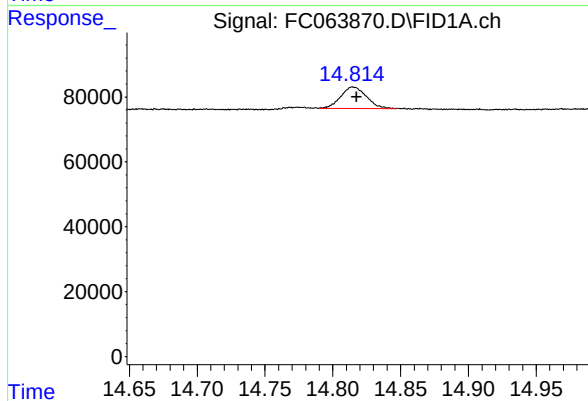

#14 n-Tetracosane (C24)


R.T.: 14.815 min
Delta R.T.: -0.003 min
Response: 87397
Conc: 0.64 ug/ml

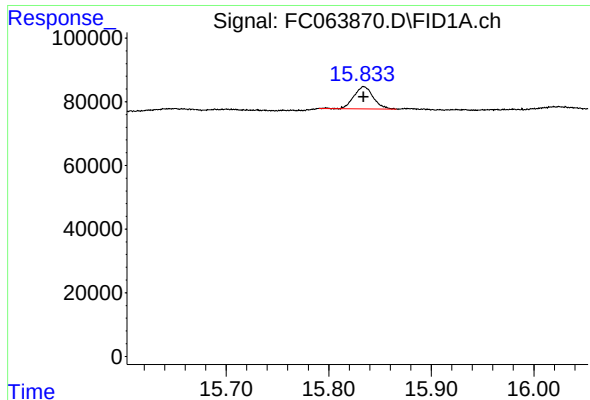

#15 n-Hexacosane (C26)

R.T.: 15.834 min
Delta R.T.: 0.000 min
Response: 92185
Conc: 0.70 ug/ml

Instrument :
FID_C
ClientSampleId :

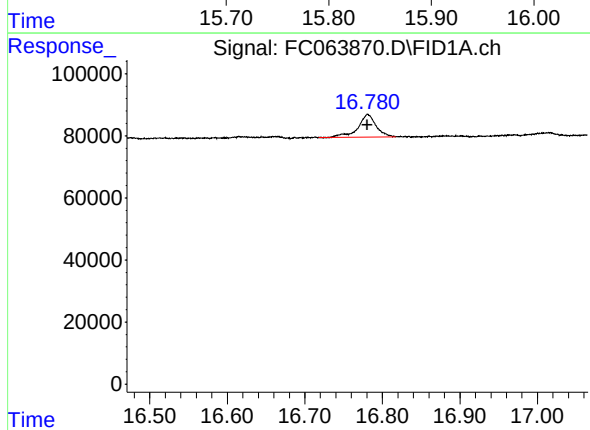

#16 n-Octacosane (C28)

R.T.: 16.781 min
Delta R.T.: 0.000 min
Response: 118791
Conc: 0.94 ug/ml