

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061820AL\
 Data File : FC047911.D
 Signal(s) : FID1A.CH
 Acq On : 18 Jun 2020 7:27
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Jun 19 02:16:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 060920.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 10 08:39:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	15.007	59940	0.522 ug/ml
15) T n-Hexacosane (C26)	15.991	128423	1.124 ug/ml
16) T n-Octacosane (C28)	16.935	218715	1.924 ug/ml
17) T n-Tricontane (C30)	17.818	268369	2.449 ug/ml
18) T n-Dotriacontane (C32)	18.643	245646	2.478 ug/ml
19) T n-Tetratriacontane (C34)	19.422	120460	1.315 ug/ml
20) T n-Hexatriacontane (C36)	20.158	238320	2.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061820AL\
Data File : FC047911.D
Signal(s) : FID1A.CH
Acq On : 18 Jun 2020 7:27
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 19 02:16:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 060920.M
Quant Title : GC Extractables
QLast Update : Wed Jun 10 08:39:57 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

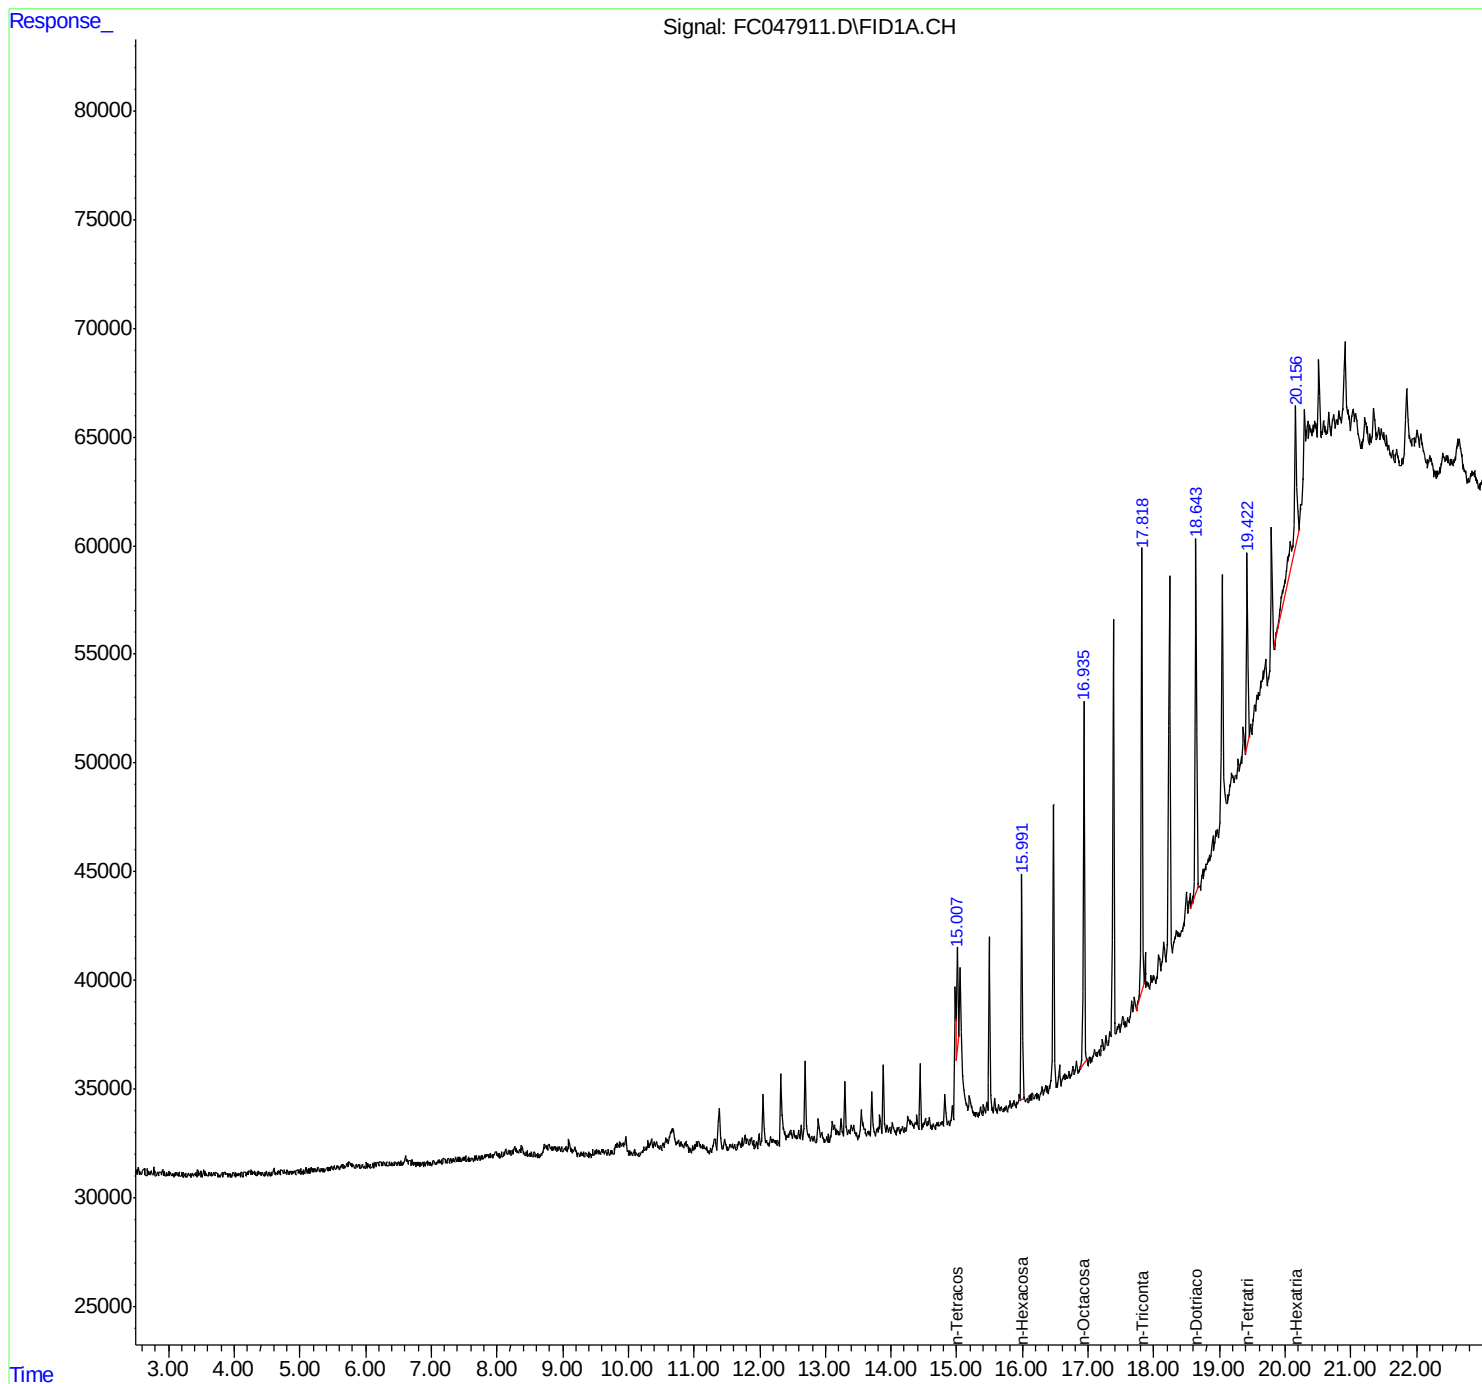


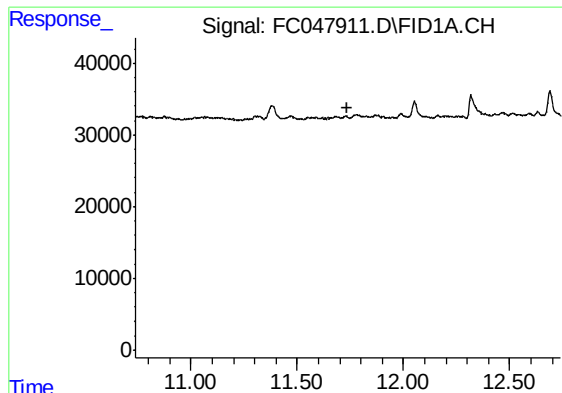

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.739 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
MECL2

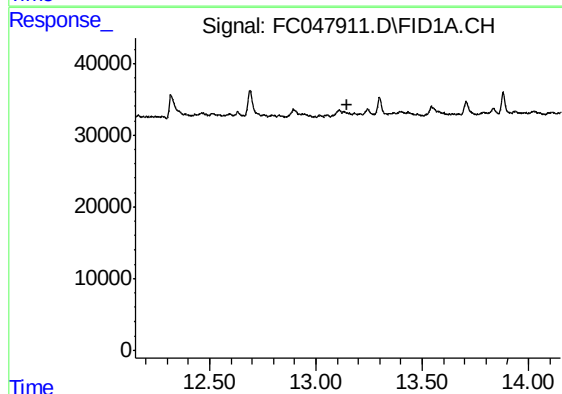


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.150 min
Response: 0
Conc: N.D.

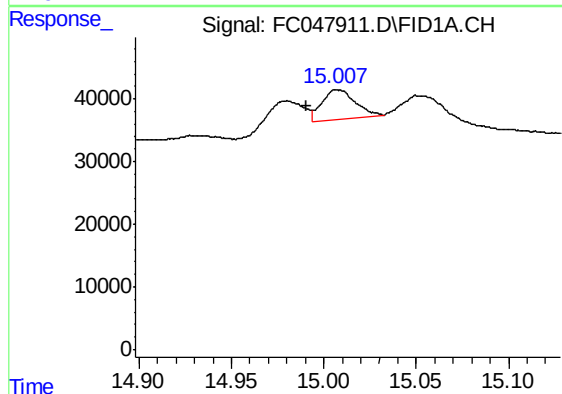


#14 n-Tetracosane (C24)

R.T.: 15.007 min
Delta R.T.: 0.017 min
Response: 59940
Conc: 0.52 ug/ml

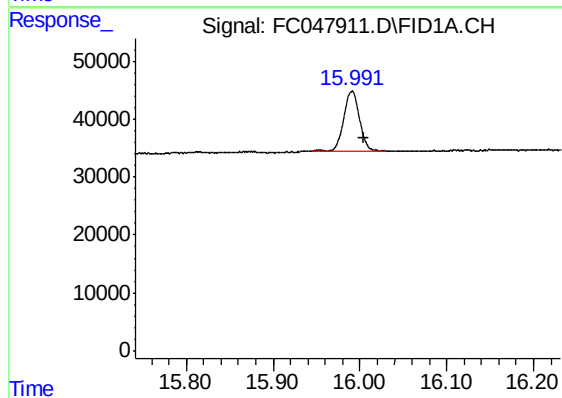

#15 n-Hexacosane (C26)


R.T.: 15.991 min
Delta R.T.: -0.013 min
Response: 128423
Conc: 1.12 ug/ml

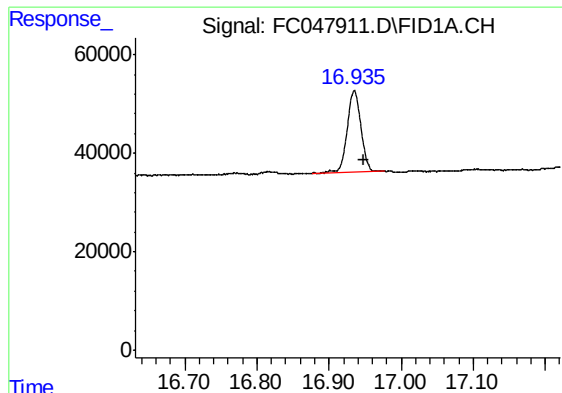

#16 n-Octacosane (C28)


R.T.: 16.935 min
Delta R.T.: -0.013 min
Response: 218715
Conc: 1.92 ug/ml

Instrument :
FID_C
ClientSampleId :
MECL2

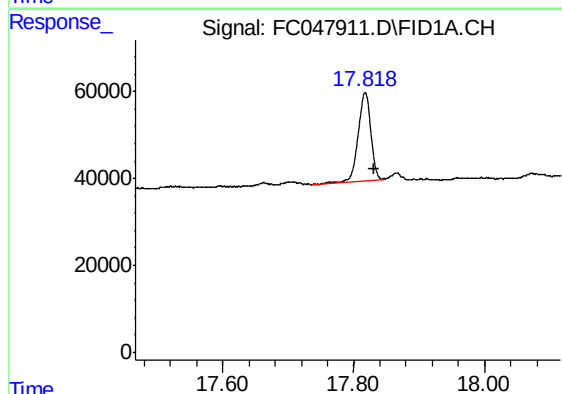


#17 n-Tricontane (C30)

R.T.: 17.818 min
Delta R.T.: -0.013 min
Response: 268369
Conc: 2.45 ug/ml

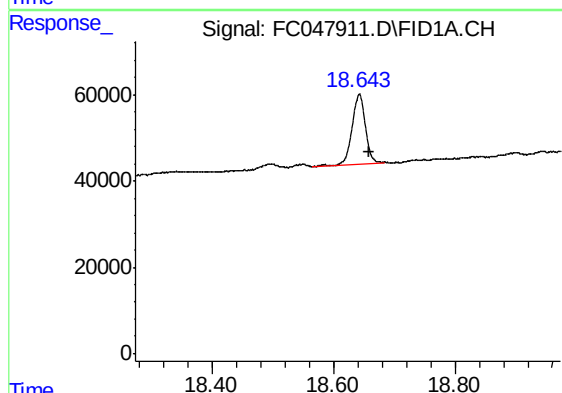


#18 n-Dotriacontane (C32)

R.T.: 18.643 min
Delta R.T.: -0.016 min
Response: 245646
Conc: 2.48 ug/ml

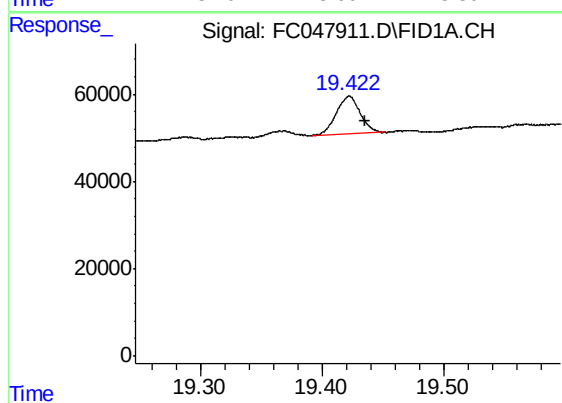

#19 n-Tetratriacontane (C34)

R.T.: 19.422 min
Delta R.T.: -0.013 min
Response: 120460
Conc: 1.32 ug/ml

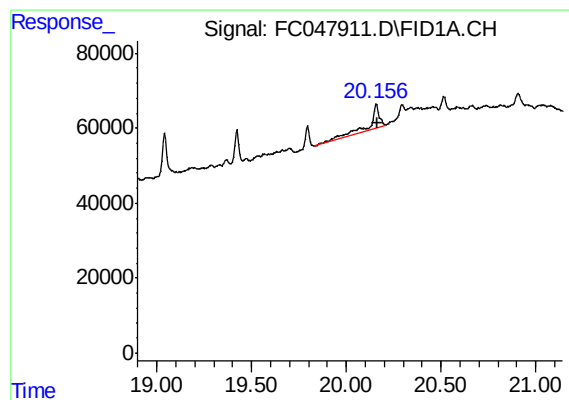

#20 n-Hexatriacontane (C36)

R.T.: 20.158 min
Delta R.T.: -0.009 min
Response: 238320
Conc: 2.78 ug/ml

Instrument :
FID_C
ClientSampleId :
MECL2