

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061820AL\
 Data File : FC047932.D
 Signal(s) : FID1A.CH
 Acq On : 19 Jun 2020 1:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Jun 19 02:21:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 060920.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 10 08:39:57 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	15.012	184017	1.601 ug/ml
15) T n-Hexacosane (C26)	15.988	127063	1.112 ug/ml
16) T n-Octacosane (C28)	16.931	227826	2.004 ug/ml
17) T n-Tricontane (C30)	17.813	284186	2.593 ug/ml
18) T n-Dotriacontane (C32)	18.639	242699	2.448 ug/ml
19) T n-Tetratriacontane (C34)	19.418	118470	1.294 ug/ml
20) T n-Hexatriacontane (C36)	20.153	154849	1.806 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061820AL\
Data File : FC047932.D
Signal(s) : FID1A.CH
Acq On : 19 Jun 2020 1:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 19 02:21:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 060920.M
Quant Title : GC Extractables
QLast Update : Wed Jun 10 08:39:57 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rx1-1ms
Signal Info : 20M x 0.18mm x 0.18um

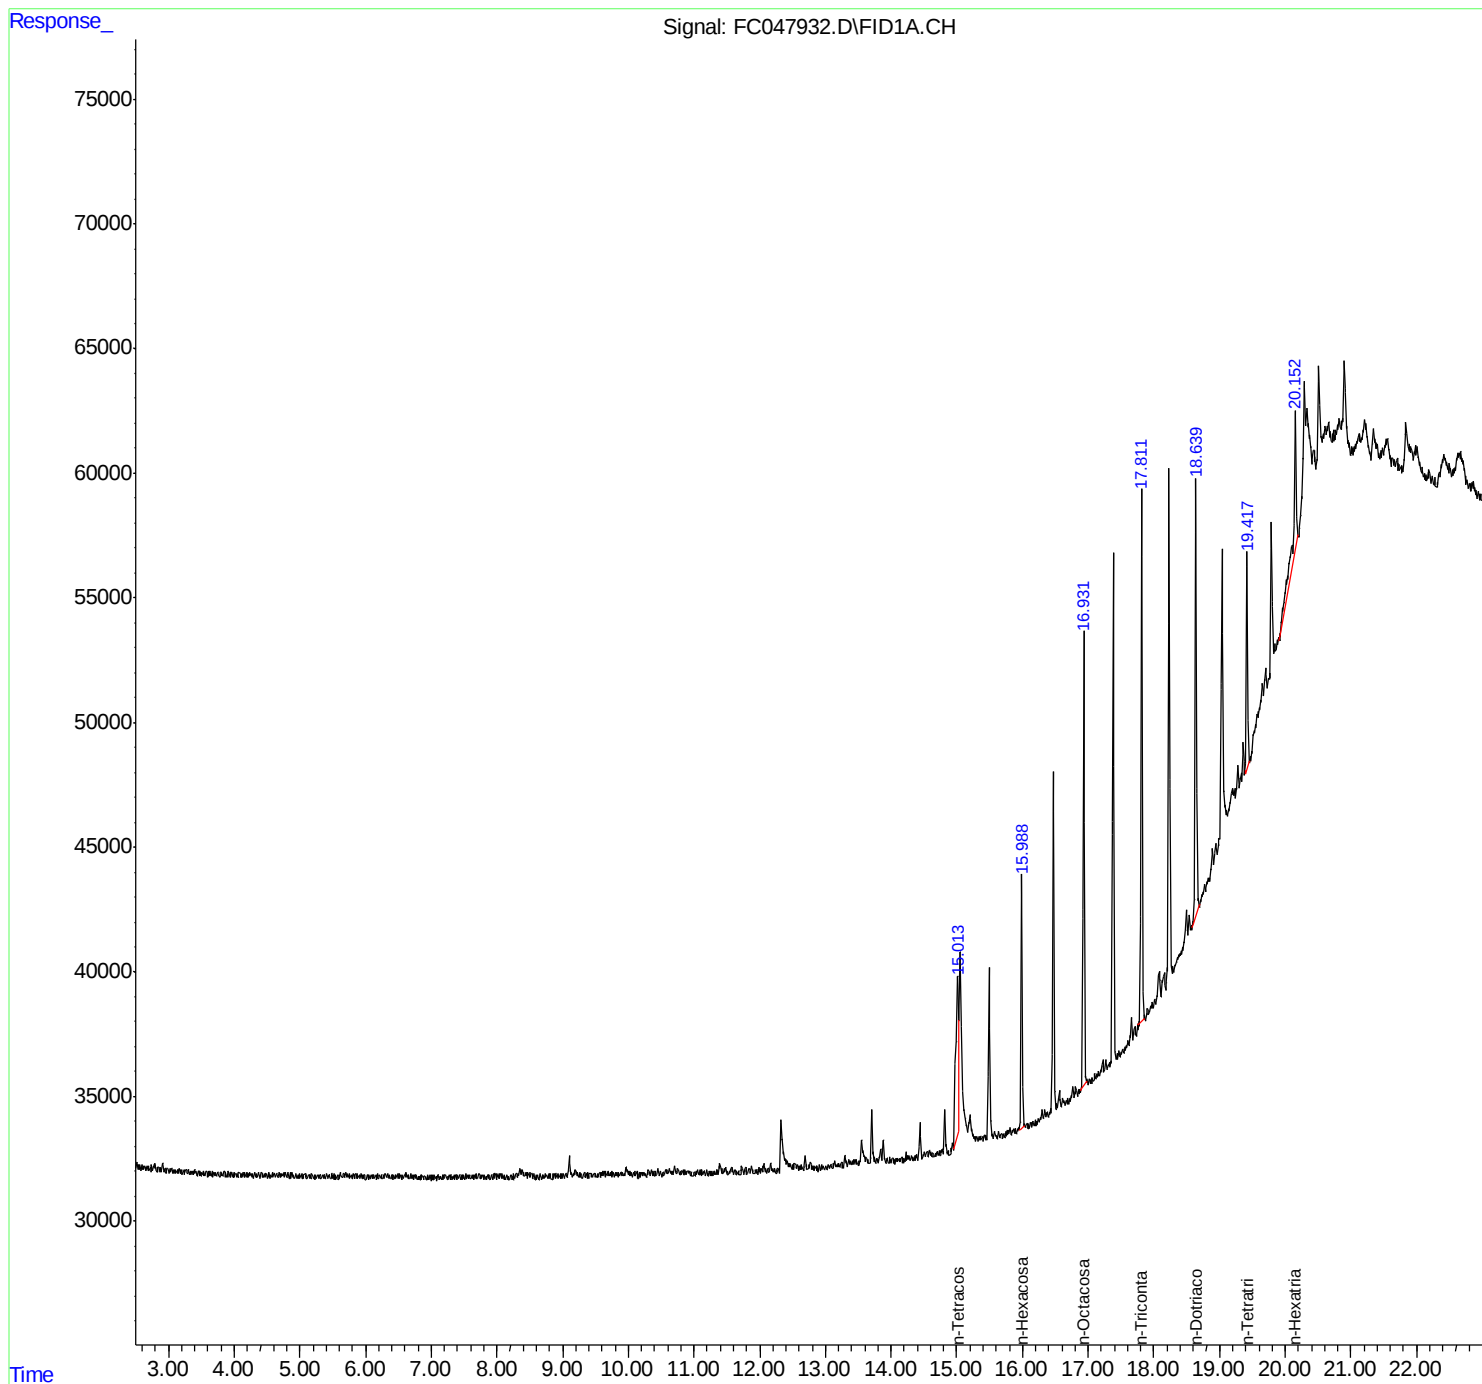


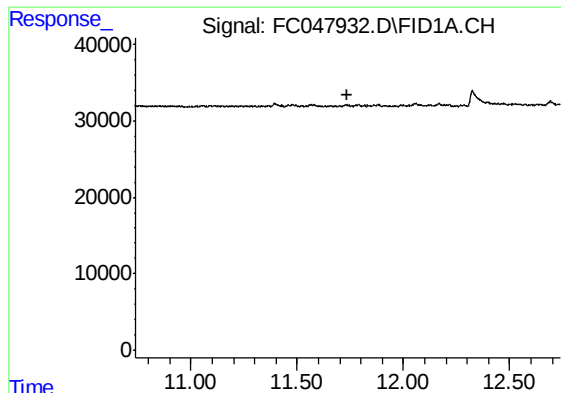

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.739 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

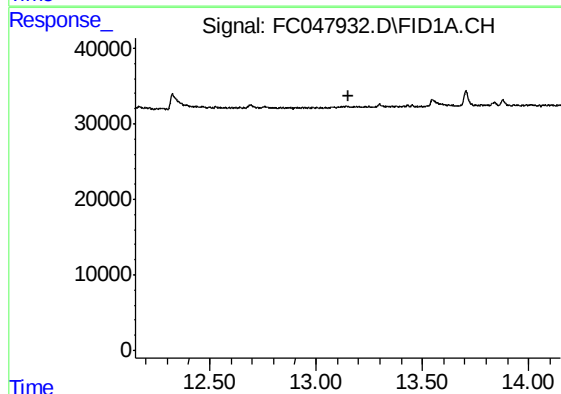


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.150 min
Response: 0
Conc: N.D.

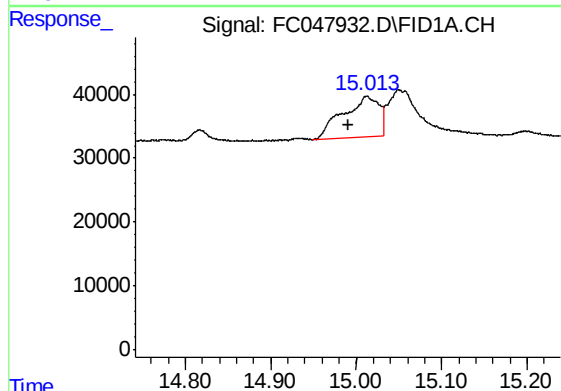


#14 n-Tetracosane (C24)

R.T.: 15.012 min
Delta R.T.: 0.022 min
Response: 184017
Conc: 1.60 ug/ml

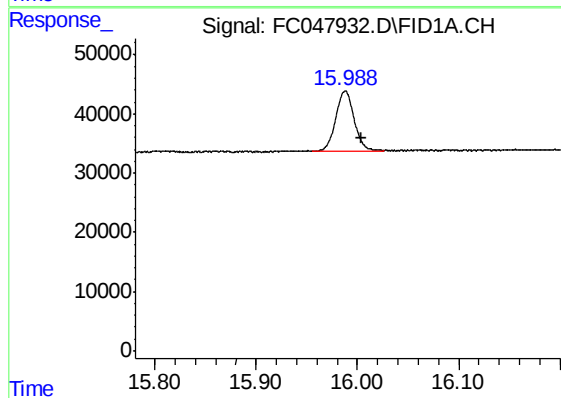

#15 n-Hexacosane (C26)


R.T.: 15.988 min
Delta R.T.: -0.016 min
Response: 127063
Conc: 1.11 ug/ml

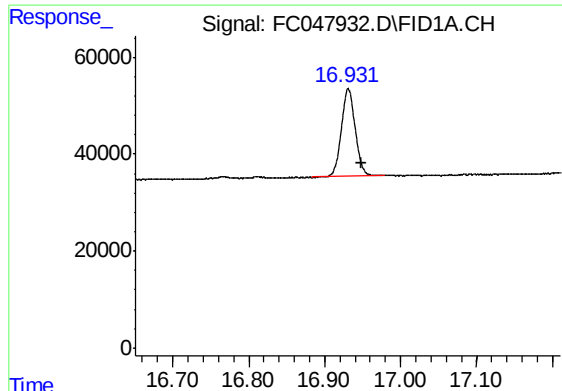

#16 n-Octacosane (C28)


R.T.: 16.931 min
Delta R.T.: -0.017 min
Response: 227826
Conc: 2.00 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK

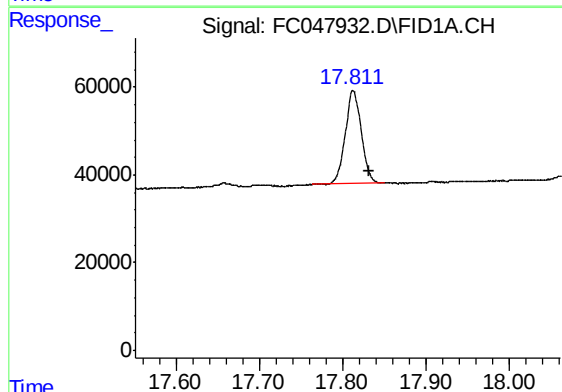


#17 n-Tricontane (C30)

R.T.: 17.813 min
Delta R.T.: -0.018 min
Response: 284186
Conc: 2.59 ug/ml

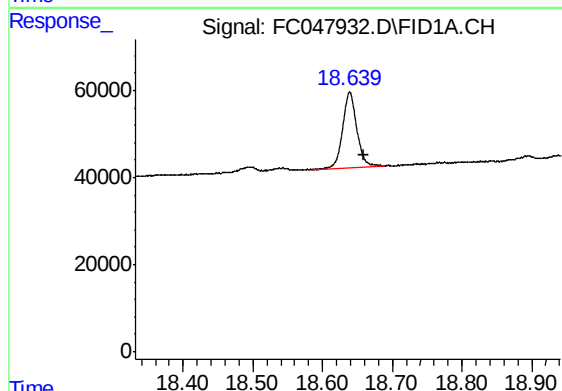


#18 n-Dotriacontane (C32)

R.T.: 18.639 min
Delta R.T.: -0.020 min
Response: 242699
Conc: 2.45 ug/ml

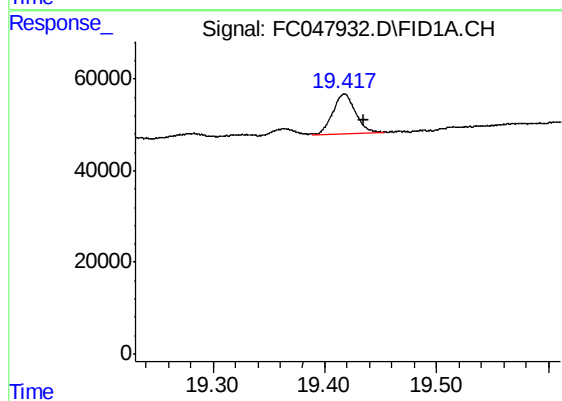

#19 n-Tetratriacontane (C34)

R.T.: 19.418 min
Delta R.T.: -0.018 min
Response: 118470
Conc: 1.29 ug/ml

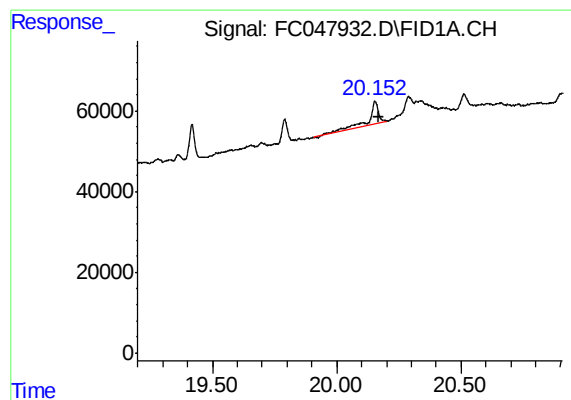

#20 n-Hexatriacontane (C36)

R.T.: 20.153 min
Delta R.T.: -0.014 min
Response: 154849
Conc: 1.81 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK