

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061824AL\
 Data File : FC066620.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jun 2024 09:44
 Operator : YP/AJ
 Sample : P2887-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 03:38:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.543	5102256	29.580 ug/ml
Spiked Amount 50.000		Recovery =	59.16%
12) S 1-chlorooctadecane (S...	12.982	4280996	31.026 ug/ml
Spiked Amount 50.000		Recovery =	62.05%
Target Compounds			
14) T n-Tetracosane (C24)	14.835	59834	0.377 ug/ml
15) T n-Hexacosane (C26)	15.857	79833	0.523 ug/ml
16) T n-Octacosane (C28)	16.807	81172	0.563 ug/ml
17) T n-Tricontane (C30)	17.694	110099	0.788 ug/ml
18) T n-Dotriacontane (C32)	18.526	109595	0.830 ug/ml
19) T n-Tetratriacontane (C34)	19.312	69189	0.559 ug/ml
20) T n-Hexatriacontane (C36)	20.055	47971	0.398 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC061824AL\
Data File : FC066620.D
Signal(s) : FID1A.ch
Acq On : 18 Jun 2024 09:44
Operator : YP/AJ
Sample : P2887-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 03:38:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

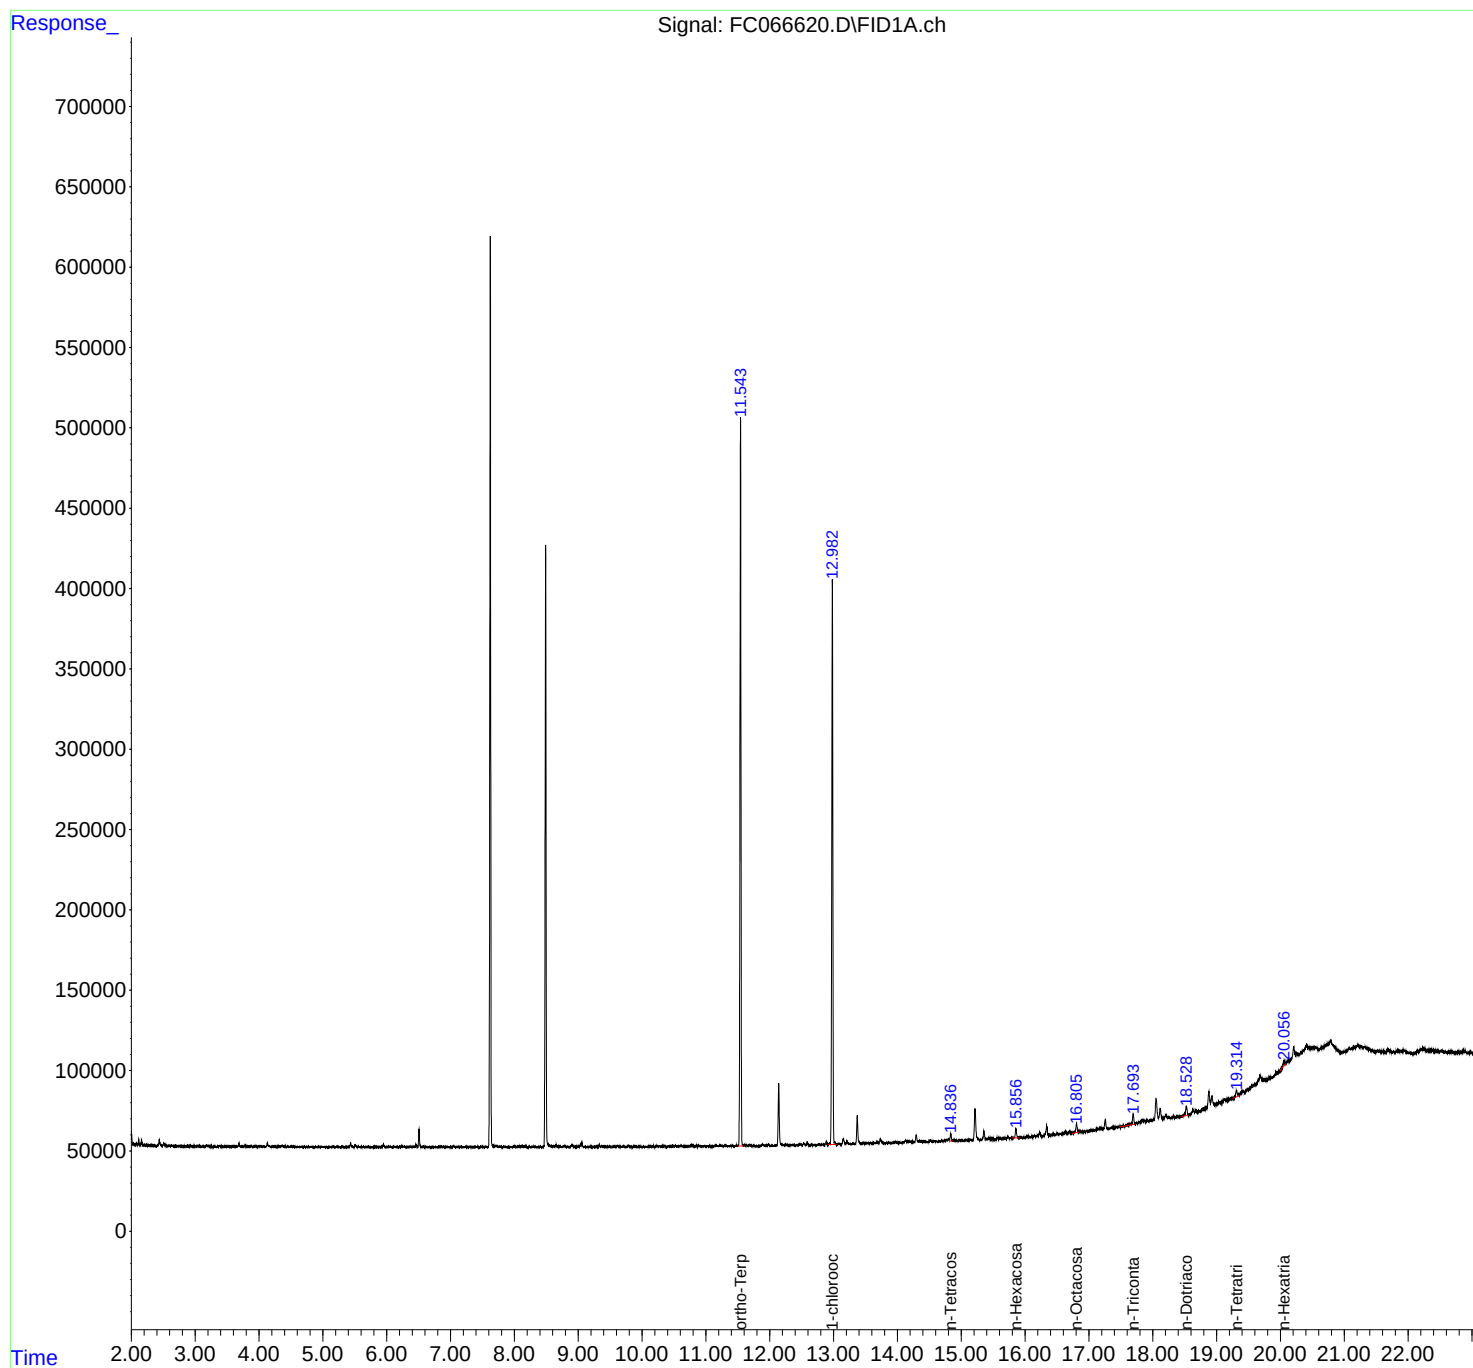


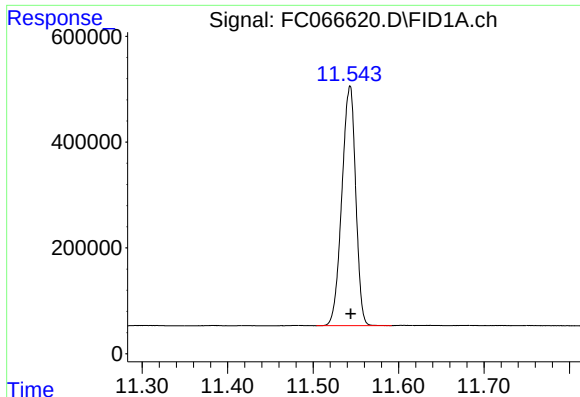

#9 ortho-Terphenyl (SURR)


R.T.: 11.543 min
Delta R.T.: -0.001 min
Response: 5102256
Conc: 29.58 ug/ml

Instrument :
FID_C
ClientSampleId :

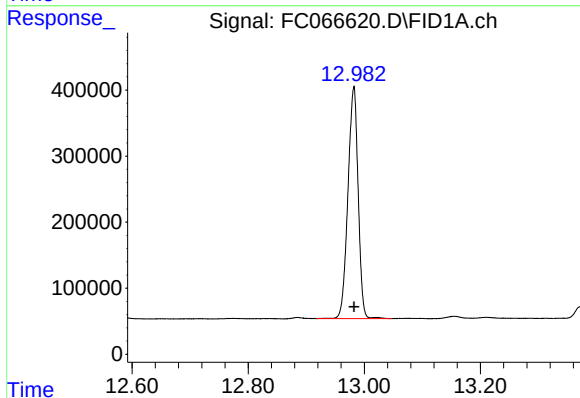


#12 1-chlorooctadecane (SURR)

R.T.: 12.982 min
Delta R.T.: 0.000 min
Response: 4280996
Conc: 31.03 ug/ml

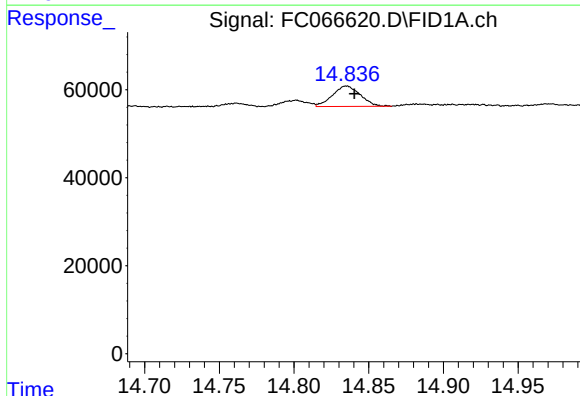


#14 n-Tetracosane (C24)

R.T.: 14.835 min
Delta R.T.: -0.005 min
Response: 59834
Conc: 0.38 ug/ml

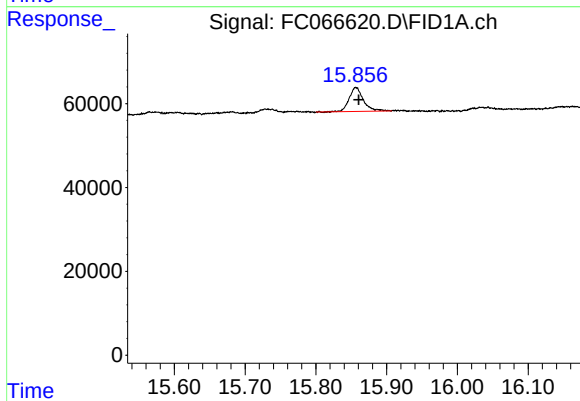

#15 n-Hexacosane (C26)


R.T.: 15.857 min
Delta R.T.: -0.004 min
Response: 79833
Conc: 0.52 ug/ml

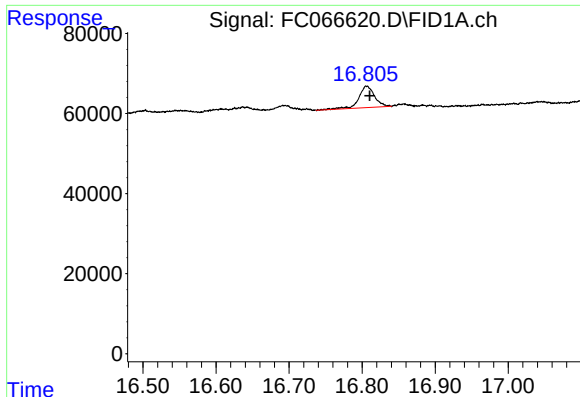

#16 n-Octacosane (C28)


R.T.: 16.807 min
Delta R.T.: -0.004 min
Response: 81172
Conc: 0.56 ug/ml

Instrument :
FID_C
ClientSampleId :

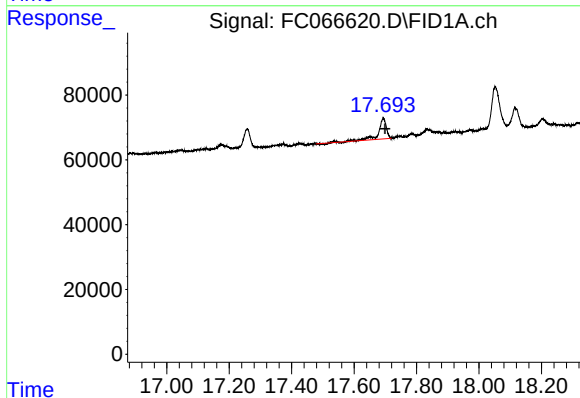


#17 n-Tricontane (C30)

R.T.: 17.694 min
Delta R.T.: -0.006 min
Response: 110099
Conc: 0.79 ug/ml

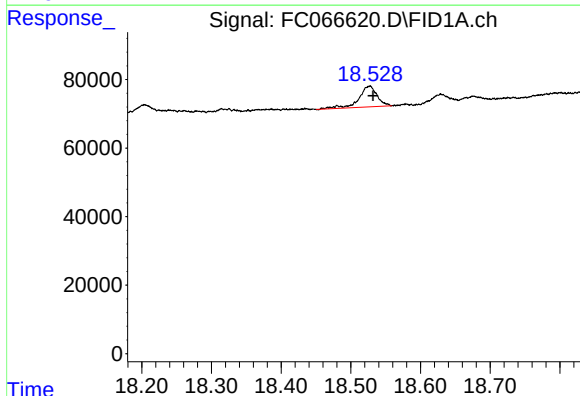


#18 n-Dotriacontane (C32)

R.T.: 18.526 min
Delta R.T.: -0.005 min
Response: 109595
Conc: 0.83 ug/ml

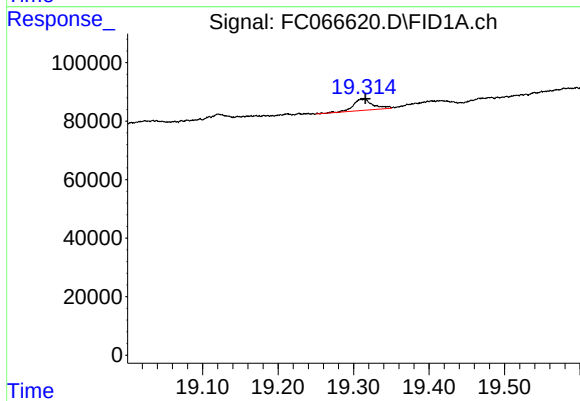

#19 n-Tetratriacontane (C34)

R.T.: 19.312 min
Delta R.T.: -0.003 min
Response: 69189
Conc: 0.56 ug/ml

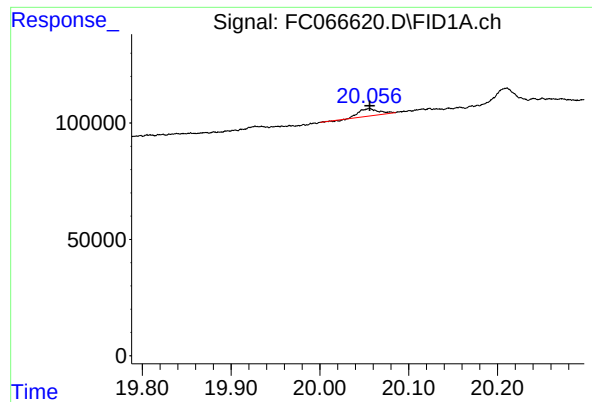

#20 n-Hexatriacontane (C36)

R.T.: 20.055 min
Delta R.T.: 0.000 min
Response: 47971
Conc: 0.40 ug/ml

Instrument :

FID_C

ClientSampleId :